

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018248.D
 Acq On : 18 Nov 2023 07:36
 Operator : MA/JU
 Sample : PB157221BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	17	rVB	29490	32935	1.40%	0.148%
2	3.593	83	86	97	rBV	243980	408075	17.30%	1.837%
3	4.540	245	247	250	rVB3	2460	2744	0.12%	0.012%
4	6.040	497	502	505	rBV7	1727	2738	0.12%	0.012%
5	6.946	651	656	677	rBV	318851	606503	25.72%	2.730%
6	7.128	681	687	698	rBV	268446	423031	17.94%	1.904%
7	7.299	710	716	734	rBV	358915	628461	26.65%	2.829%
8	7.775	790	797	818	rBV	220608	401429	17.02%	1.807%
9	8.246	872	877	881	rBV8	2321	3892	0.17%	0.018%
10	8.505	915	921	940	rBV	384603	736859	31.24%	3.317%
11	8.987	996	1003	1019	rBV	316901	604884	25.65%	2.723%
12	9.116	1023	1025	1030	rVB6	1558	2621	0.11%	0.012%
13	9.699	1115	1124	1144	rBV	275976	566304	24.01%	2.549%
14	10.228	1207	1214	1240	rBV	330769	773787	32.81%	3.483%
15	10.593	1269	1276	1290	rBV	333323	553421	23.47%	2.491%
16	10.781	1301	1308	1328	rBV	295458	710335	30.12%	3.197%
17	11.628	1446	1452	1453	rBV6	2567	2839	0.12%	0.013%
18	11.993	1508	1514	1516	rBV7	1763	3083	0.13%	0.014%
19	12.252	1553	1558	1560	rBV4	3959	5669	0.24%	0.026%
20	13.299	1730	1736	1743	rBV5	7291	12323	0.52%	0.055%
21	13.657	1795	1797	1802	rVB6	1653	2450	0.10%	0.011%
22	13.881	1829	1835	1847	rBV	870357	1239623	52.56%	5.580%
23	14.157	1875	1882	1900	rBV	900772	1308051	55.46%	5.888%
24	14.457	1925	1933	1945	rBV	480911	720862	30.56%	3.245%
25	14.734	1975	1980	2001	rBV	129483	462424	19.61%	2.082%
26	15.040	2029	2032	2035	rBV5	1620	2395	0.10%	0.011%
27	15.463	2097	2104	2118	rBV	1182099	1736421	73.63%	7.816%
28	15.628	2124	2132	2143	rBV	319310	596664	25.30%	2.686%
29	16.045	2199	2203	2208	rBV8	2357	3321	0.14%	0.015%
30	16.251	2235	2238	2243	rVB7	1894	3518	0.15%	0.016%
31	17.239	2399	2406	2416	rBV	668561	945734	40.10%	4.257%
32	17.339	2417	2423	2448	rVB	1261701	1952864	82.80%	8.791%
33	18.104	2549	2553	2555	rBV4	3731	5137	0.22%	0.023%
34	19.175	2730	2735	2741	rBV5	16917	24312	1.03%	0.109%
35	19.251	2744	2748	2757	rVB	14280	24661	1.05%	0.111%
36	19.598	2801	2807	2821	rBV	1753062	2298050	97.44%	10.344%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018248.D
Acq On : 18 Nov 2023 07:36
Operator : MA/JU
Sample : PB157221BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	21.375	3105	3109	3119	rBV	686467	999089	42.36%	4.497%
38	23.686	3494	3502	3516	rVB2	1140070	2358463	100.00%	10.616%
39	23.851	3523	3530	3545	rVB	465611	1049546	44.50%	4.724%




Sum of corrected areas: 22215518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018248.D
Acq On : 18 Nov 2023 07:36
Operator : MA/JU
Sample : PB157221BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

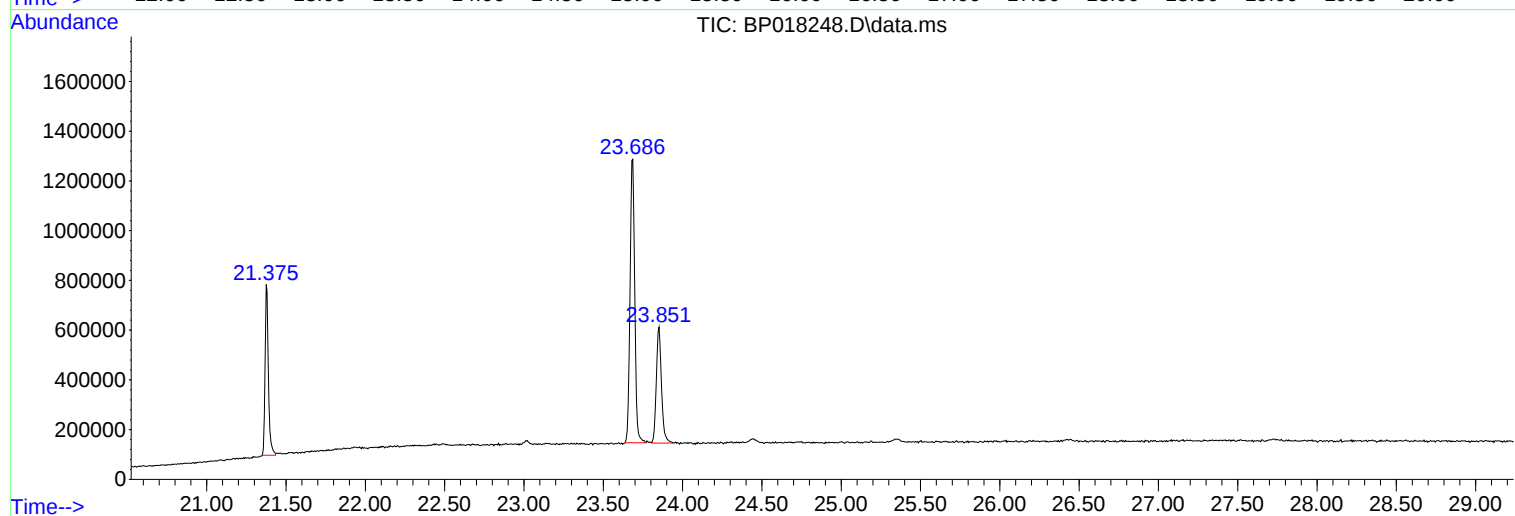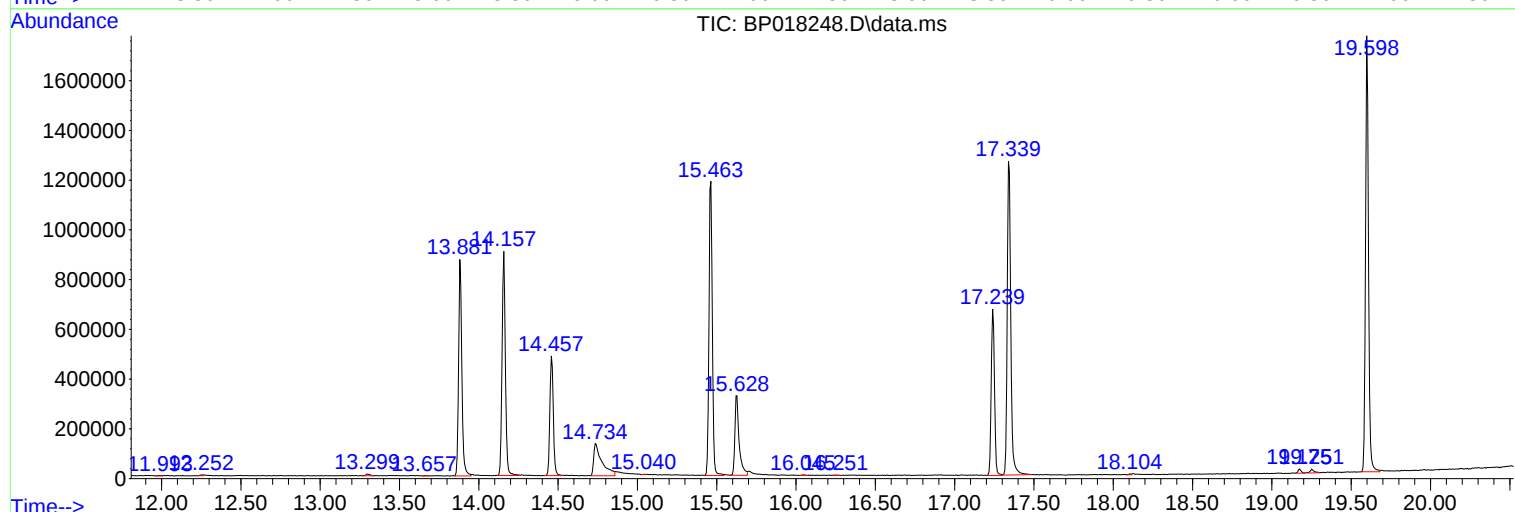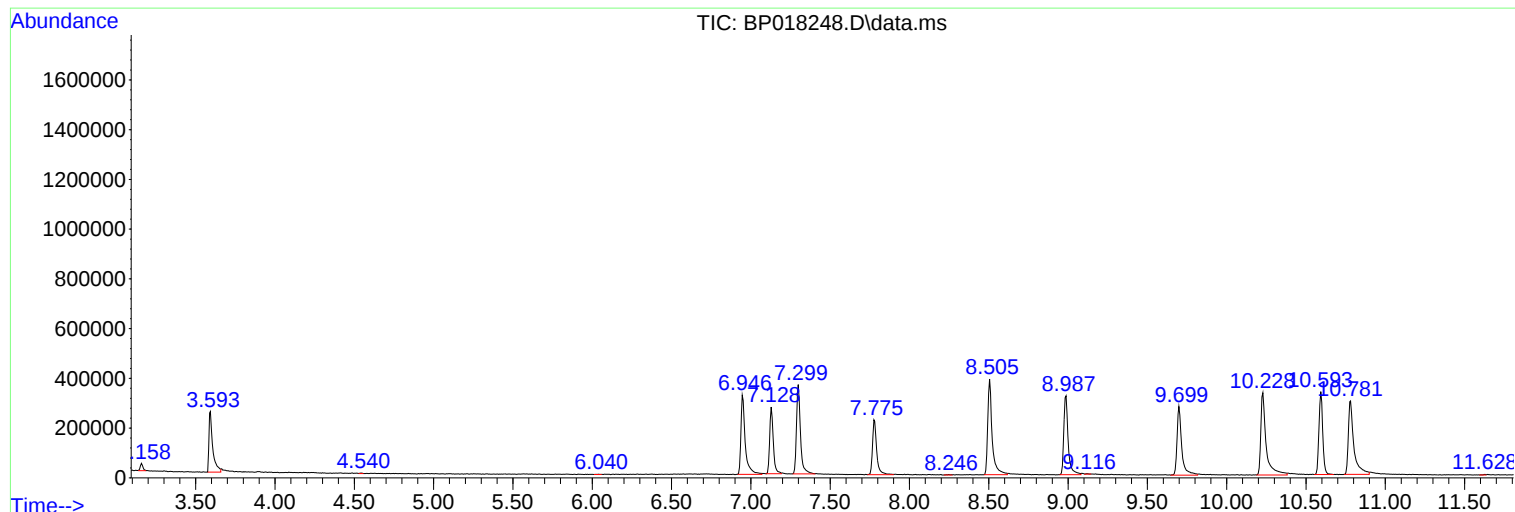

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018248.D
Acq On : 18 Nov 2023 07:36
Operator : MA/JU
Sample : PB157221BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018248.D
Acq On : 18 Nov 2023 07:36
Operator : MA/JU
Sample : PB157221BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc