

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018262.D
 Acq On : 18 Nov 2023 15:30
 Operator : MA/JU
 Sample : PB157223BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	8	12	18	rBB	28919	37530	1.66%	0.160%
2	3.522	72	74	79	rBV5	2836	3165	0.14%	0.014%
3	3.587	82	85	98	rBV	278928	454184	20.09%	1.941%
4	3.899	134	138	141	rBV4	5075	8015	0.35%	0.034%
5	4.464	232	234	238	rBV5	2085	2807	0.12%	0.012%
6	6.340	550	553	554	rBV3	2153	2361	0.10%	0.010%
7	6.946	650	656	674	rBV	374029	696130	30.79%	2.976%
8	7.128	681	687	701	rBV	308449	496959	21.98%	2.124%
9	7.299	709	716	734	rBV	391347	687479	30.41%	2.939%
10	7.775	791	797	820	rBV	308774	542808	24.01%	2.320%
11	8.505	914	921	945	rBV	426692	849605	37.58%	3.632%
12	8.981	994	1002	1016	rBV	370077	692563	30.63%	2.960%
13	9.163	1031	1033	1037	rVB5	2982	2644	0.12%	0.011%
14	9.699	1116	1124	1142	rBV	317362	625666	27.67%	2.674%
15	10.222	1207	1213	1230	rBV	374216	815460	36.07%	3.486%
16	10.593	1268	1276	1290	rBV	423745	706009	31.23%	3.018%
17	10.775	1298	1307	1329	rBV	328648	782057	34.59%	3.343%
18	11.099	1360	1362	1366	rVB5	2181	2530	0.11%	0.011%
19	11.716	1464	1467	1472	rVB7	2086	3355	0.15%	0.014%
20	12.246	1553	1557	1558	rBV3	3050	3156	0.14%	0.013%
21	12.840	1654	1658	1663	rVB8	1307	2848	0.13%	0.012%
22	13.293	1728	1735	1744	rVB8	7180	14959	0.66%	0.064%
23	13.681	1796	1801	1803	rBV6	2058	2391	0.11%	0.010%
24	13.881	1828	1835	1850	rBV	842231	1241417	54.91%	5.307%
25	14.157	1875	1882	1893	rVV	858729	1326280	58.66%	5.669%
26	14.457	1926	1933	1943	rBV	575232	843736	37.32%	3.607%
27	14.734	1974	1980	2001	rBV	133445	467083	20.66%	1.997%
28	15.463	2097	2104	2120	rBV	1194306	1694804	74.97%	7.245%
29	15.628	2126	2132	2143	rBV	321104	589580	26.08%	2.520%
30	16.034	2199	2201	2206	rVB6	1918	2884	0.13%	0.012%
31	17.239	2399	2406	2417	rBV	736746	1043243	46.15%	4.459%
32	17.345	2417	2424	2449	rVB	1229946	1882947	83.29%	8.049%
33	17.710	2481	2486	2487	rBV5	1618	2602	0.12%	0.011%
34	17.945	2523	2526	2531	rBV6	1568	2863	0.13%	0.012%
35	18.504	2617	2621	2623	rBV5	2098	2819	0.12%	0.012%
36	18.816	2671	2674	2676	rBV4	1980	2576	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018262.D
Acq On : 18 Nov 2023 15:30
Operator : MA/JU
Sample : PB157223BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Title : SVOA CALIBRATION

37	19.051	2712	2714	2718	rBV5	2180	3102	0.14%	0.013%
38	19.175	2731	2735	2740	rBV4	15401	20942	0.93%	0.090%
39	19.251	2745	2748	2759	rVV3	10944	22142	0.98%	0.095%
40	19.598	2802	2807	2819	rBV	1602634	2241953	99.17%	9.583%
41	21.380	3105	3110	3122	rBV	802955	1159912	51.31%	4.958%
42	23.692	3495	3503	3514	rBV2	1179441	2260780	100.00%	9.664%
43	23.857	3524	3531	3544	rVB	522984	1147556	50.76%	4.905%




Sum of corrected areas: 23393902

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018262.D
Acq On : 18 Nov 2023 15:30
Operator : MA/JU
Sample : PB157223BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

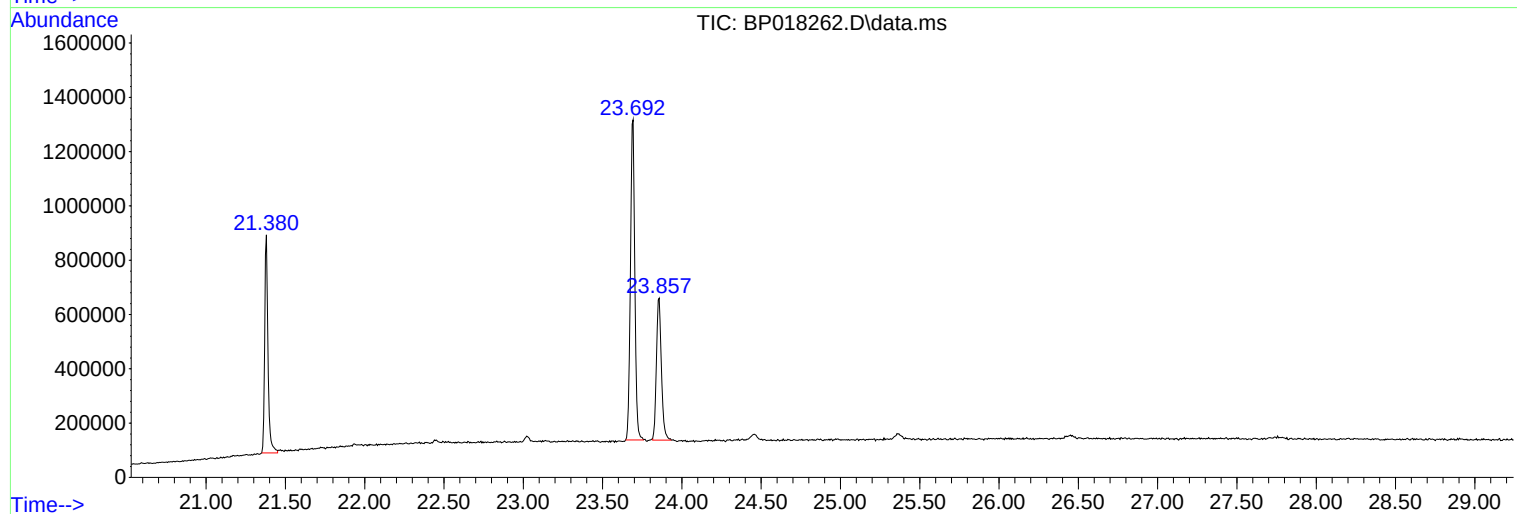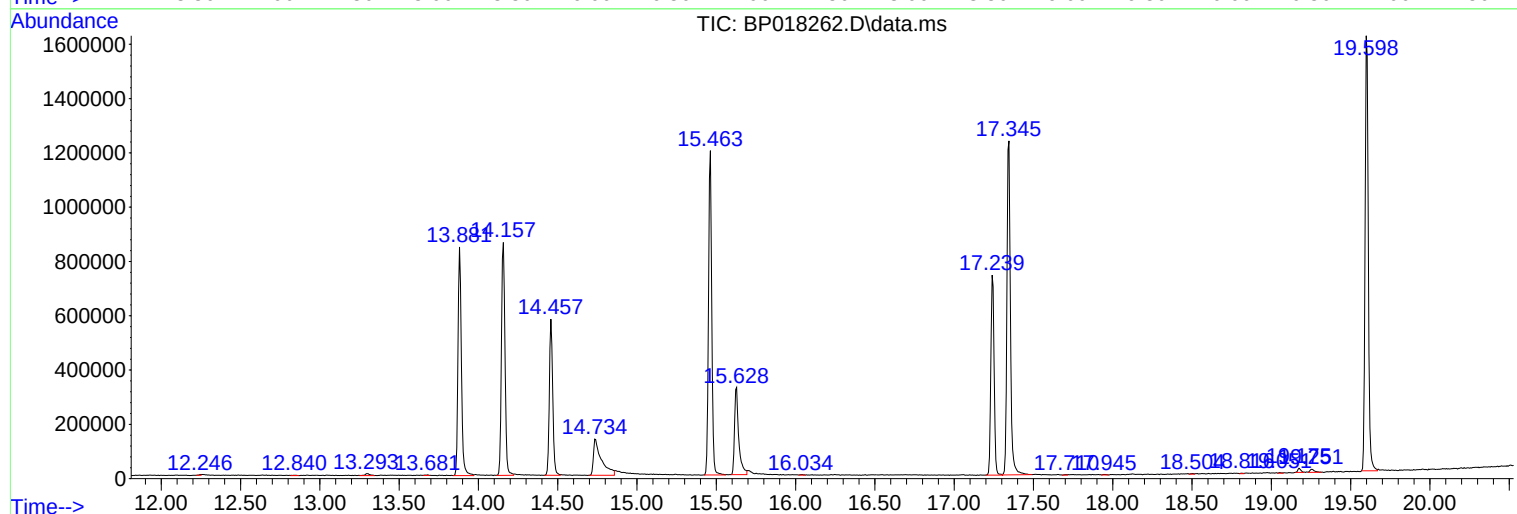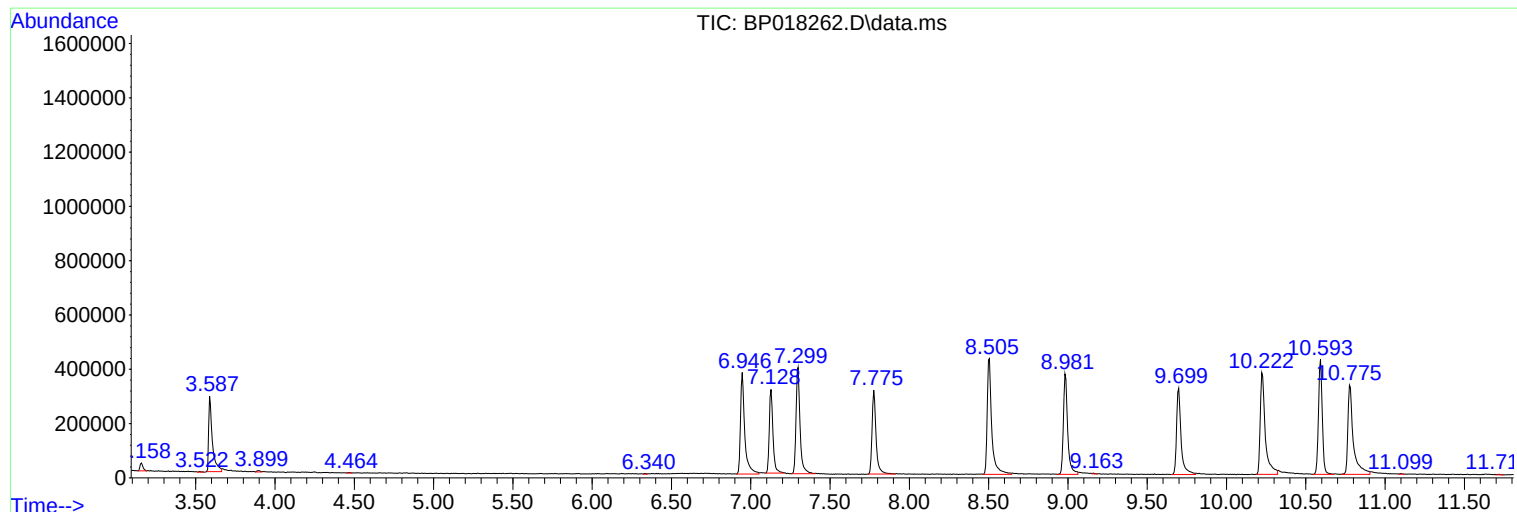

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018262.D
Acq On : 18 Nov 2023 15:30
Operator : MA/JU
Sample : PB157223BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018262.D
Acq On : 18 Nov 2023 15:30
Operator : MA/JU
Sample : PB157223BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc