

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018264.D
 Acq On : 18 Nov 2023 16:38
 Operator : MA/JU
 Sample : PB157225BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	9	12	20	rVB2	25948	34453	1.72%	0.173%
2	3.587	82	85	103	rBV	222138	401984	20.11%	2.018%
3	5.564	416	421	425	rVB8	1741	2693	0.13%	0.014%
4	5.752	450	453	456	rBV5	1635	2093	0.10%	0.011%
5	5.999	494	495	501	rVB6	1928	2281	0.11%	0.011%
6	6.734	619	620	625	rVB5	2087	2140	0.11%	0.011%
7	6.946	649	656	681	rBV	278804	541422	27.08%	2.718%
8	7.128	681	687	704	rVV	238283	390218	19.52%	1.959%
9	7.299	710	716	731	rBV	319351	566340	28.33%	2.843%
10	7.434	738	739	745	rVB6	2379	2716	0.14%	0.014%
11	7.510	748	752	754	rBV5	1607	2198	0.11%	0.011%
12	7.775	790	797	816	rBV	236943	432491	21.63%	2.171%
13	8.452	908	912	914	rBV5	1671	2507	0.13%	0.013%
14	8.505	914	921	946	rVV	320313	656814	32.86%	3.298%
15	8.716	952	957	960	rVB6	1644	3079	0.15%	0.015%
16	8.981	993	1002	1024	rBV	267076	540633	27.04%	2.714%
17	9.134	1027	1028	1031	rVV3	2809	2769	0.14%	0.014%
18	9.699	1117	1124	1147	rBV	235307	489276	24.48%	2.457%
19	9.875	1151	1154	1156	rBV4	1869	2296	0.11%	0.012%
20	10.228	1207	1214	1242	rBV	285949	678941	33.96%	3.409%
21	10.593	1269	1276	1290	rVB	344391	583225	29.17%	2.928%
22	10.781	1300	1308	1329	rBV	252513	634692	31.75%	3.187%
23	11.863	1489	1492	1496	rVB6	1592	2171	0.11%	0.011%
24	12.251	1552	1558	1559	rBV6	3955	4398	0.22%	0.022%
25	12.610	1616	1619	1621	rBV3	1926	2228	0.11%	0.011%
26	13.298	1731	1736	1741	rBV7	4964	8431	0.42%	0.042%
27	13.457	1758	1763	1765	rVB5	2111	3270	0.16%	0.016%
28	13.663	1797	1798	1802	rVB4	2947	3161	0.16%	0.016%
29	13.740	1809	1811	1815	rBV4	1568	2274	0.11%	0.011%
30	13.881	1829	1835	1849	rBV	721672	1059282	52.99%	5.318%
31	14.157	1875	1882	1896	rBV	762333	1152801	57.67%	5.788%
32	14.304	1905	1907	1912	rVB6	2235	2838	0.14%	0.014%
33	14.457	1926	1933	1943	rBV	499138	735476	36.79%	3.693%
34	14.745	1973	1982	1998	rBV3	101186	367421	18.38%	1.845%
35	15.463	2096	2104	2115	rBV	987927	1456897	72.88%	7.315%
36	15.545	2115	2118	2120	rVB4	2485	2841	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
 Data File : BP018264.D
 Acq On : 18 Nov 2023 16:38
 Operator : MA/JU
 Sample : PB157225BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
 Title : SVOA CALIBRATION

37	15.628	2126	2132	2143	rBV	267906	483809	24.20%	2.429%
38	16.263	2238	2240	2244	rVB5	1521	2076	0.10%	0.010%
39	16.551	2287	2289	2291	rBV3	1922	2382	0.12%	0.012%
40	16.916	2347	2351	2353	rBV5	2180	2780	0.14%	0.014%
41	17.039	2370	2372	2376	rBV5	1522	2115	0.11%	0.011%
42	17.239	2400	2406	2414	rBV	655369	907160	45.38%	4.555%
43	17.339	2417	2423	2437	rBV2	1021695	1604464	80.26%	8.056%
44	17.581	2461	2464	2466	rVB4	2191	2384	0.12%	0.012%
45	17.616	2466	2470	2471	rBV4	1896	2257	0.11%	0.011%
46	17.980	2530	2532	2537	rBV6	995	2049	0.10%	0.010%
47	18.128	2551	2557	2559	rBV7	3416	6880	0.34%	0.035%
48	18.922	2691	2692	2695	rBV3	2442	2202	0.11%	0.011%
49	19.175	2731	2735	2741	rBV3	14791	20074	1.00%	0.101%
50	19.257	2744	2749	2752	rBV	10562	16033	0.80%	0.080%
51	19.598	2802	2807	2821	rBV	1437015	1977749	98.93%	9.930%
52	21.380	3105	3110	3122	rBV	715599	1041922	52.12%	5.231%
53	23.686	3495	3502	3513	rBV2	1001569	1999080	100.00%	10.037%
54	23.857	3524	3531	3547	rVB	473708	1063216	53.19%	5.338%




Sum of corrected areas: 19917382

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018264.D
Acq On : 18 Nov 2023 16:38
Operator : MA/JU
Sample : PB157225BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

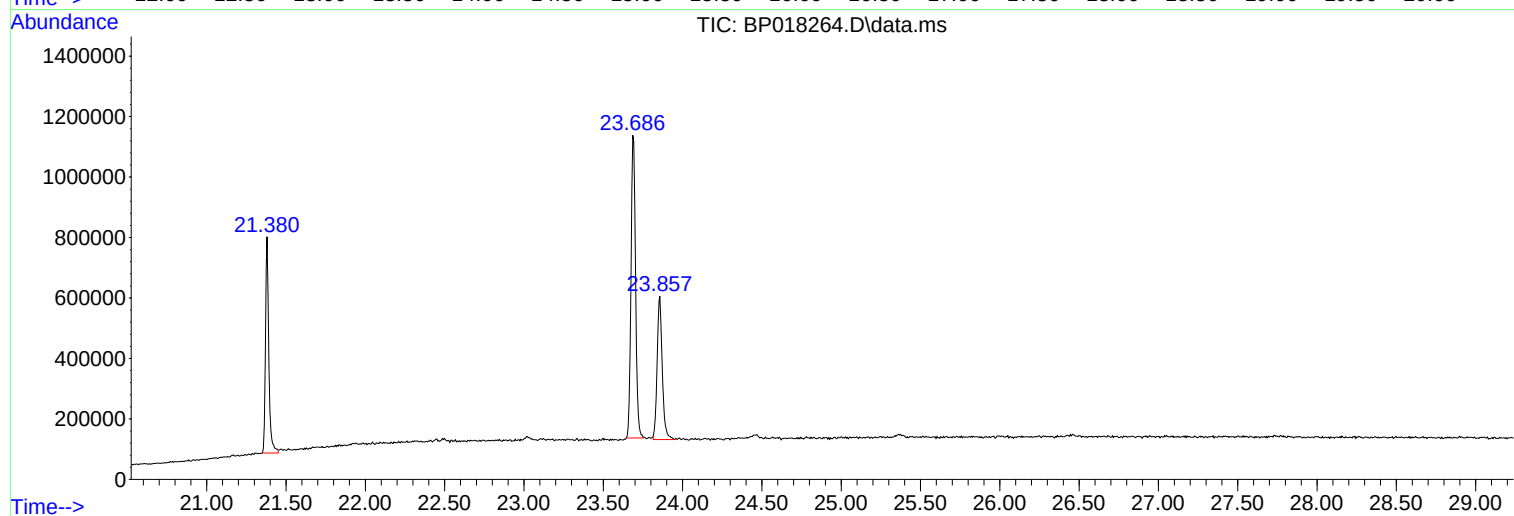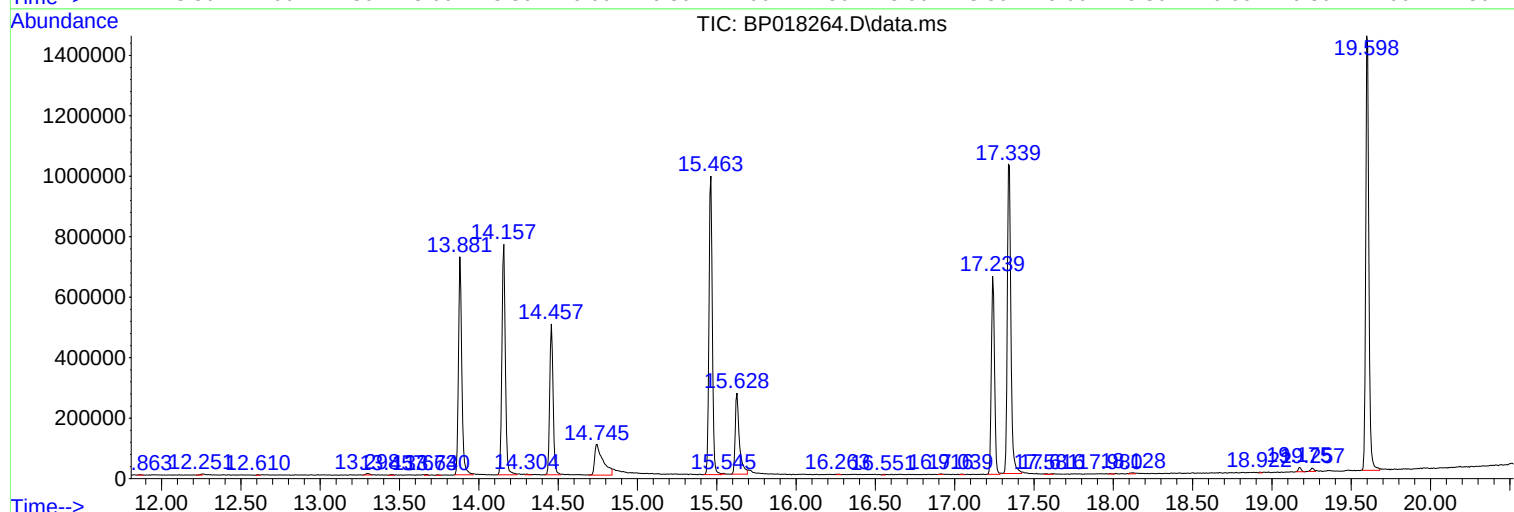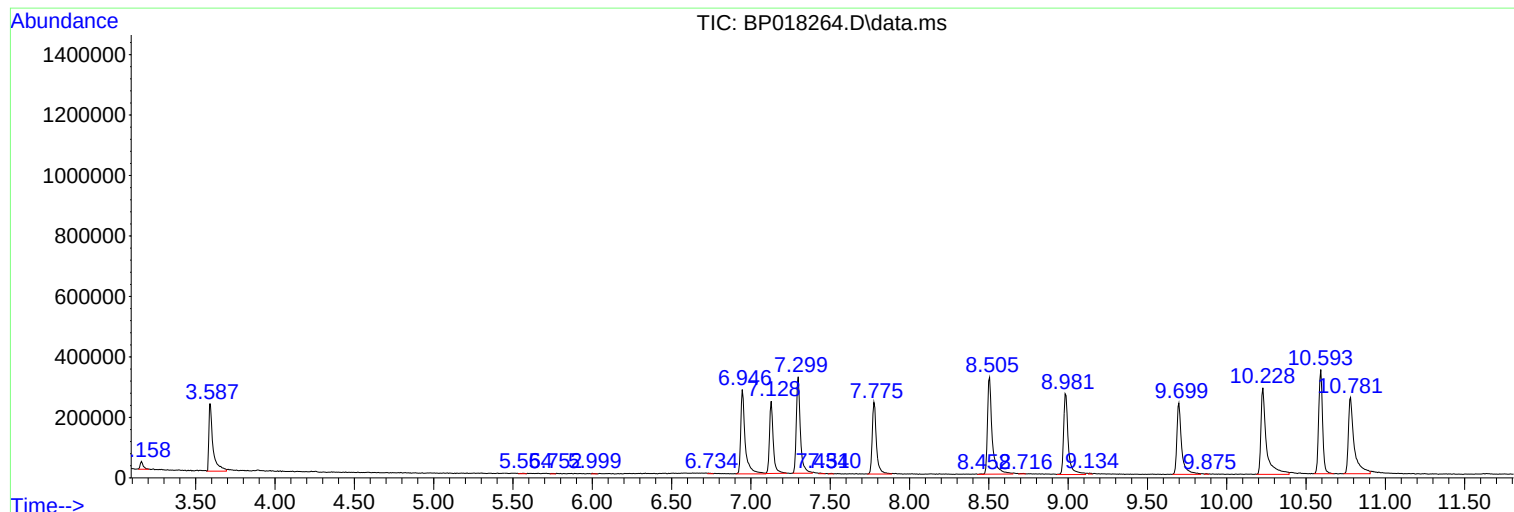

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018264.D
Acq On : 18 Nov 2023 16:38
Operator : MA/JU
Sample : PB157225BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111723\
Data File : BP018264.D
Acq On : 18 Nov 2023 16:38
Operator : MA/JU
Sample : PB157225BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK225

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP111023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------