


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP111819\
 Data File : BP001063.D
 Acq On : 18 Nov 2019 16:01
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 06 17:07:13 2019

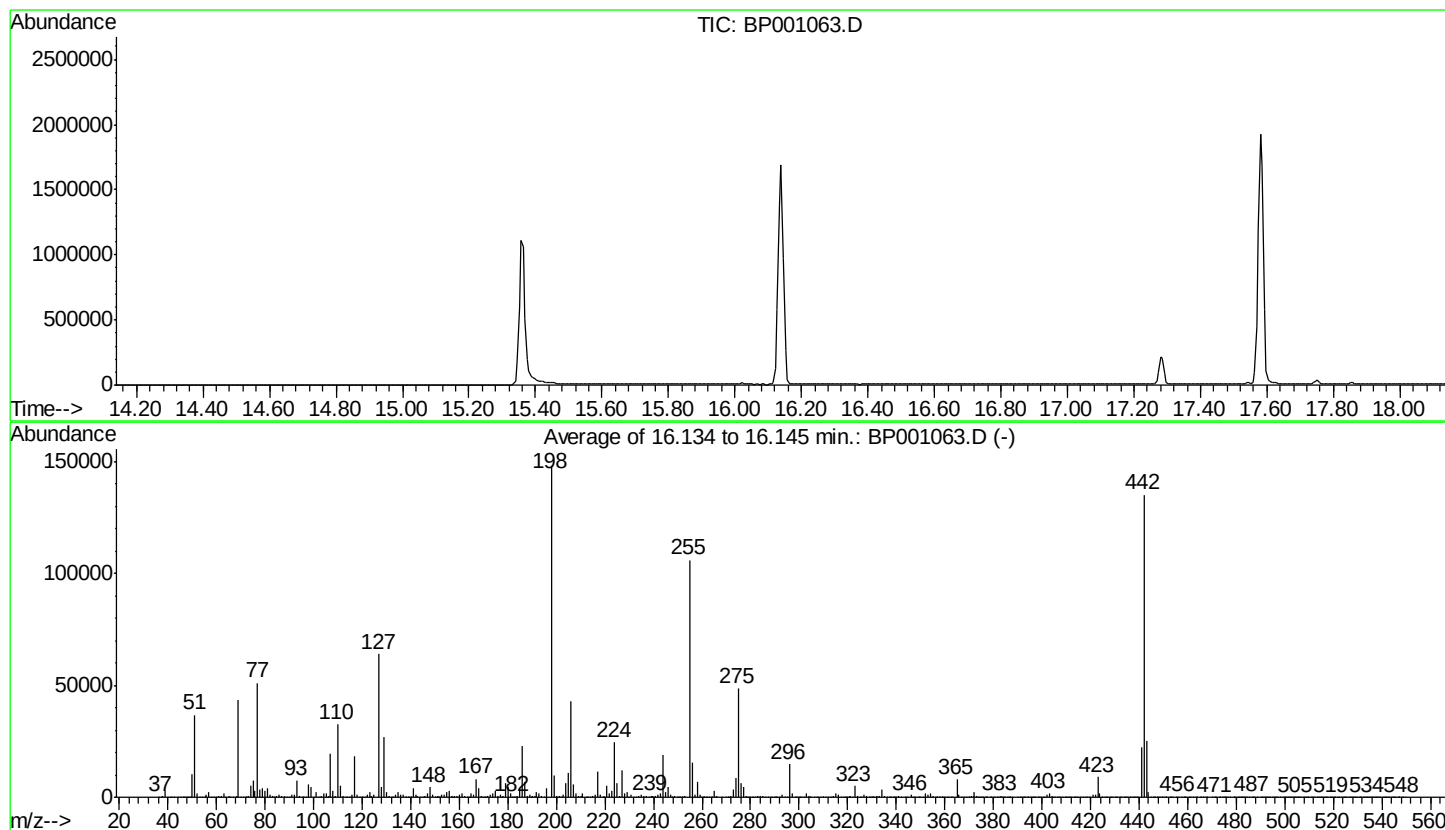

AutoFind: Scans 2388, 2389, 2390; Background Corrected with Scan 2380

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.7	36668	PASS
68	69	0.00	2	1.0	439	PASS
69	198	0.00	100	29.5	43720	PASS
70	69	0.00	2	0.5	229	PASS
127	198	10	80	43.1	63889	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148250	PASS
199	198	5	9	6.4	9468	PASS
275	198	10	60	32.7	48520	PASS
365	198	1	100	5.3	7838	PASS
441	198	0.01	100	15.3	22618	PASS
442	198	50	100	91.2	135212	PASS
443	442	15	24	18.6	25170	PASS