
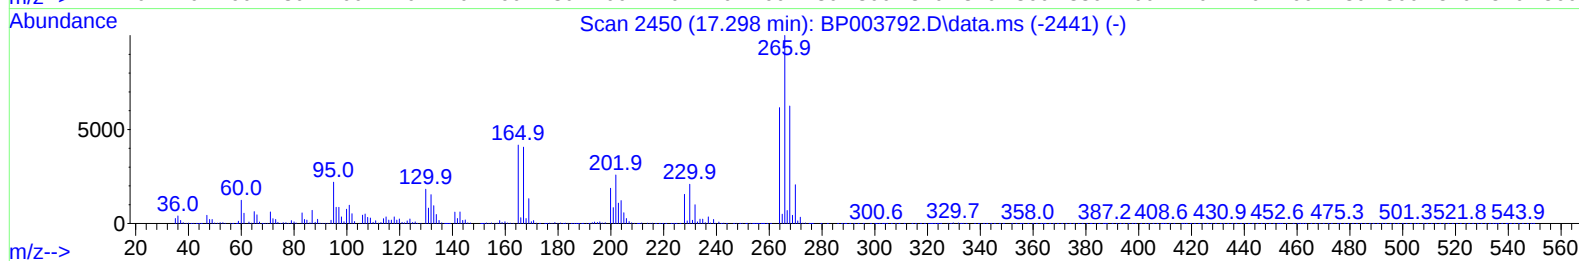
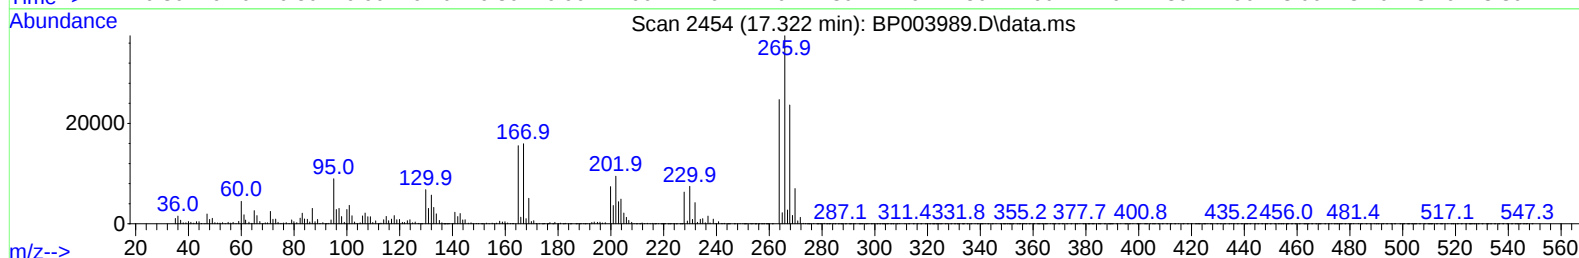


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111820\
 Data File : BP003989.D
 Acq On : 18 Nov 2020 11:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 02:17:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 12 15:22:47 2020
 Response via : Initial Calibration

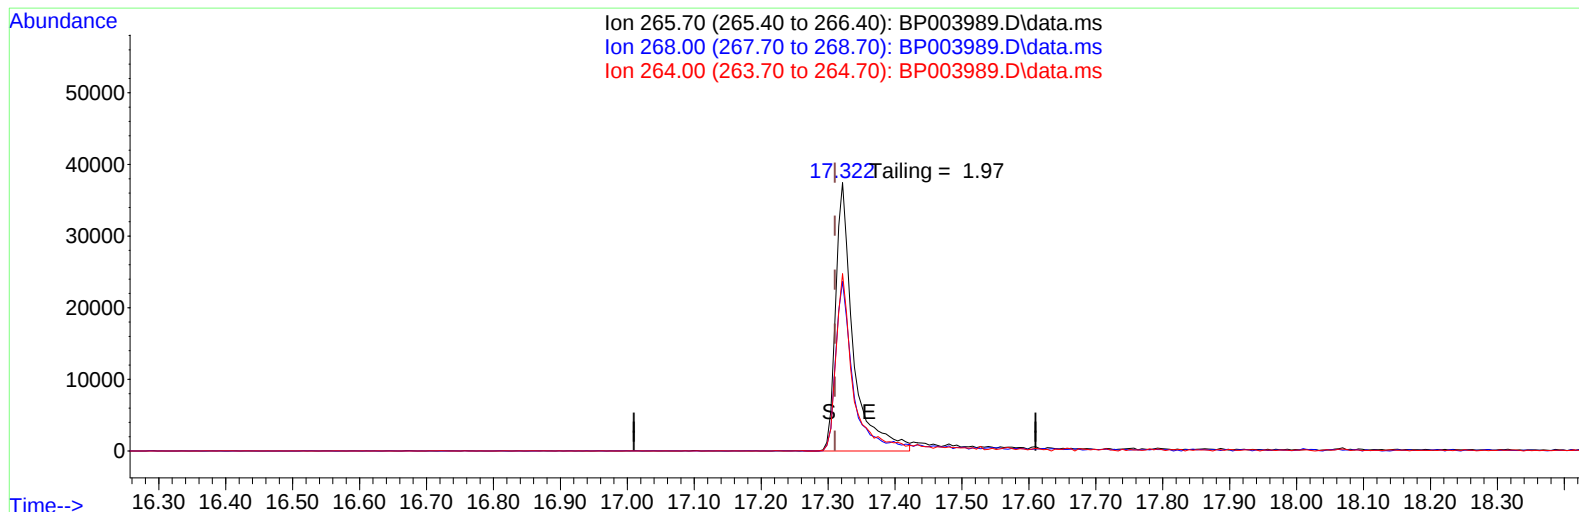

TIC: BP003989.D\data.ms

(70) Pentachlorophenol (C)




17.322min (+ 0.012) 21165.40 ng

response 68667

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.14
264.00	63.30	66.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111820\
Data File : BP003989.D
Acq On : 18 Nov 2020 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 02:17:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration

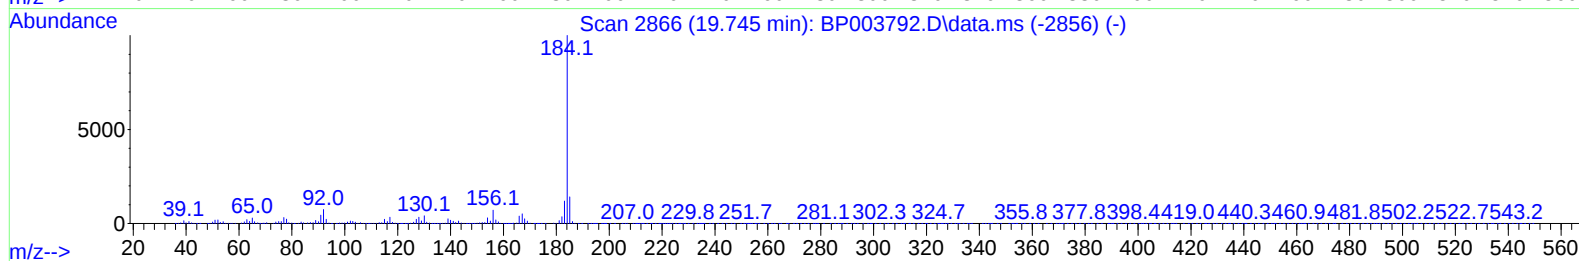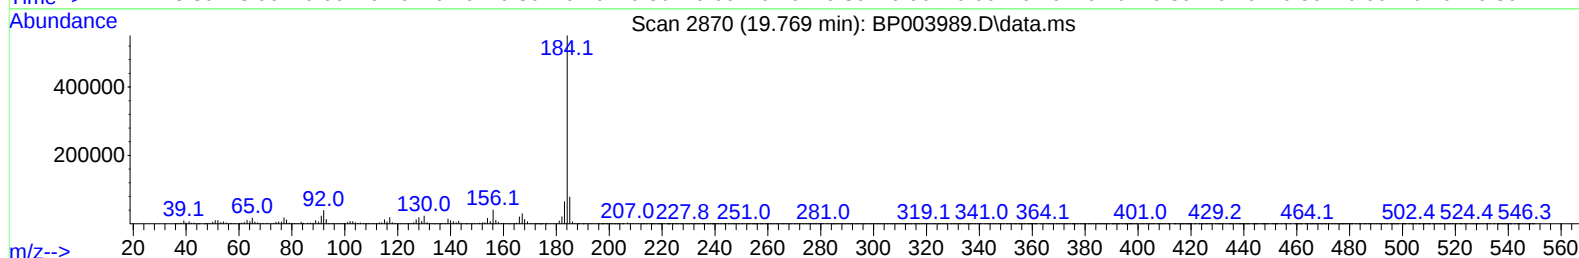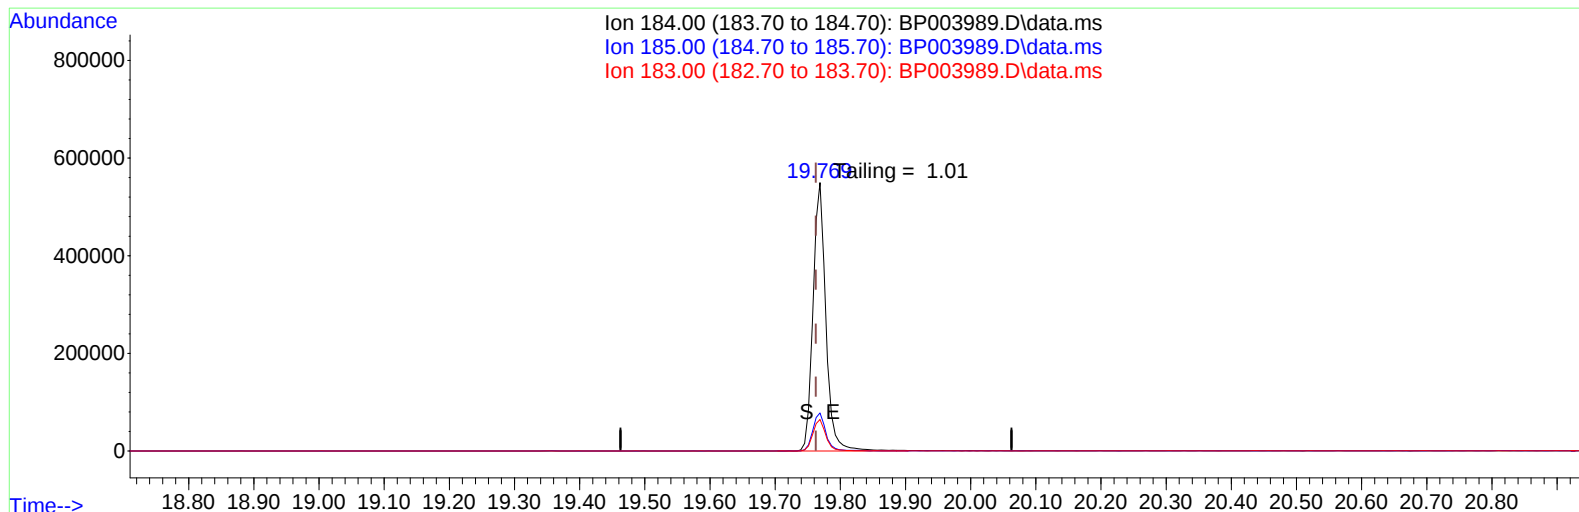

TIC: BP003989.D\data.ms

(77) Benzidine

19.769min (+ 0.006) 13318.48 ng

response 755847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.20
183.00	12.00	11.77
0.00	0.00	0.00