
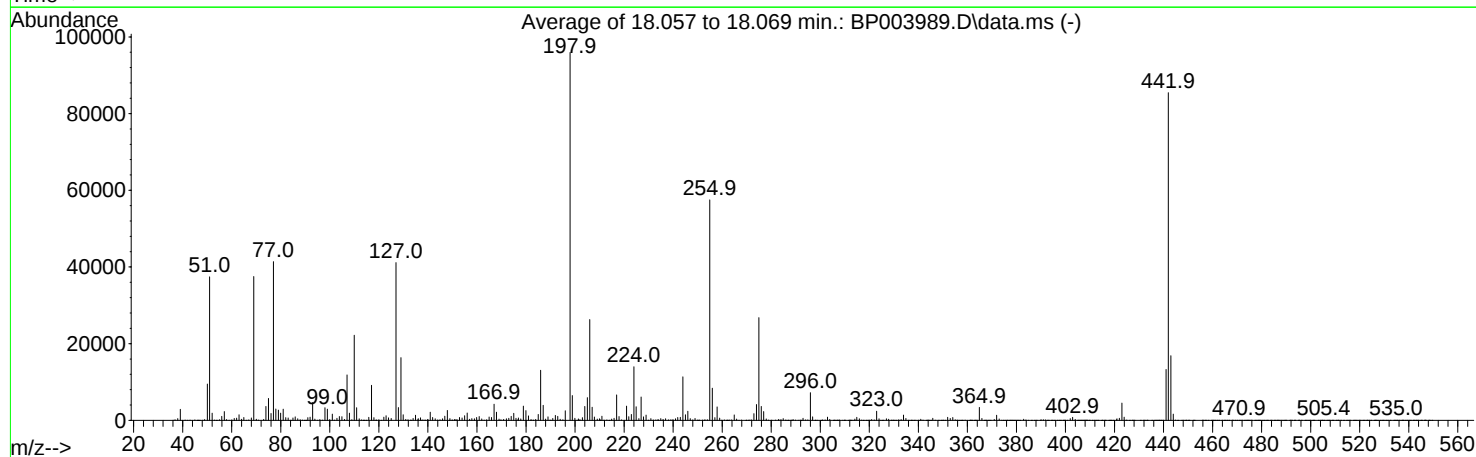


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111820\
Data File : BP003989.D
Acq On : 18 Nov 2020 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 12 15:22:47 2020

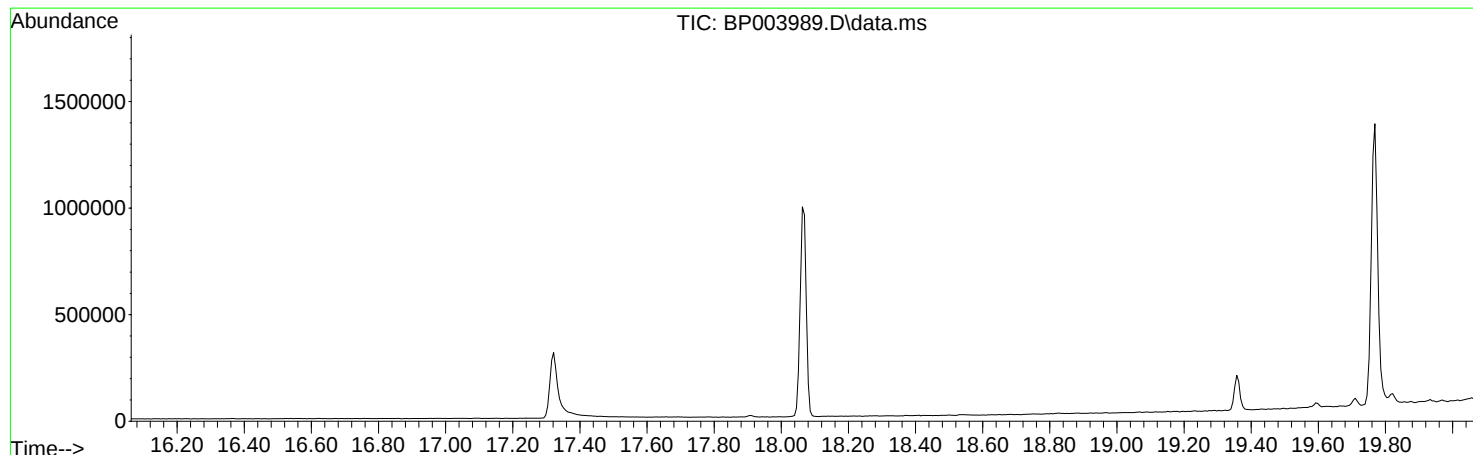

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2570

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	37451	PASS
68	69	0.00	2	1.7	648	PASS
69	198	0.00	100	39.1	37504	PASS
70	69	0.00	2	0.8	300	PASS
127	198	10	80	42.9	41149	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95936	PASS
199	198	5	9	6.7	6468	PASS
275	198	10	60	27.9	26811	PASS
365	198	1	100	3.5	3376	PASS
441	198	0.01	100	13.8	13286	PASS
442	198	50	100	89.1	85483	PASS
443	442	15	24	19.7	16881	PASS