
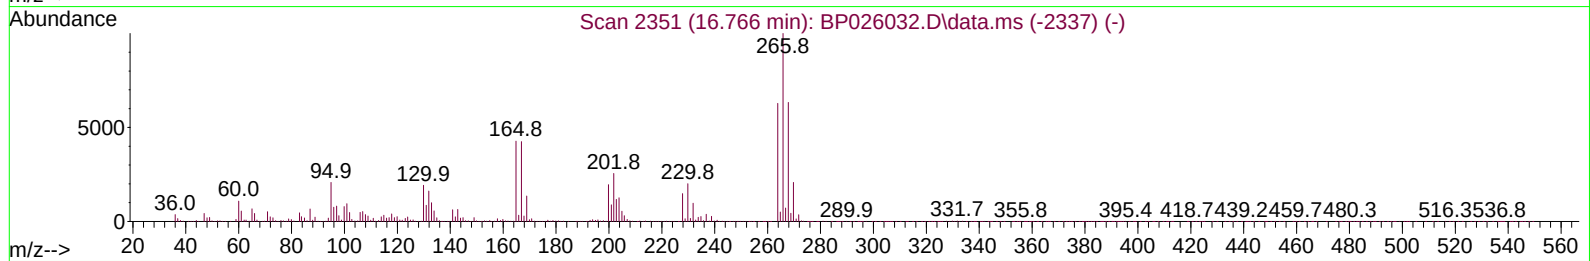
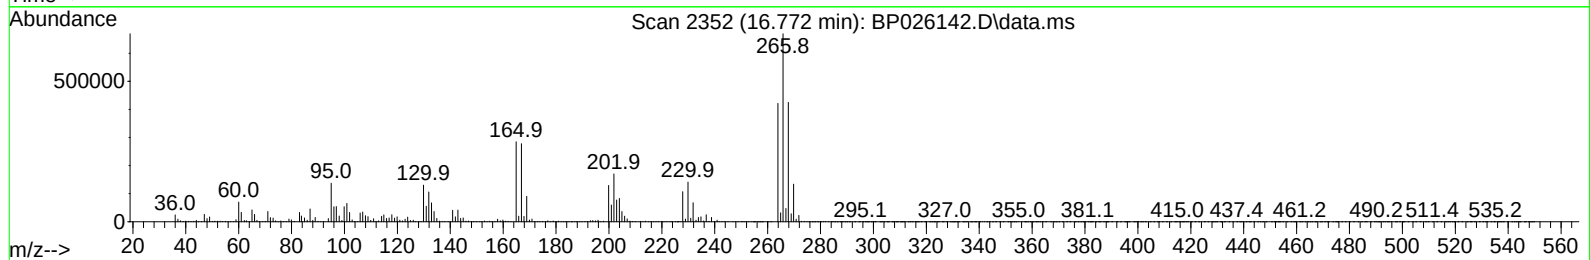


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111825\
Data File : BP026142.D
Acq On : 18 Nov 2025 13:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 00:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 00:37:08 2025
Response via : Initial Calibration

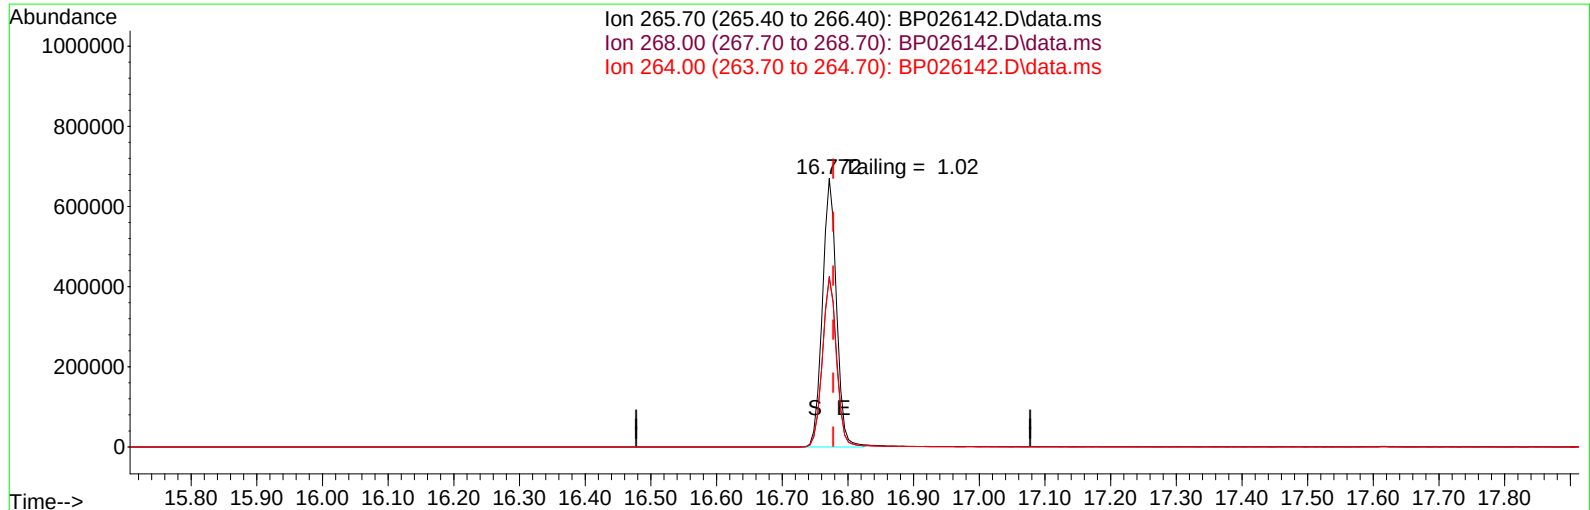

TIC: BP026142.D\data.ms

(70) Pentachlorophenol (C)




16.772min (-0.006) 1416102.53 ng

response 1013882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.49
264.00	62.70	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111825\
Data File : BP026142.D
Acq On : 18 Nov 2025 13:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 00:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 00:37:08 2025
Response via : Initial Calibration

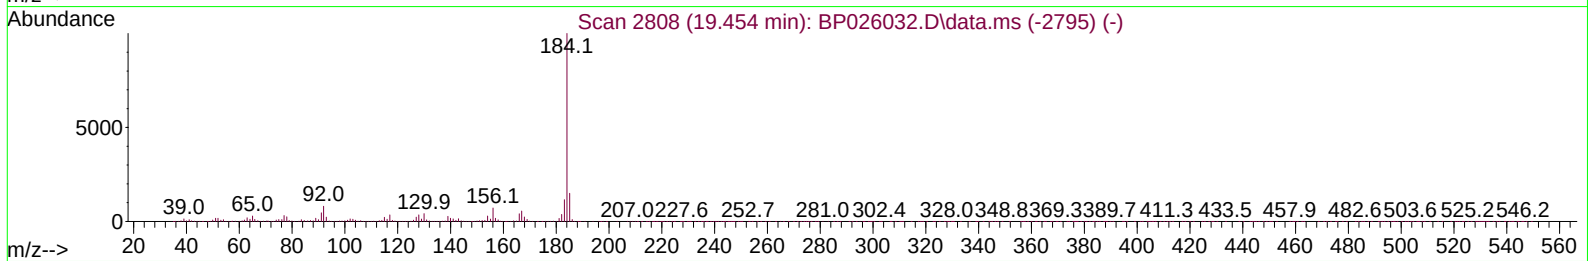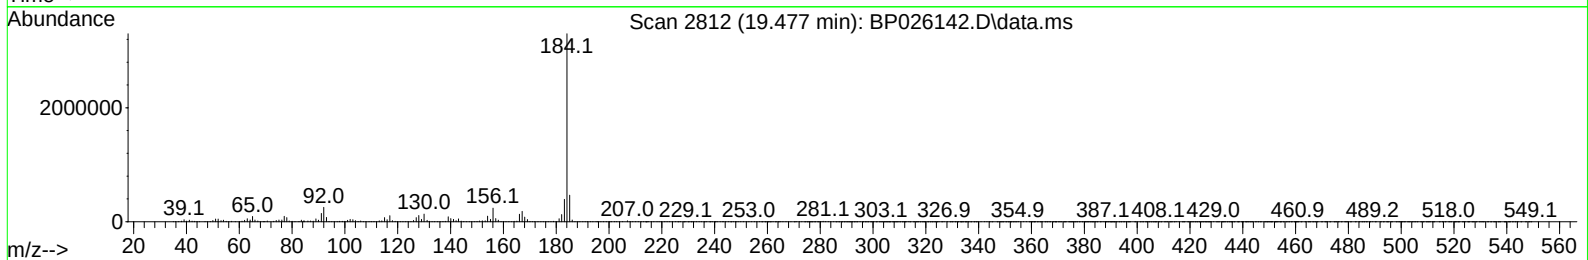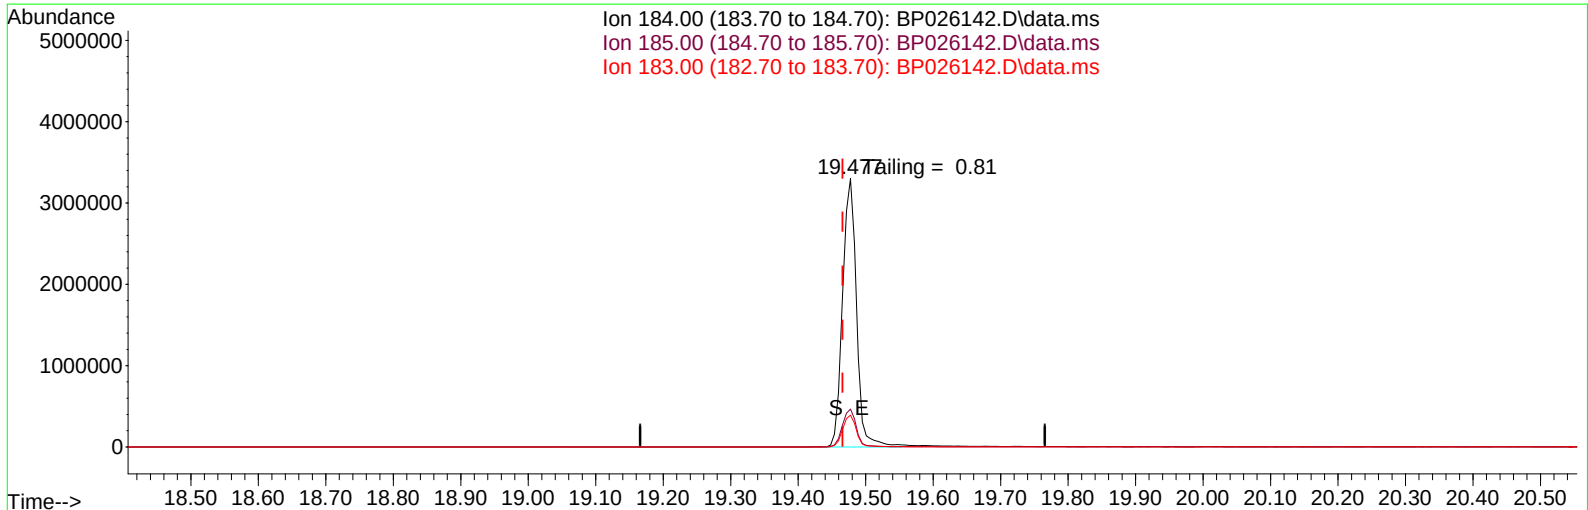

TIC: BP026142.D\data.ms

(77) Benzidine

19.477min (+ 0.012) 743702.57 ng

response 4726021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.13
183.00	11.30	11.87
0.00	0.00	0.00