
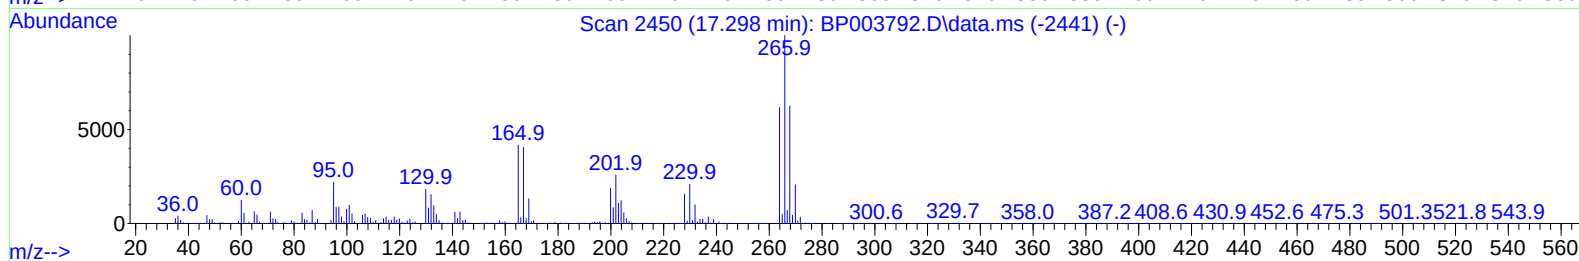
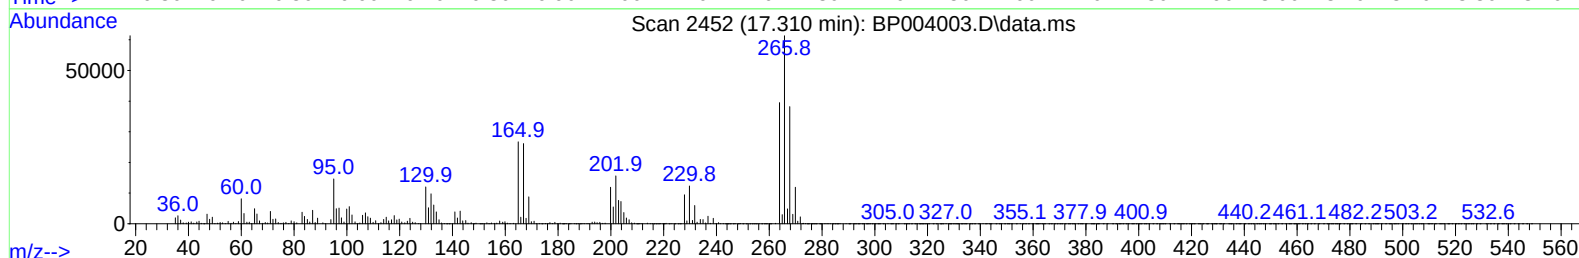


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111920\
Data File : BP004003.D
Acq On : 19 Nov 2020 14:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 08:06:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration

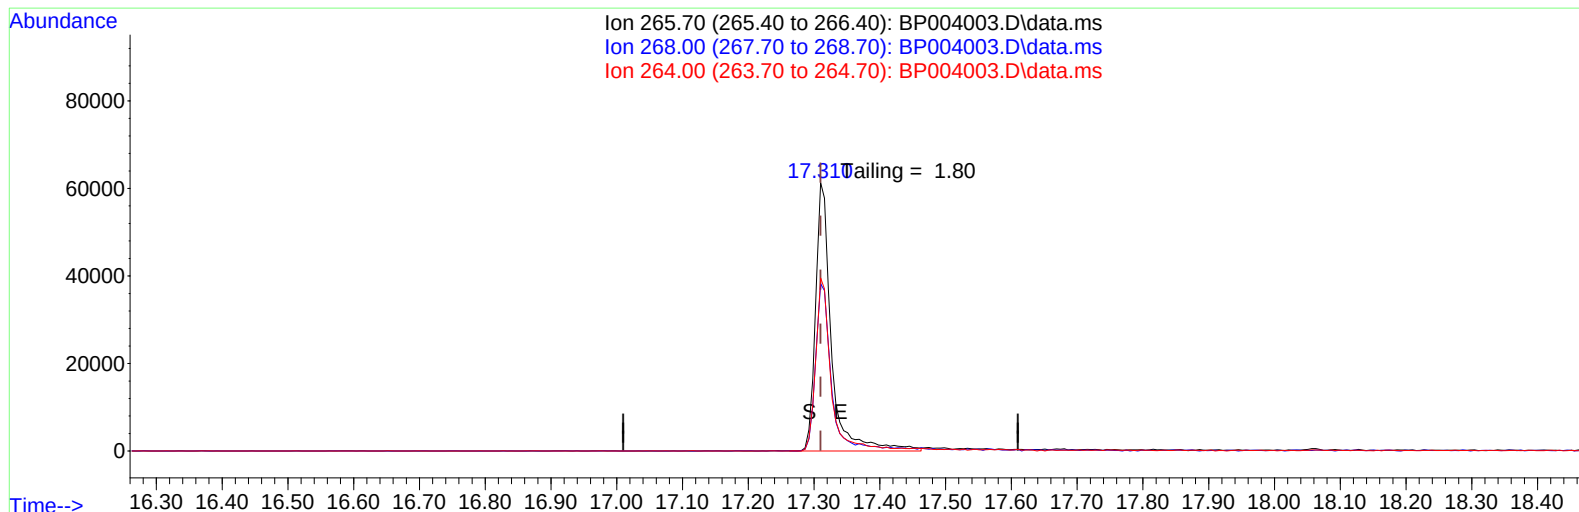

TIC: BP004003.D\data.ms

(70) Pentachlorophenol (C)




17.310min (-0.000) 16203.43 ng

response 103275

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.29
264.00	63.30	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111920\
Data File : BP004003.D
Acq On : 19 Nov 2020 14:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 08:06:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration

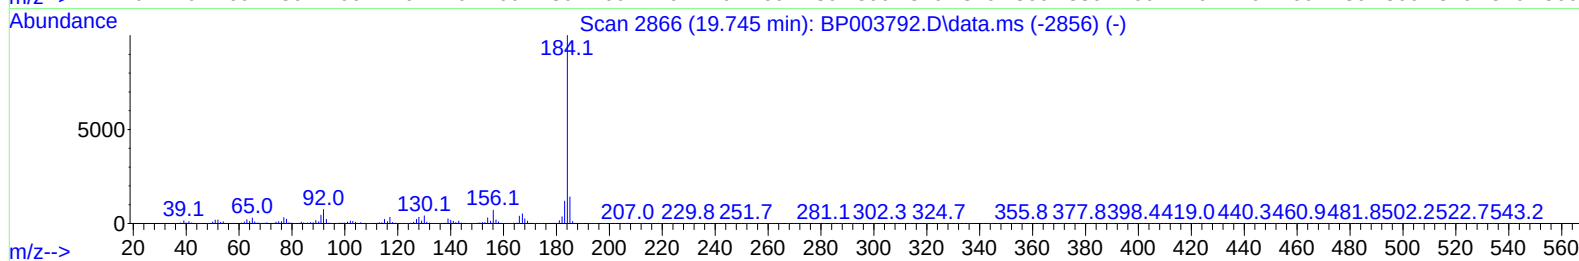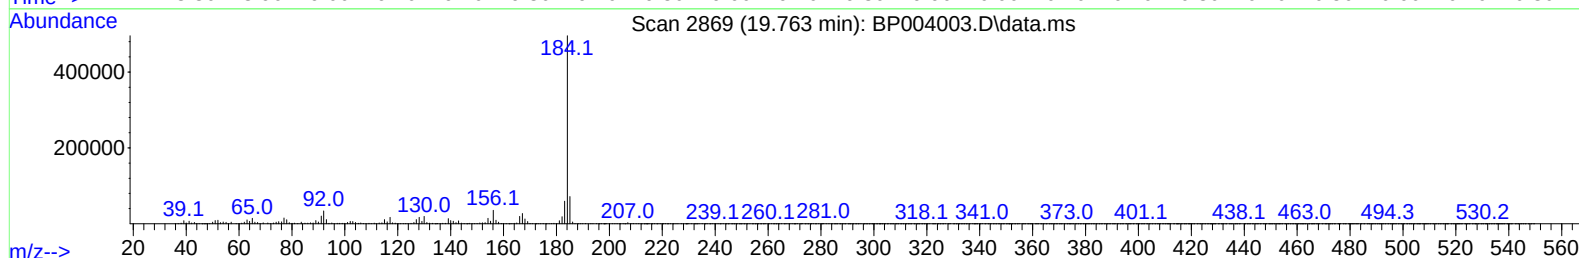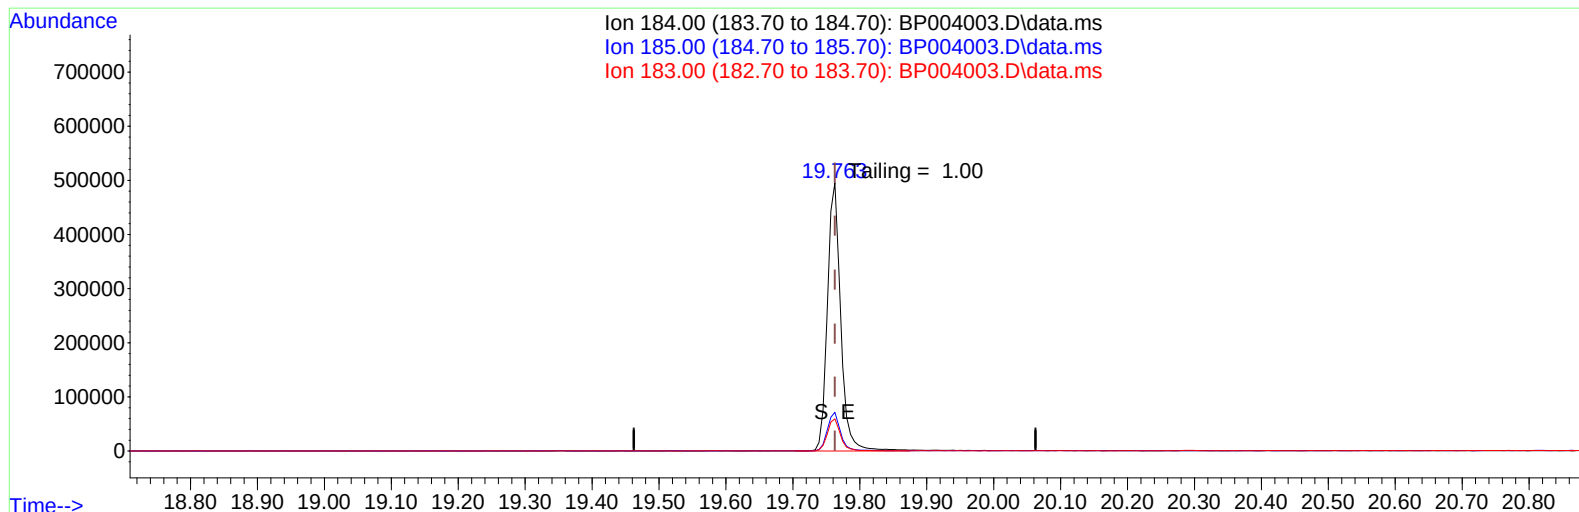

TIC: BP004003.D\data.ms

(77) Benzidine**19.763min (-0.000) 6916.73 ng****response 683431**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.44
183.00	12.00	12.02
0.00	0.00	0.00