

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111920\
 Data File : BP004008.D
 Acq On : 19 Nov 2020 17:08
 Operator : CG/JU
 Sample : PB133123BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB133123BL

Quant Time: Nov 19 17:44:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 12 15:22:47 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.269	152	123926	20.00	ng	-0.01
21) Naphthalene-d8	11.099	136	472495	20.00	ng	#-0.02
39) Acenaphthene-d10	14.893	164	294657	20.00	ng	-0.02
64) Phenanthrene-d10	17.628	188	625333	20.00	ng	#-0.01
76) Chrysene-d12	21.663	240	539761	20.00	ng	-0.01
86) Perylene-d12	24.133	264	550970	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.799	112	1031676	138.94	ng	0.00
7) Phenol-d6	7.446	99	1317739	123.63	ng	0.00
23) Nitrobenzene-d5	9.434	82	845484	87.64	ng	-0.01
42) 2,4,6-Tribromophenol	16.375	330	462830	125.58	ng	-0.02
45) 2-Fluorobiphenyl	13.516	172	1820410	86.37	ng	-0.01
79) Terphenyl-d14	20.128	244	2462587	88.14	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111920\
Data File : BP004008.D
Acq On : 19 Nov 2020 17:08
Operator : CG/JU
Sample : PB133123BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB133123BL

Quant Time: Nov 19 17:44:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 12 15:22:47 2020
Response via : Initial Calibration




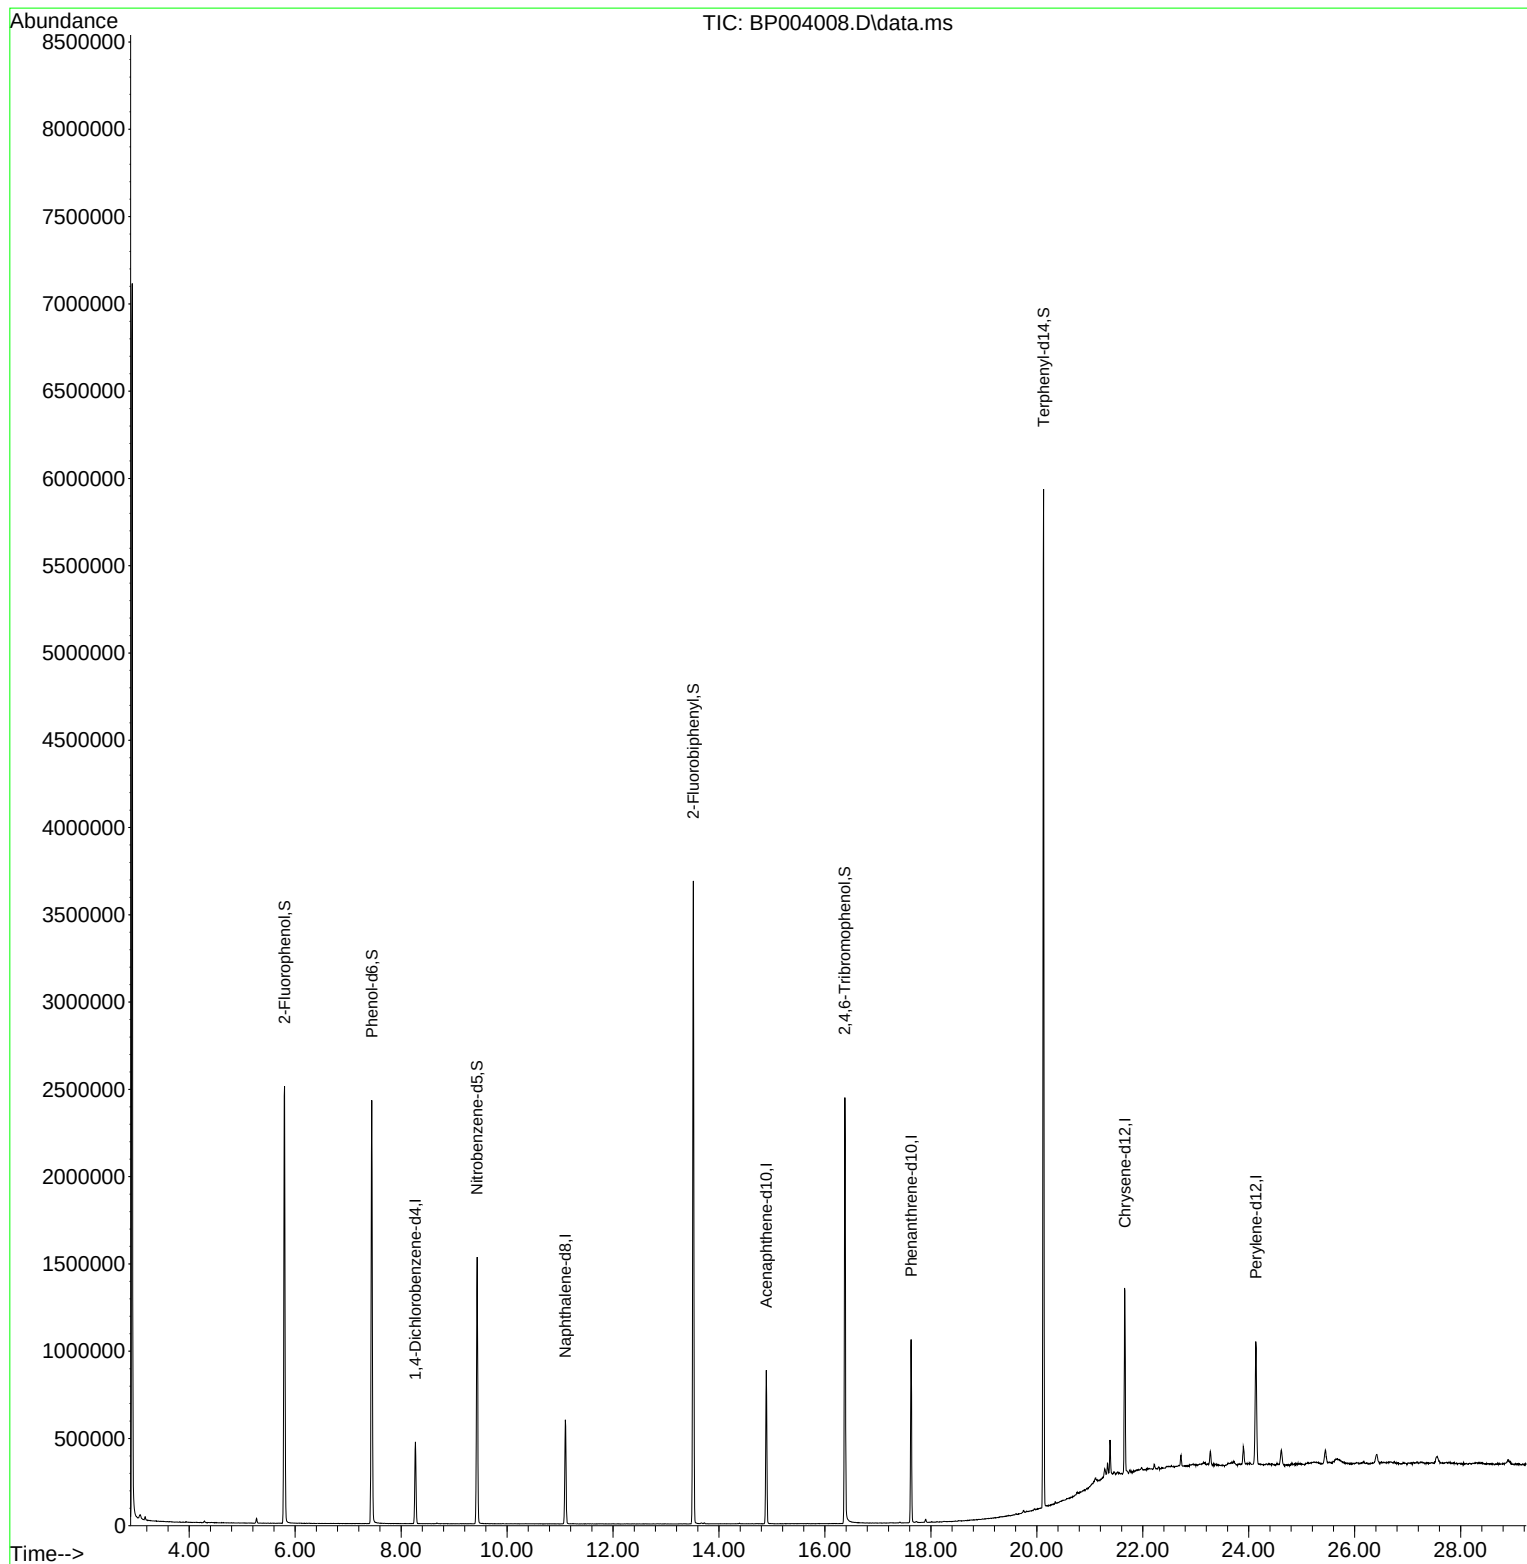




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.269 min Scan# 915
Delta R.T. -0.012 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08




Instrument :
BNA_P
ClientSampleId :
PB133123BL


Tgt Ion:152 Resp: 123926
Ion Ratio Lower Upper
152 100
150 157.3 123.8 185.6
115 60.8 43.8 65.6

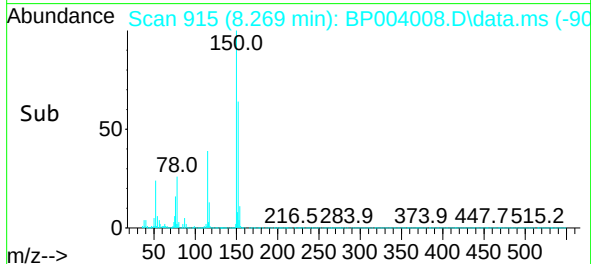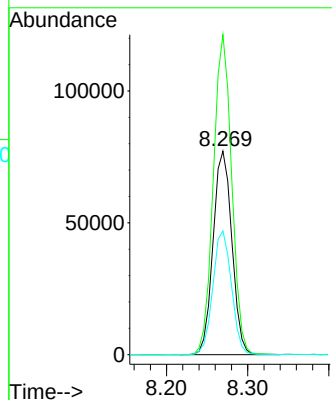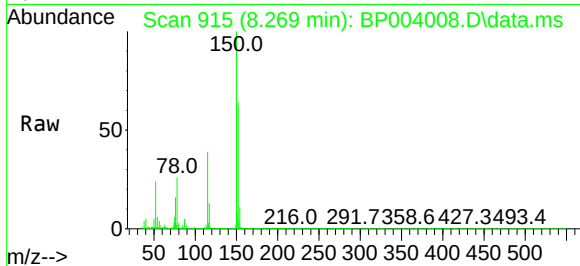

#5
2-Fluorophenol
Concen: 138.94 ng
RT: 5.799 min Scan# 495
Delta R.T. -0.006 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08

Tgt Ion:112 Resp: 1031676
Ion Ratio Lower Upper
112 100
64 63.0 32.8 49.2#
63 33.4 17.0 25.4#


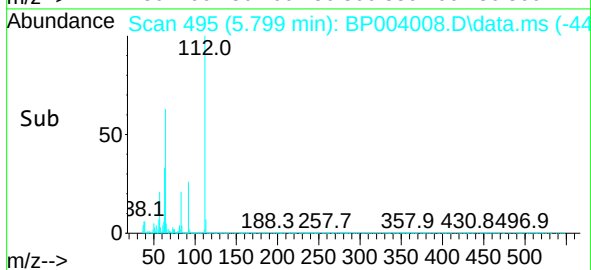
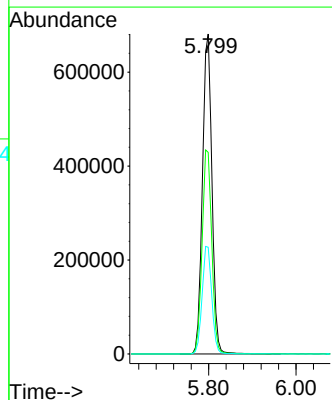
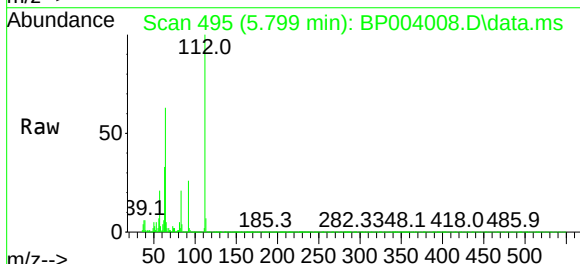




#7
Phenol-d6
Concen: 123.63 ng
RT: 7.446 min Scan# 775
Delta R.T. -0.006 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08




Instrument :
BNA_P
ClientSampleId :
PB133123BL


Tgt Ion: 99 Resp: 1317739
Ion Ratio Lower Upper
99 100
42 19.9 8.6 13.0#
71 36.2 23.4 35.2#

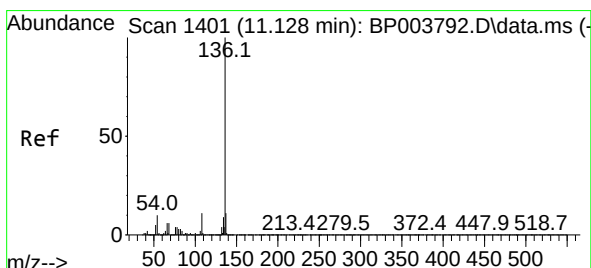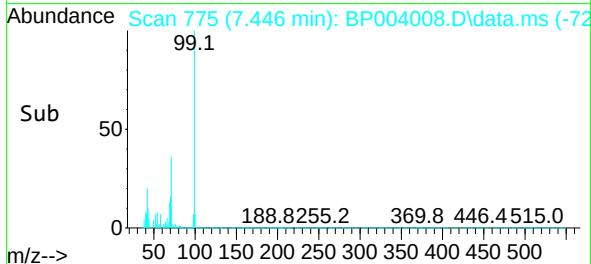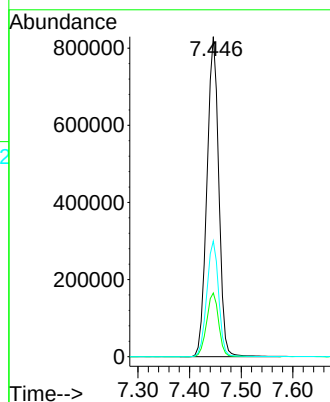

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.099 min Scan# 1396
Delta R.T. -0.017 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08

Tgt Ion: 136 Resp: 472495
Ion Ratio Lower Upper
136 100
137 10.7 8.6 13.0
54 10.1 3.6 5.4#
68 5.9 3.3 4.9#


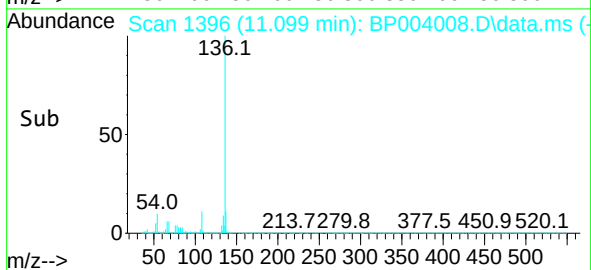
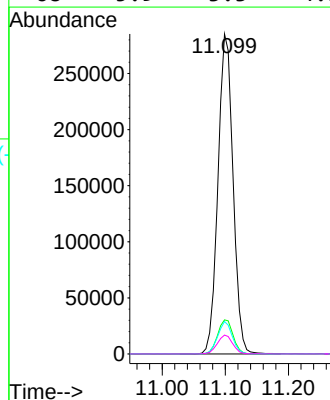
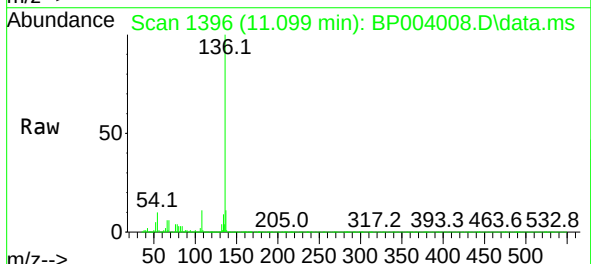




#23
Nitrobenzene-d5
Concen: 87.64 ng
RT: 9.434 min Scan# 1113
Delta R.T. -0.012 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08




Instrument :
BNA_P
ClientSampleId :
PB133123BL


Tgt Ion: 82 Resp: 845484
Ion Ratio Lower Upper
82 100
128 41.3 45.6 68.4#
54 54.8 30.1 45.1#

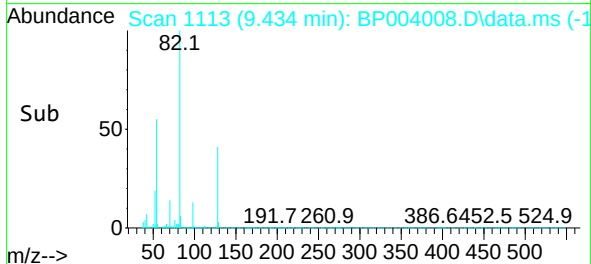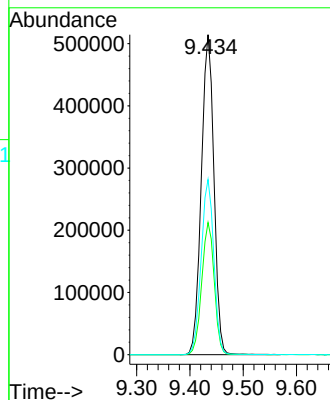

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.893 min Scan# 2041
Delta R.T. -0.017 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08

Tgt Ion:164 Resp: 294657
Ion Ratio Lower Upper
164 100
162 102.1 79.4 119.2
160 44.2 36.1 54.1


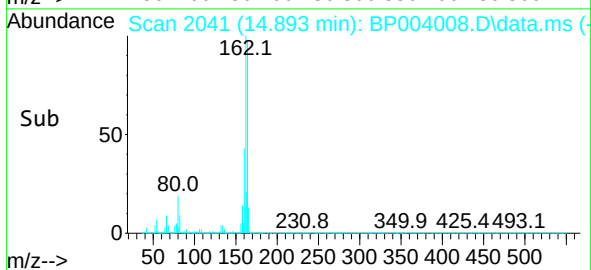
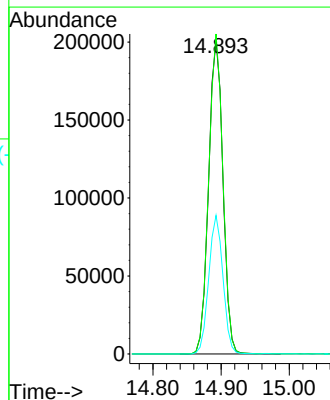
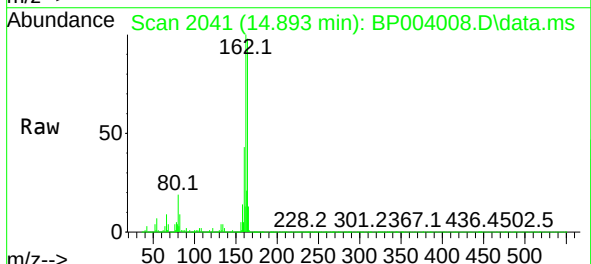




#42
2,4,6-Tribromophenol
Concen: 125.58 ng
RT: 16.375 min Scan# 2293
Delta R.T. -0.017 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08




Instrument :
BNA_P
ClientSampleId :
PB133123BL


Tgt Ion:330 Resp: 462830
Ion Ratio Lower Upper
330 100
332 97.9 77.1 115.7
141 32.7 23.4 35.2

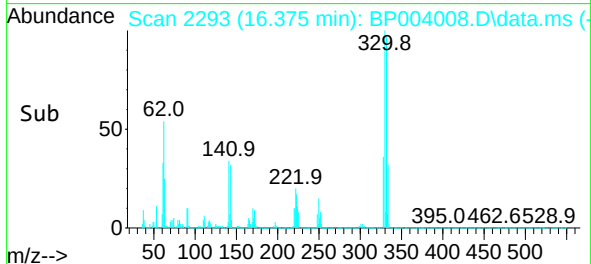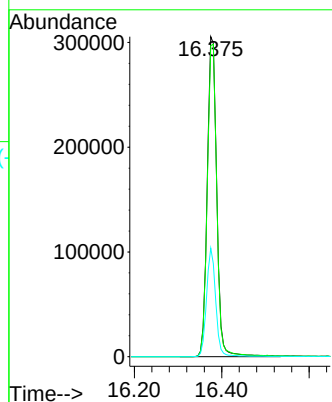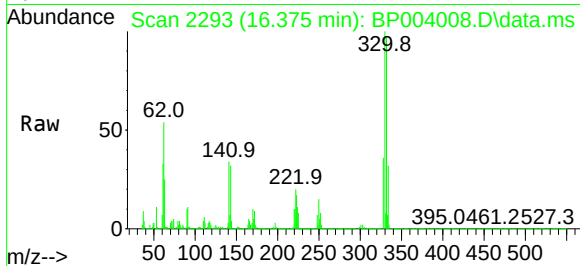

#45
2-Fluorobiphenyl
Concen: 86.37 ng
RT: 13.516 min Scan# 1807
Delta R.T. -0.012 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08

Tgt Ion:172 Resp: 1820410
Ion Ratio Lower Upper
172 100
171 35.3 28.5 42.7
170 22.9 19.2 28.8


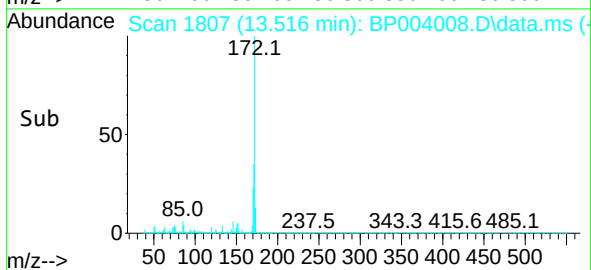
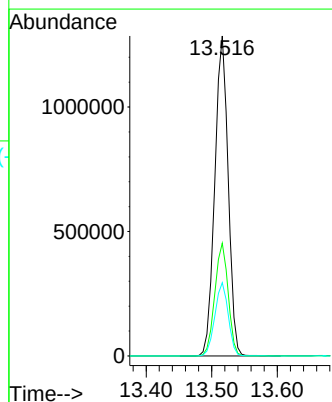
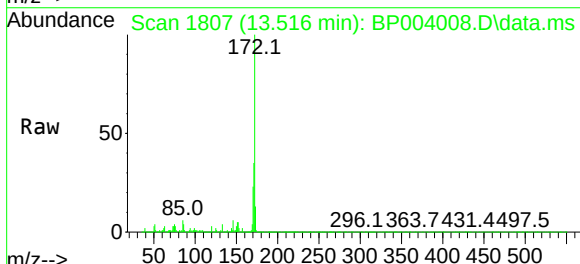




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.628 min Scan# 2506
Delta R.T. -0.012 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08




Instrument :
BNA_P
ClientSampleId :
PB133123BL


Tgt Ion:188 Resp: 625333
Ion Ratio Lower Upper
188 100
94 8.1 6.2 9.2
80 9.5 6.2 9.2#

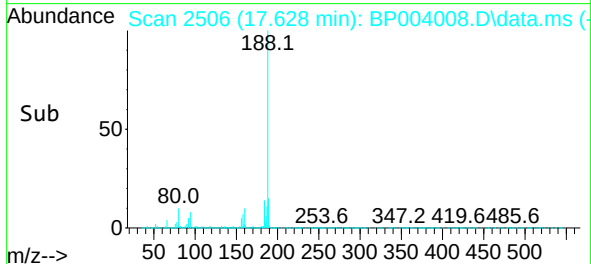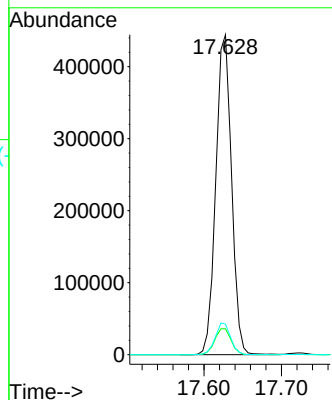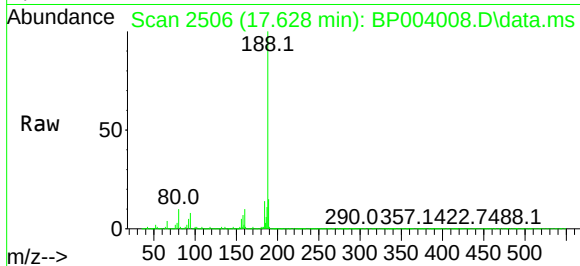

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.663 min Scan# 3192
Delta R.T. -0.012 min
Lab File: BP004008.D
Acq: 19 Nov 2020 17:08

Tgt Ion:240 Resp: 539761
Ion Ratio Lower Upper
240 100
120 8.6 7.8 11.6
236 24.0 20.8 31.2


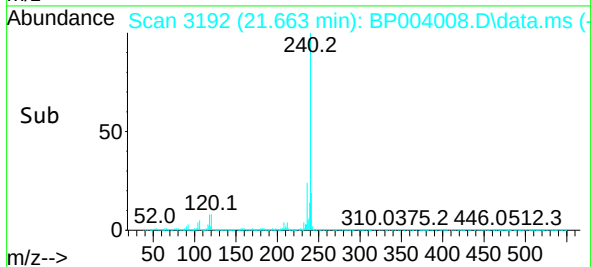
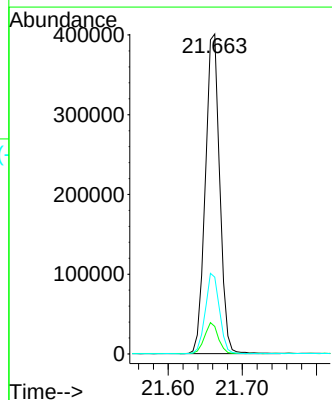
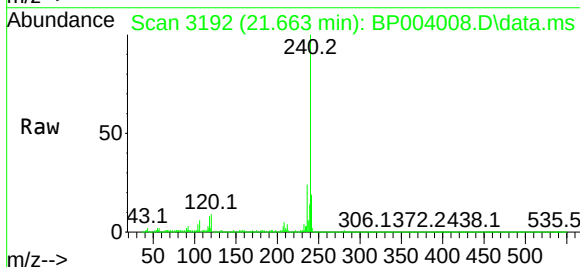




#79
 Terphenyl-d14
 Concen: 88.14 ng
 RT: 20.128 min Scan# 2931
 Delta R.T. -0.006 min
 Lab File: BP004008.D
 Acq: 19 Nov 2020 17:08

Instrument :
 BNA_P
 ClientSampleId :
 PB133123BL

Tgt Ion:244 Resp: 2462587
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.8 8.6
 122 9.1 7.8 11.8

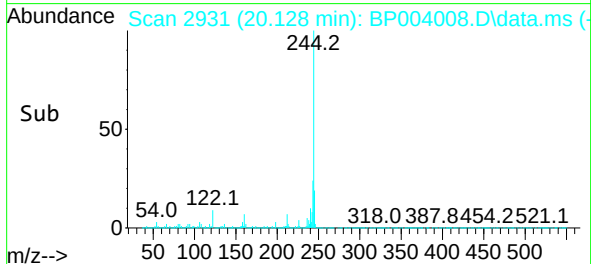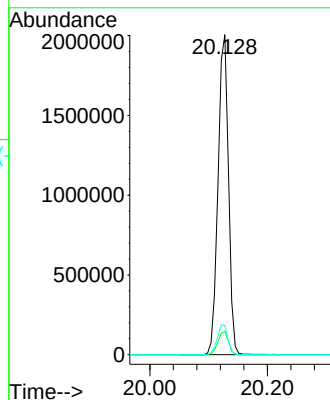

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 24.133 min Scan# 3612
 Delta R.T. -0.023 min
 Lab File: BP004008.D
 Acq: 19 Nov 2020 17:08

Tgt Ion:264 Resp: 550970
 Ion Ratio Lower Upper
 264 100
 260 23.3 18.8 28.2
 265 21.5 17.4 26.2

