
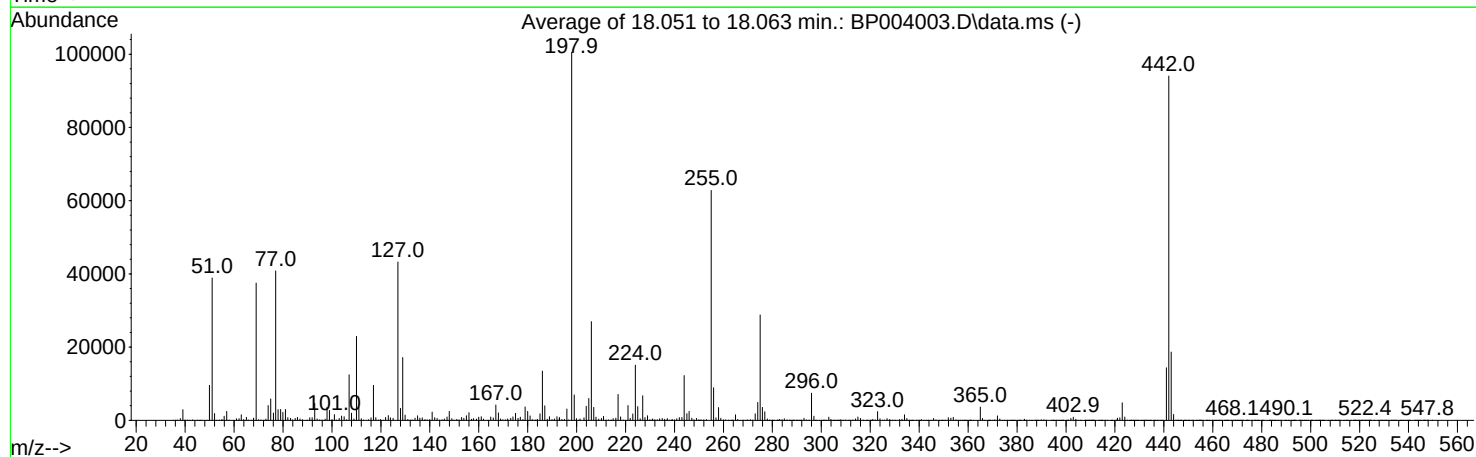


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111920\
 Data File : BP004003.D
 Acq On : 19 Nov 2020 14:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 12 15:22:47 2020

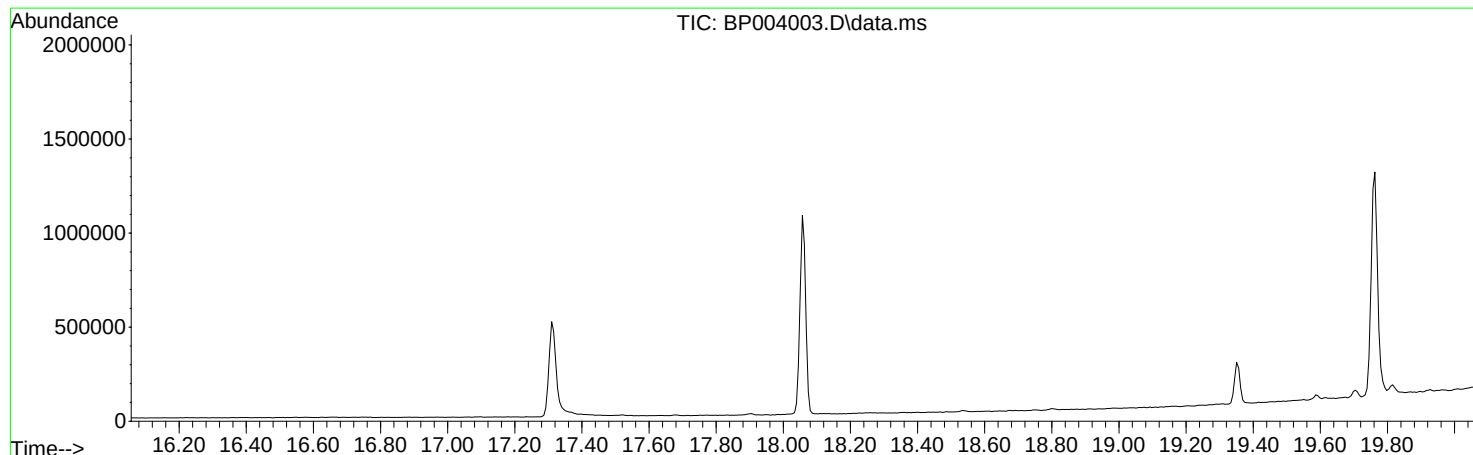

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	38902	PASS
68	69	0.00	2	1.7	623	PASS
69	198	0.00	100	37.3	37492	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	43.1	43256	PASS
197	198	0.00	2	0.1	121	PASS
198	198	100	100	100.0	100462	PASS
199	198	5	9	6.9	6957	PASS
275	198	10	60	28.7	28790	PASS
365	198	1	100	3.6	3648	PASS
441	198	0.01	100	14.3	14399	PASS
442	198	50	100	93.6	94024	PASS
443	442	15	24	19.9	18679	PASS