
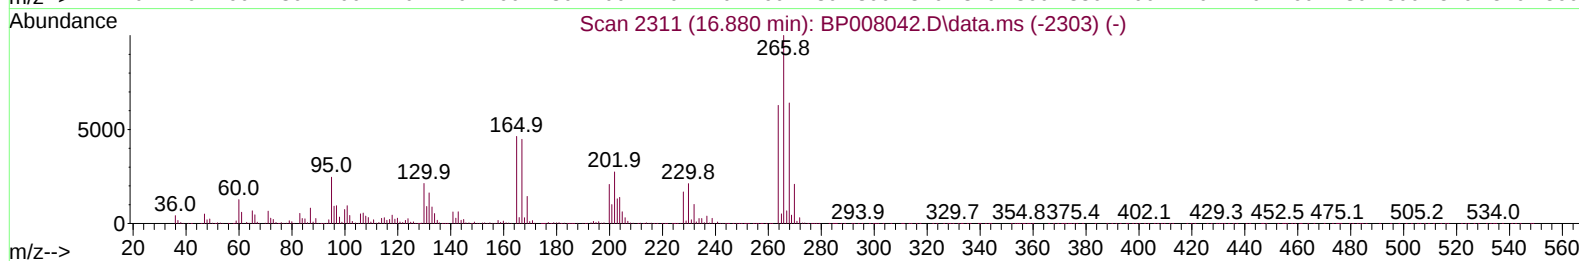
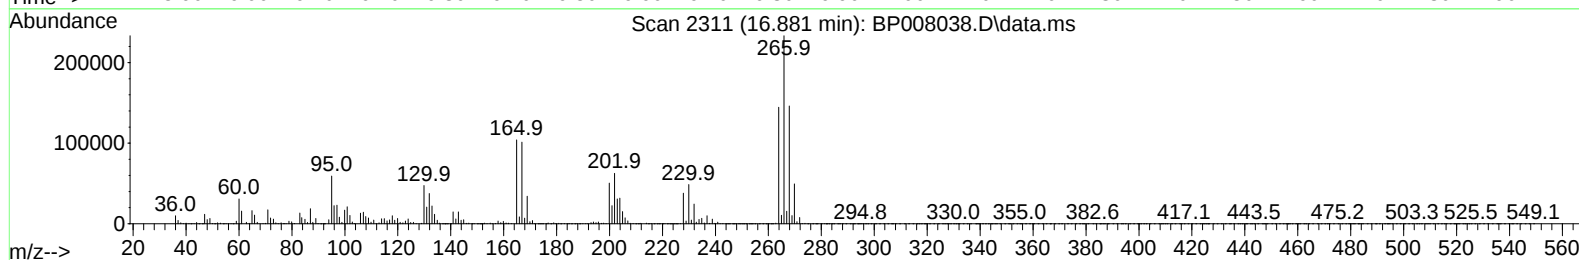


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
 Data File : BP008038.D
 Acq On : 19 Nov 2021 15:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 02:25:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

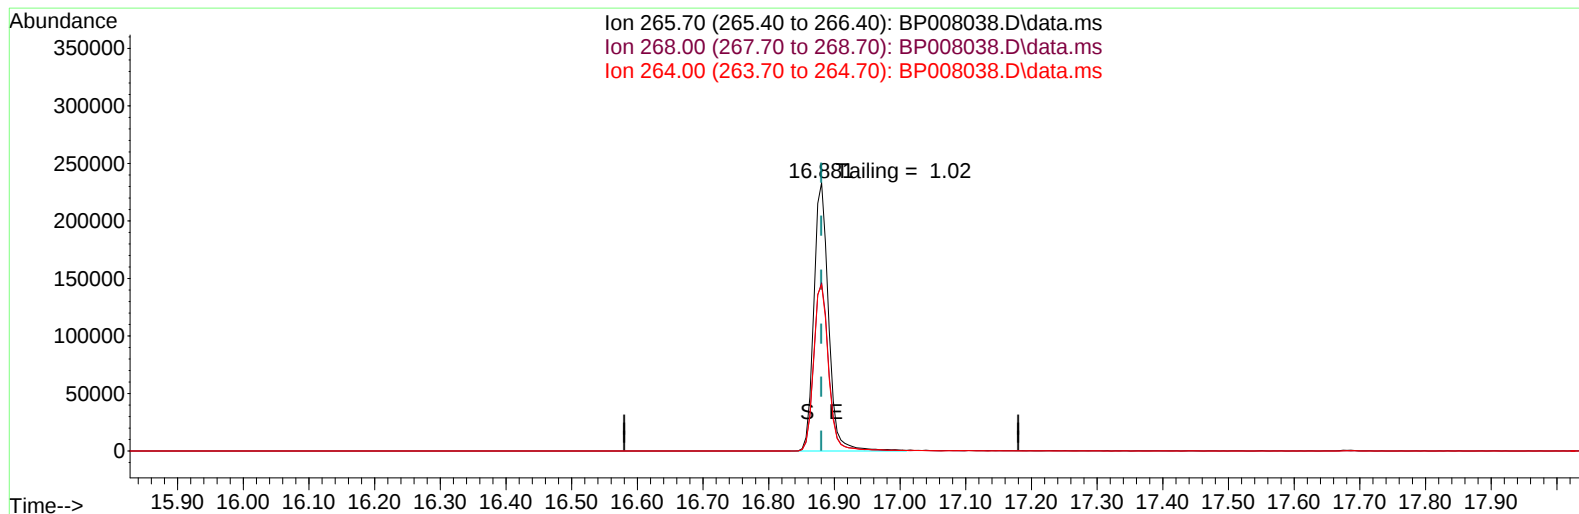




TIC: BP008038.D\data.ms

(70) Pentachlorophenol (C)**16.881min (+ 0.001) 929381.98 ng****response 364335**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.67
264.00	62.80	61.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
 Data File : BP008038.D
 Acq On : 19 Nov 2021 15:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 02:25:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

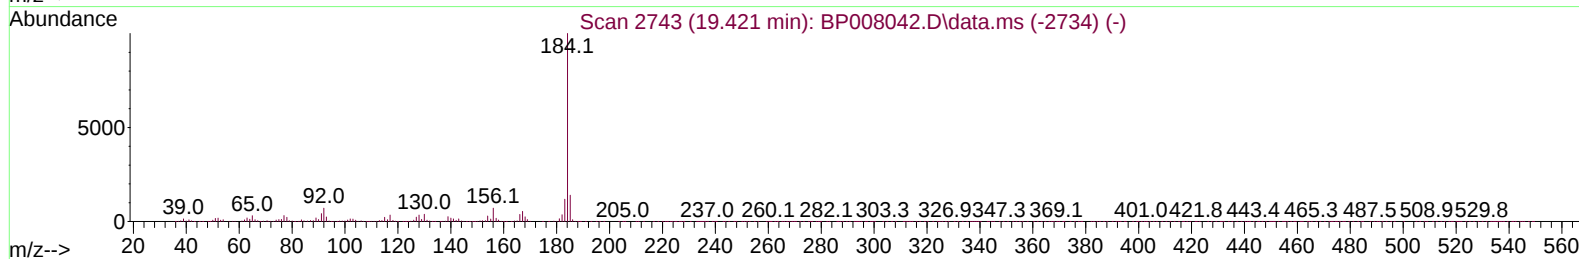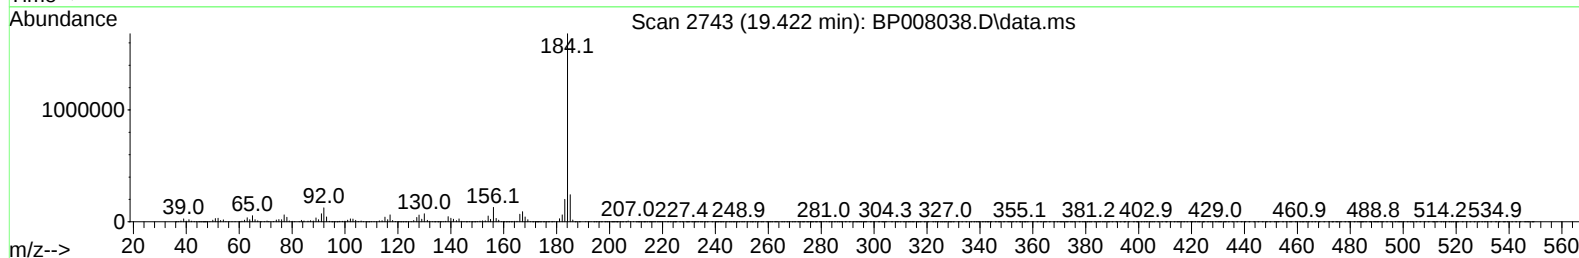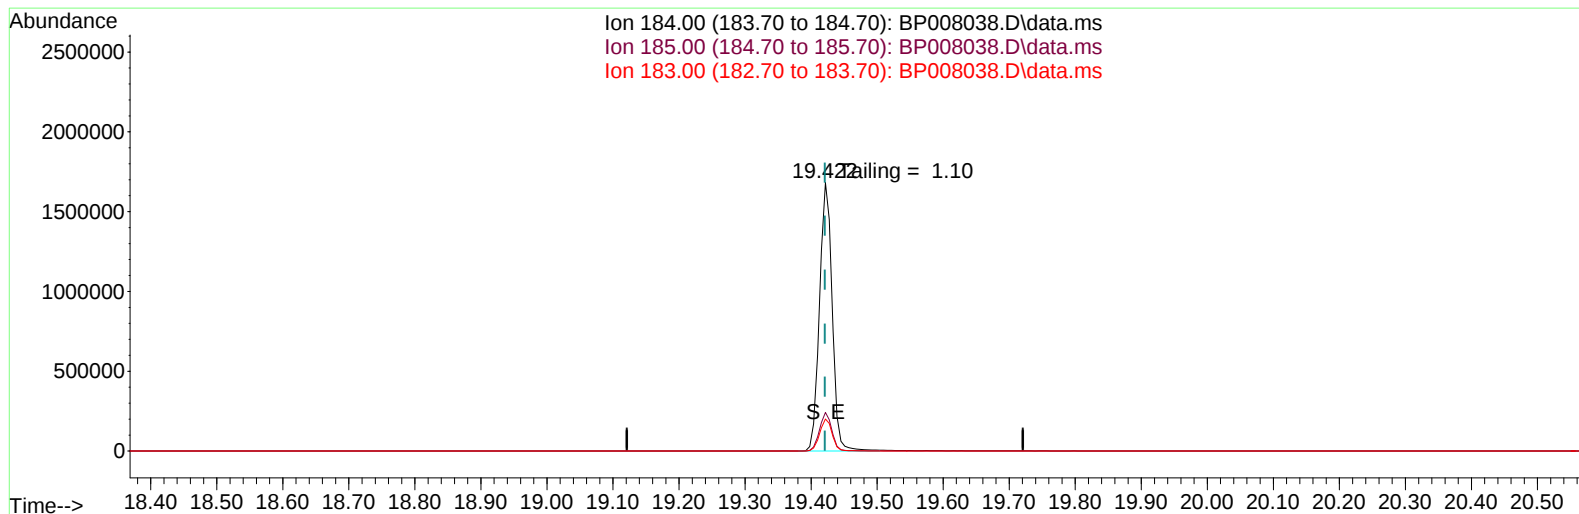

TIC: BP008038.D\data.ms

(77) Benzidine**19.422min (+ 0.001) 492152.46 ng****response 2254000**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	11.80	11.94
0.00	0.00	0.00