

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008047.D
Acq On : 19 Nov 2021 20:50
Operator : CG/JU
Sample : PB140918BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140918BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	355	362	372	rBV	3436083	5005692	47.29%	10.197%
2	7.005	624	632	647	rBV	3156873	5168683	48.83%	10.529%
3	7.822	764	771	782	rBV	663091	1063183	10.04%	2.166%
4	8.987	958	969	980	rBV	2038472	3460938	32.70%	7.050%
5	10.622	1238	1247	1261	rBV	844822	1443167	13.63%	2.940%
6	13.087	1656	1666	1682	rBV	4718880	7290718	68.88%	14.851%
7	14.463	1893	1900	1914	rBV	1358255	2031327	19.19%	4.138%
8	15.957	2147	2154	2176	rBV	3753836	5737559	54.20%	11.687%
9	17.222	2362	2369	2383	rBV	1700967	2533307	23.93%	5.160%
10	19.786	2799	2805	2810	rBV	8114077	10585265	100.00%	21.562%
11	21.310	3059	3064	3073	rBV	1934336	2625695	24.81%	5.349%
12	23.704	3465	3471	3481	rVB2	1011516	2146597	20.28%	4.373%




Sum of corrected areas: 49092131

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008047.D
Acq On : 19 Nov 2021 20:50
Operator : CG/JU
Sample : PB140918BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140918BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

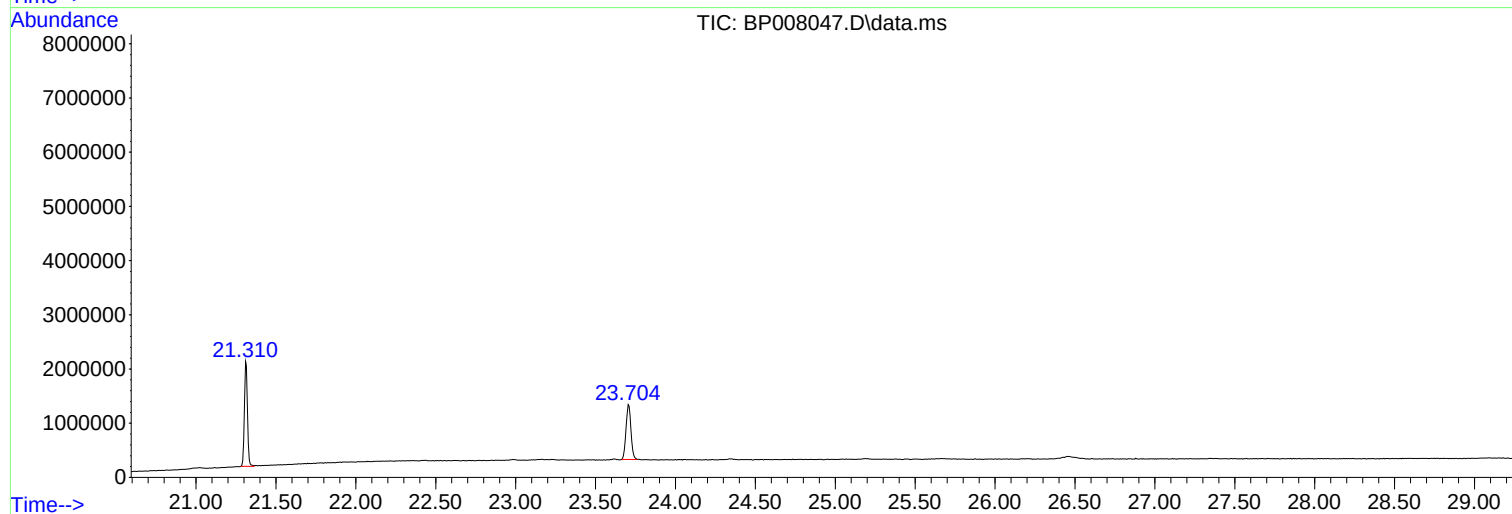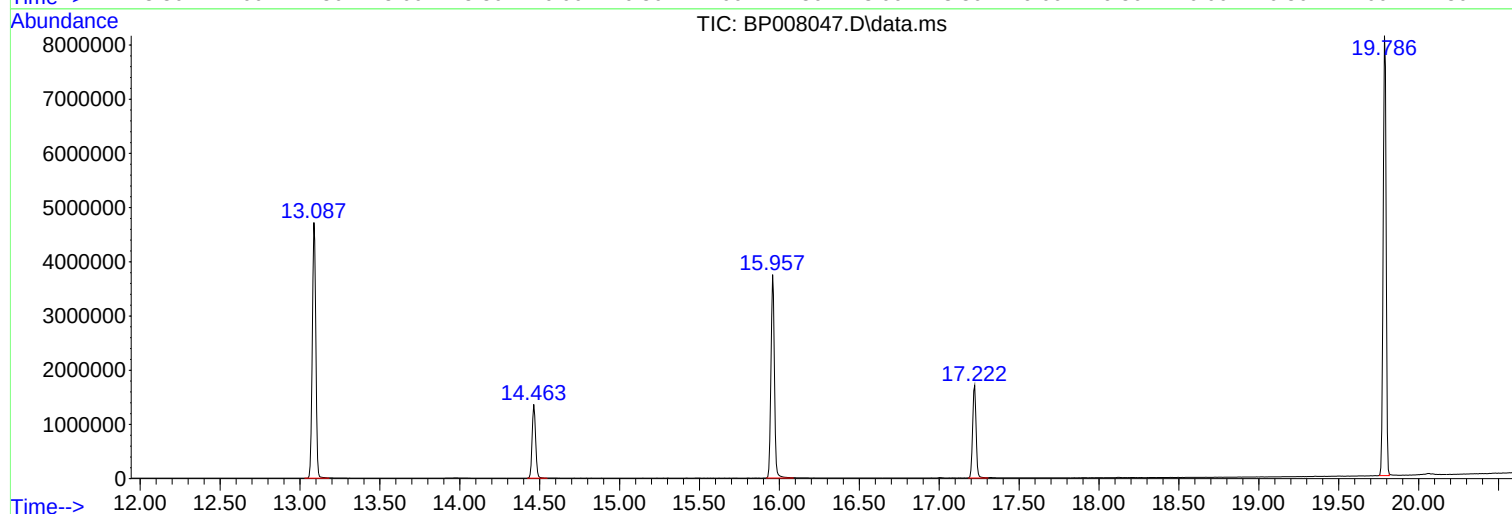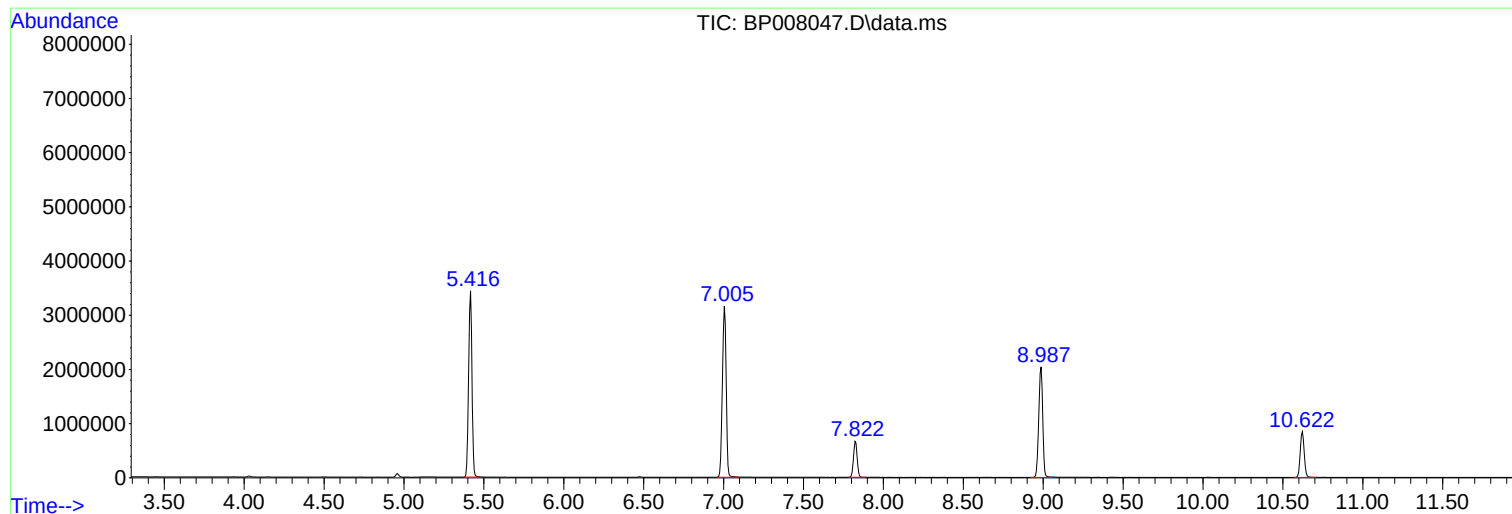

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008047.D
Acq On : 19 Nov 2021 20:50
Operator : CG/JU
Sample : PB140918BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140918BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008047.D
Acq On : 19 Nov 2021 20:50
Operator : CG/JU
Sample : PB140918BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140918BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------