

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008048.D
Acq On : 19 Nov 2021 21:24
Operator : CG/JU
Sample : PB140896BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140896BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.417	355	362	380	rBV	3598023	5380326	46.36%	10.296%
2	7.005	623	632	647	rBV	3325718	5592701	48.19%	10.702%
3	7.822	764	771	781	rBV	654973	1037106	8.94%	1.985%
4	8.987	957	969	986	rBV	2131226	3645713	31.41%	6.977%
5	10.622	1239	1247	1258	rBV	821059	1416583	12.21%	2.711%
6	13.087	1659	1666	1684	rBV	4868722	7572452	65.25%	14.491%
7	14.463	1893	1900	1916	rBV	1308854	1972087	16.99%	3.774%
8	15.957	2145	2154	2179	rBV	4004763	6167737	53.14%	11.803%
9	17.216	2362	2368	2383	rBV	1642716	2492566	21.48%	4.770%
10	19.786	2799	2805	2810	rBV	8958814	11606082	100.00%	22.210%
11	21.310	3059	3064	3074	rBV	2068644	2824983	24.34%	5.406%
12	23.704	3464	3471	3485	rBV2	1256791	2548618	21.96%	4.877%




Sum of corrected areas: 52256954

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008048.D
Acq On : 19 Nov 2021 21:24
Operator : CG/JU
Sample : PB140896BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140896BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

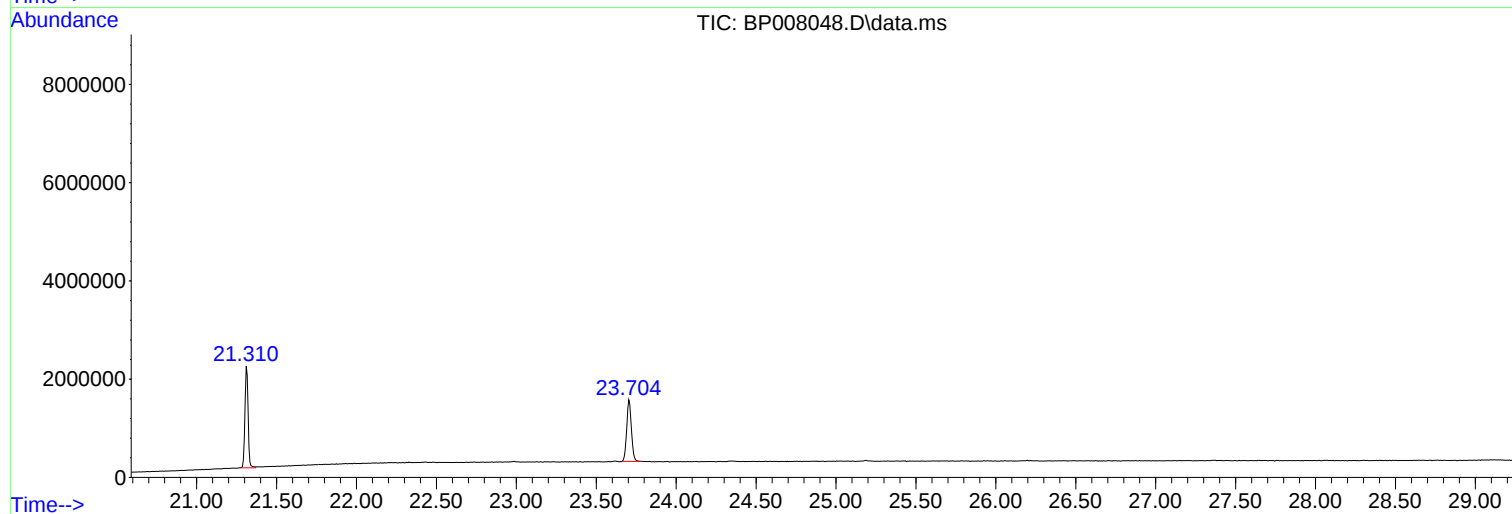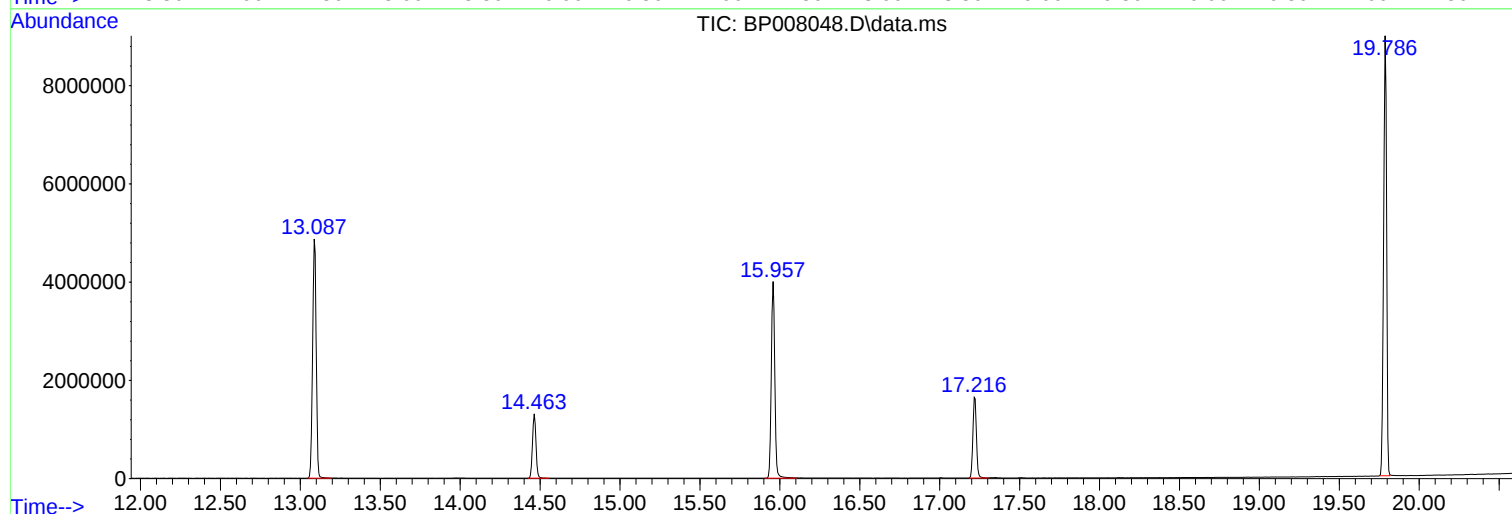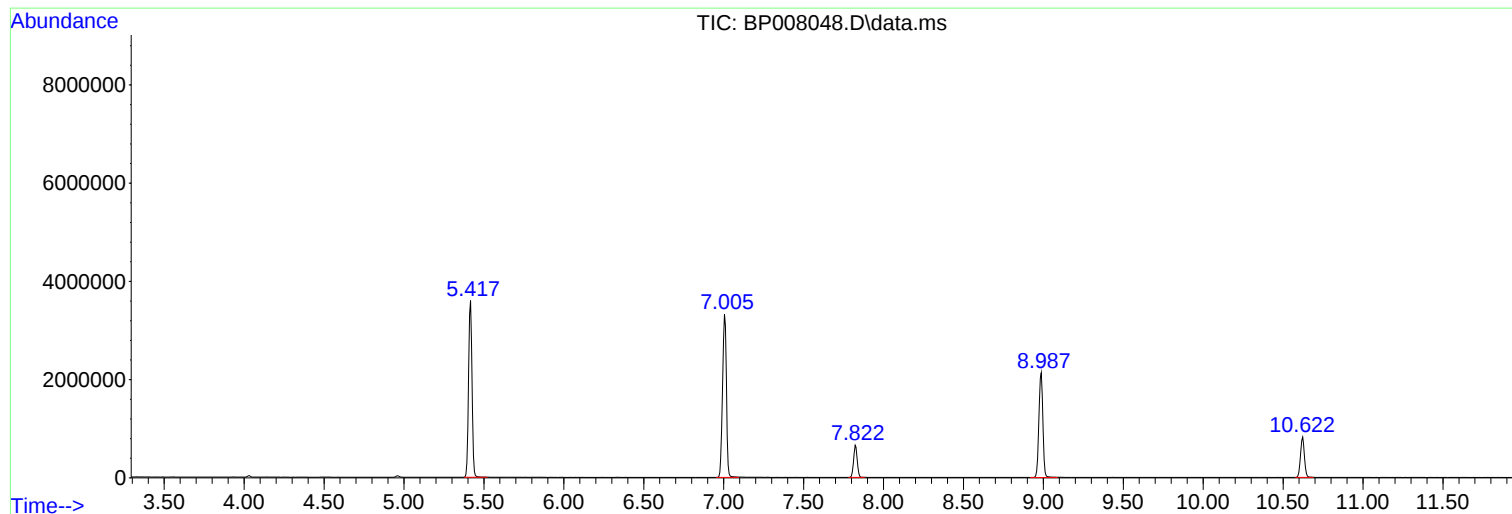

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008048.D
Acq On : 19 Nov 2021 21:24
Operator : CG/JU
Sample : PB140896BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140896BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008048.D
Acq On : 19 Nov 2021 21:24
Operator : CG/JU
Sample : PB140896BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB140896BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------