
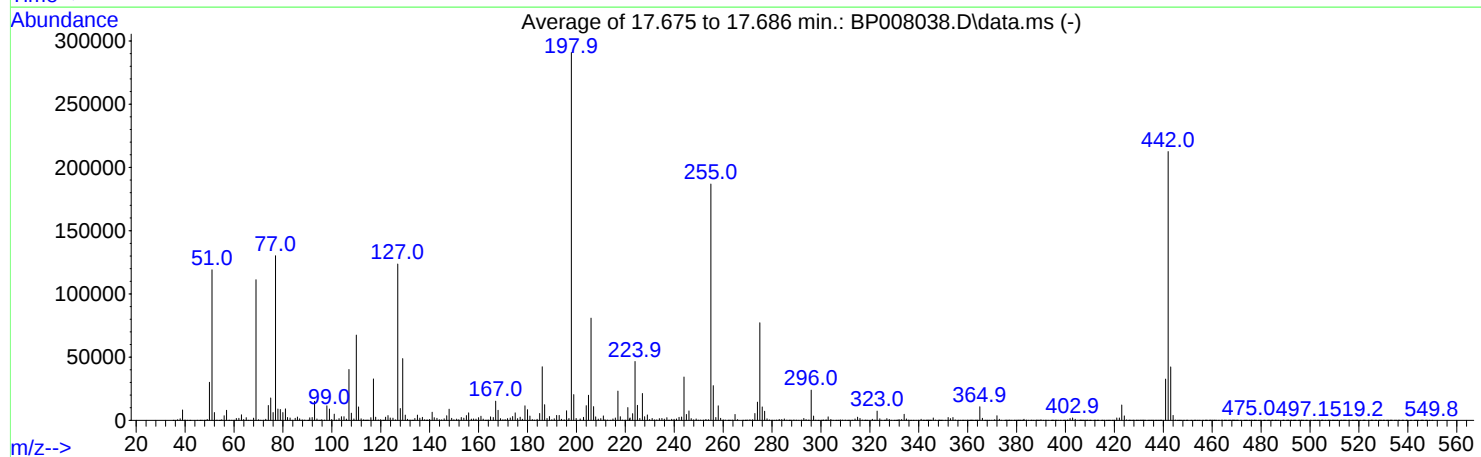


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
 Data File : BP008038.D
 Acq On : 19 Nov 2021 15:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Nov 20 00:21:11 2021

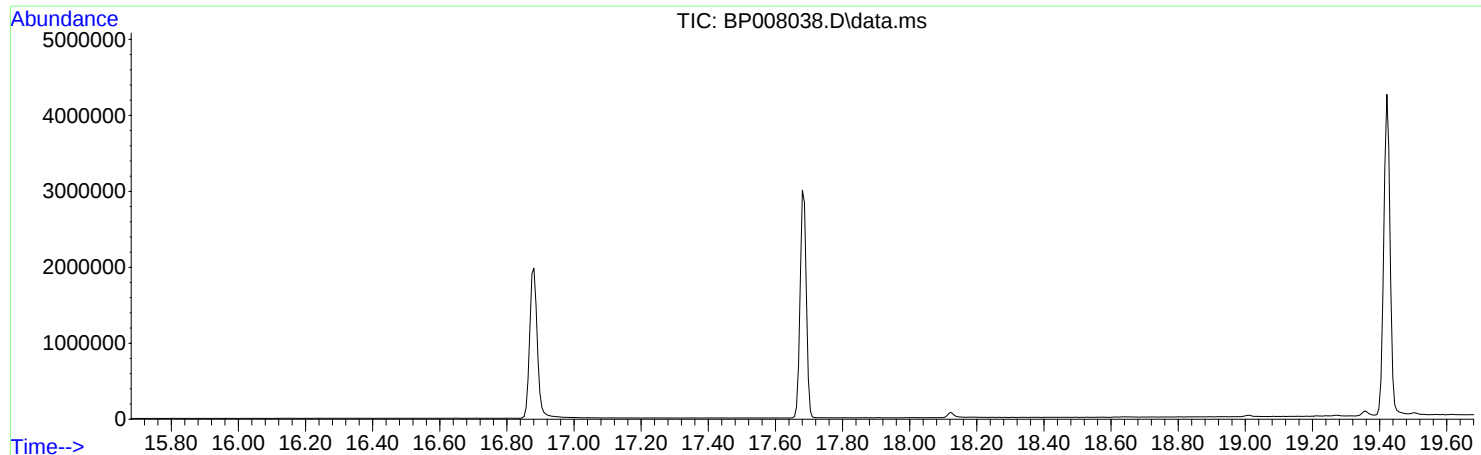


AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	119039	PASS
68	69	0.00	2	1.6	1832	PASS
69	198	0.00	100	38.2	111235	PASS
70	69	0.00	2	0.5	542	PASS
127	198	10	80	42.5	123654	PASS
197	198	0.00	2	0.5	1483	PASS
198	198	100	100	100.0	290901	PASS
199	198	5	9	7.0	20341	PASS
275	198	10	60	26.5	77211	PASS
365	198	1	100	3.7	10820	PASS
441	198	0.01	100	11.2	32682	PASS
442	442	100	100	100.0	212603	PASS
443	442	15	24	19.9	42307	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
Data File : BP008038.D
Acq On : 19 Nov 2021 15:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 20 02:25:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 20 00:21:11 2021
Response via : Initial Calibration

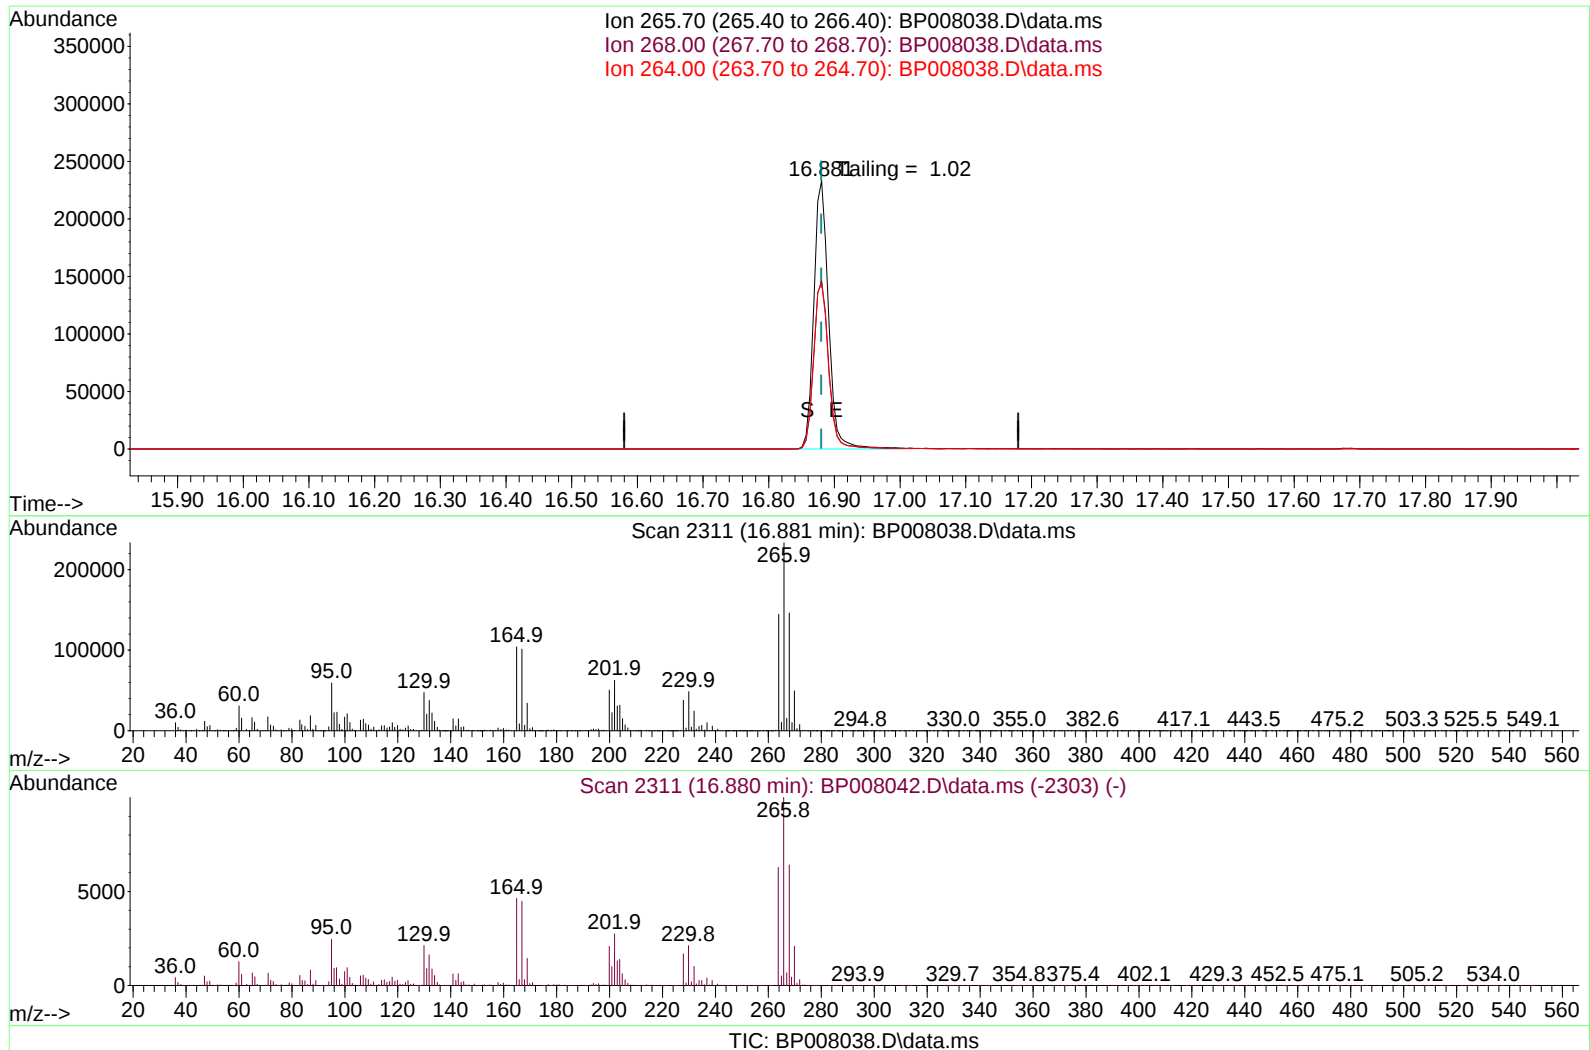

(70) Pentachlorophenol (C)

16.881min (+ 0.001) 929381.98 ng




response 364335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.67
264.00	62.80	61.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111921\
 Data File : BP008038.D
 Acq On : 19 Nov 2021 15:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 20 02:25:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 20 00:21:11 2021
 Response via : Initial Calibration

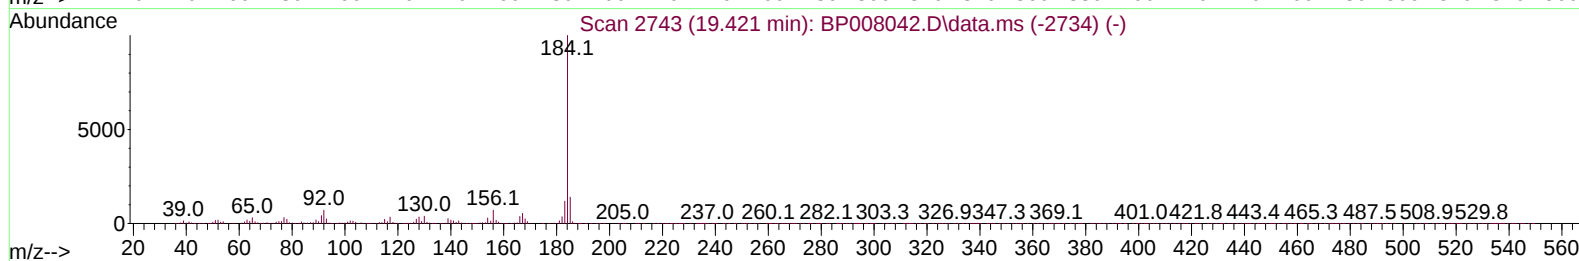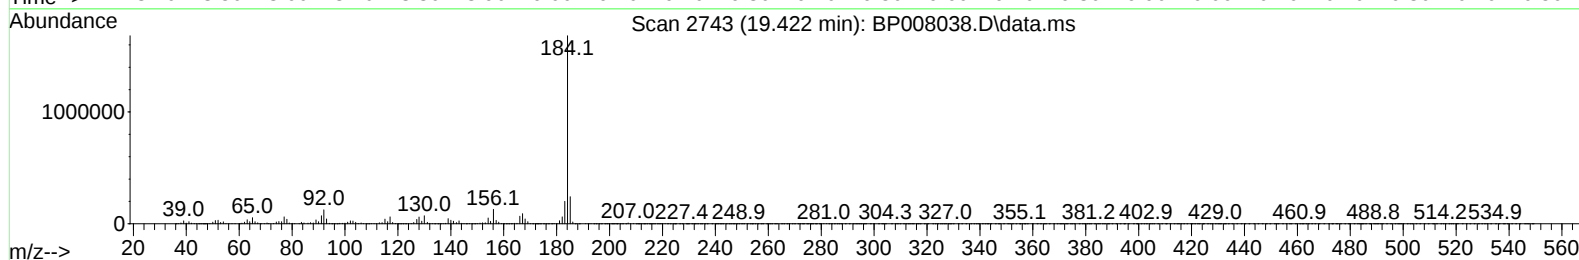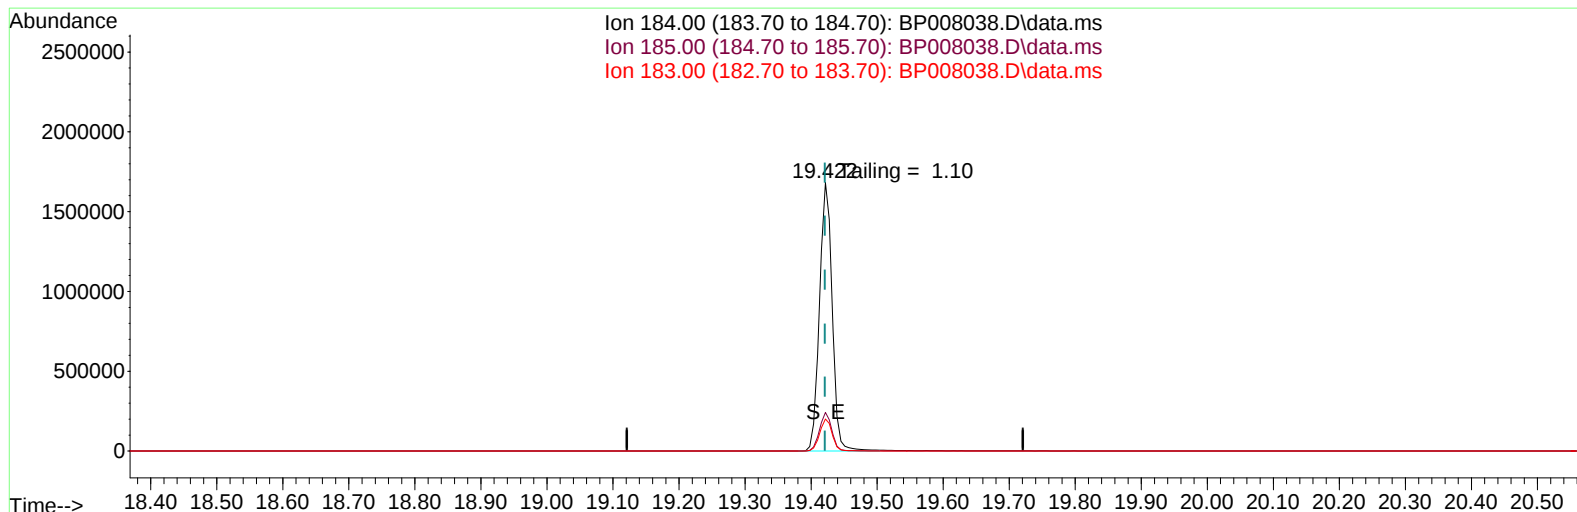

TIC: BP008038.D\data.ms

(77) Benzidine

19.422min (+ 0.001) 492152.46 ng

response 2254000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	11.80	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2021	BNA_P	BP008038.D
Compound Name	Response	Retention Time
DDT	1149369	20.627
DDD	9194	20.245
DDE	1057	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10251	1159620	0.88