
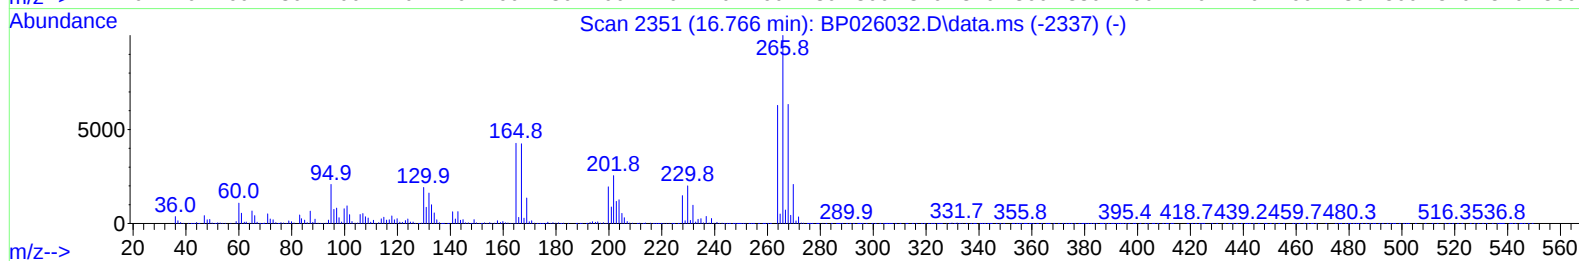
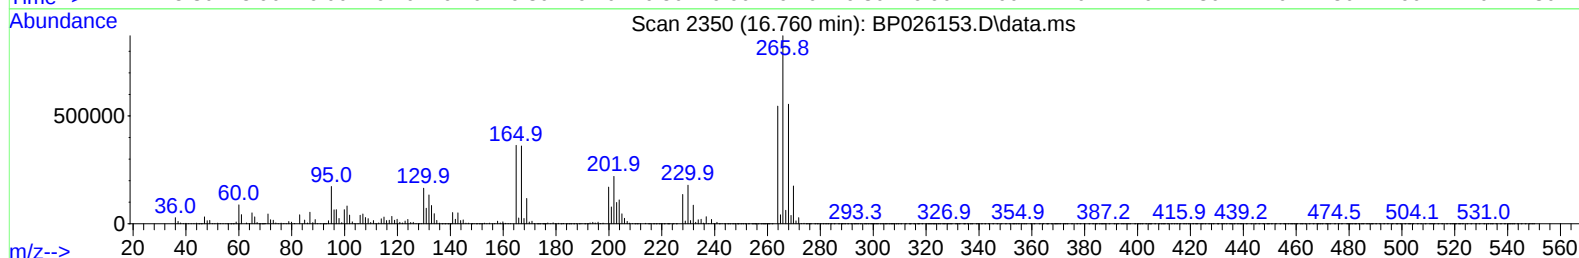


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111925\
Data File : BP026153.D
Acq On : 19 Nov 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 10:25:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

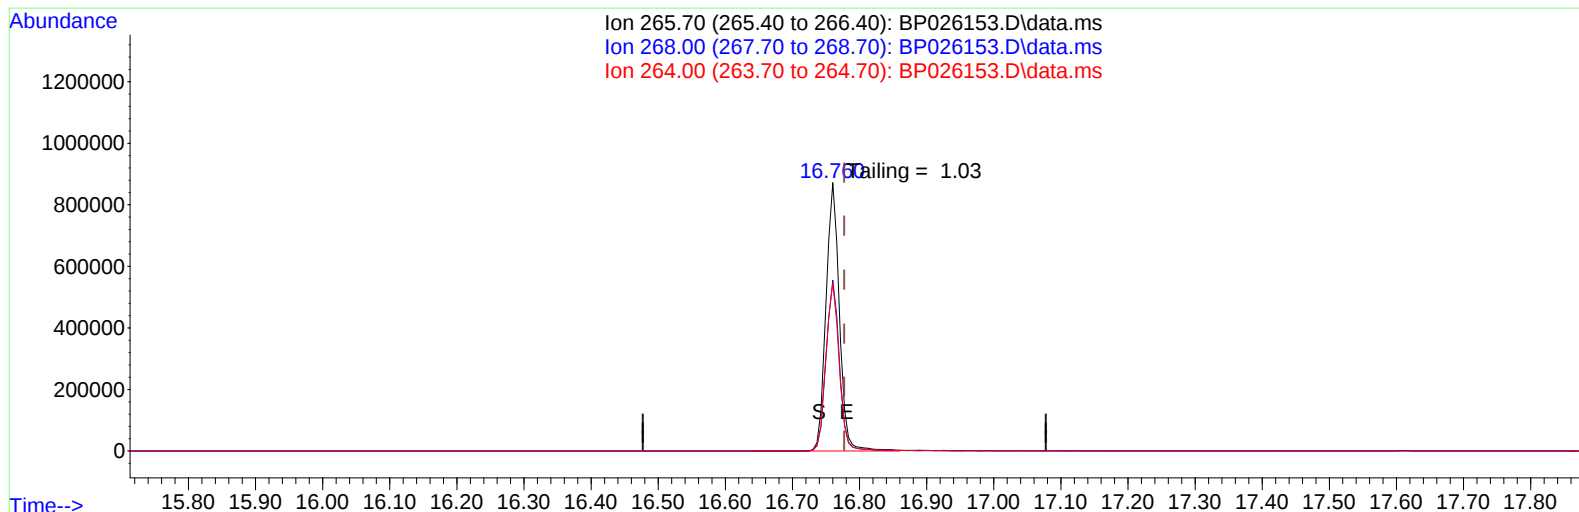

TIC: BP026153.D\data.ms

(70) Pentachlorophenol (C)

16.760min (-0.017) 66392.47 ng

response 1207974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.54
264.00	62.70	62.57
0.00	0.00	0.00

