
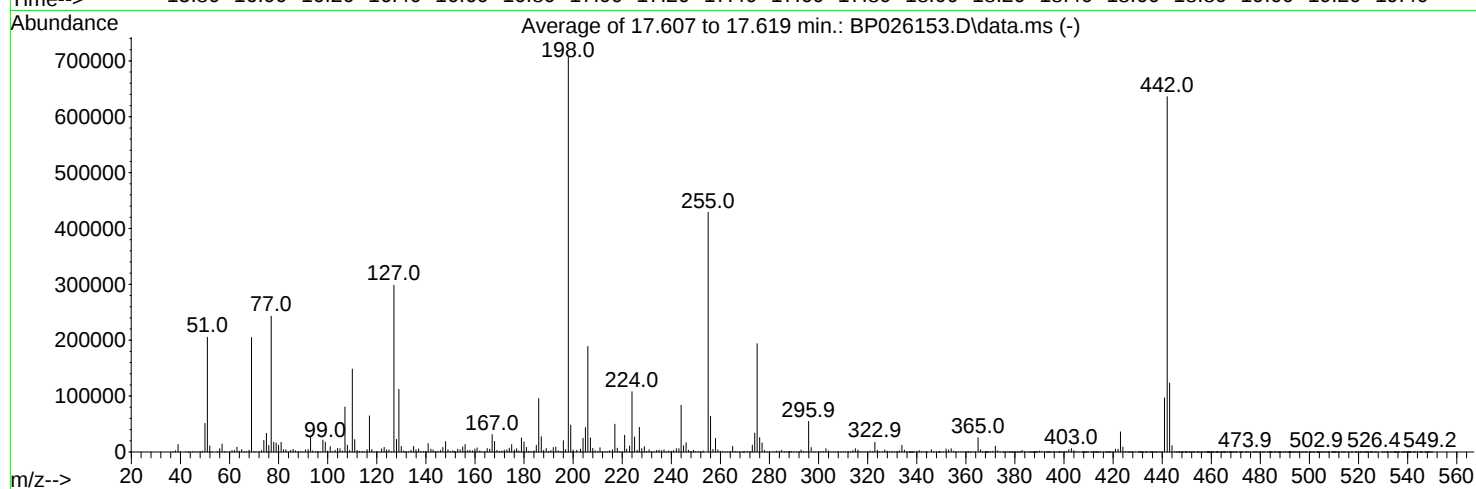


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111925\
Data File : BP026153.D
Acq On : 19 Nov 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

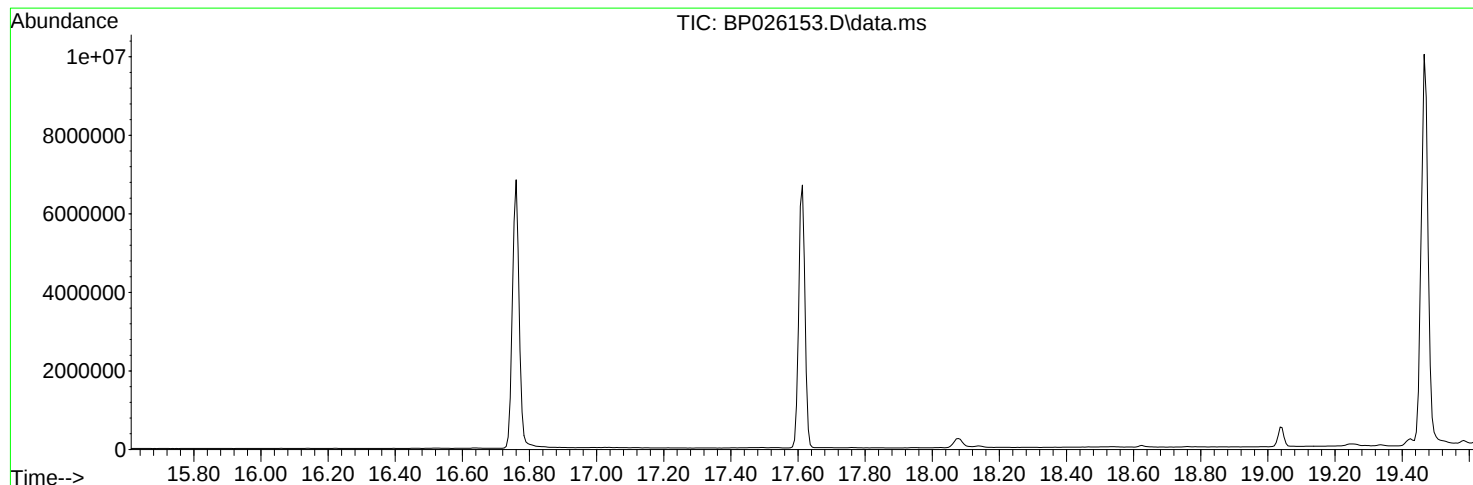




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3423	PASS
69	69	100	100	100.0	204759	PASS
70	69	0.00	2	0.4	889	PASS
197	198	0.00	2	0.6	4032	PASS
198	198	100	100	100.0	706781	PASS
199	198	5	9	6.8	48083	PASS
365	198	1	100	3.6	25485	PASS
441	443	0.01	150	78.4	96711	PASS
442	442	100	100	100.0	636053	PASS
443	442	15	24	19.4	123328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111925\
Data File : BP026153.D
Acq On : 19 Nov 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 19 10:25:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

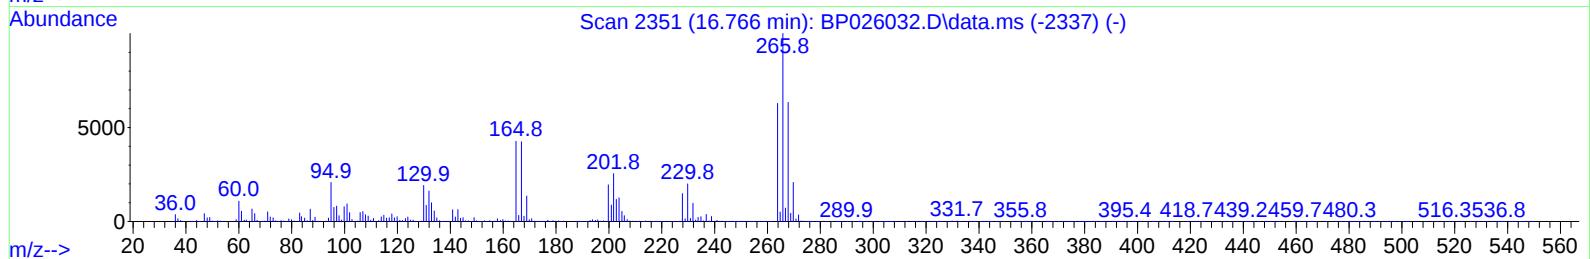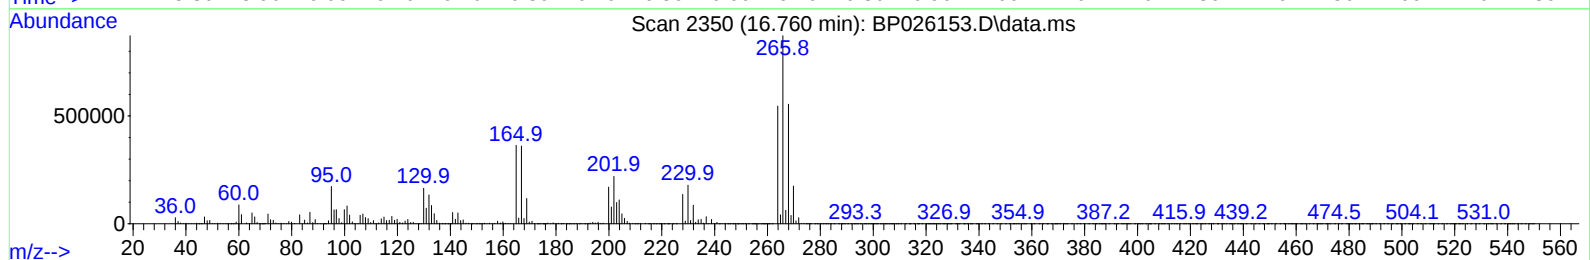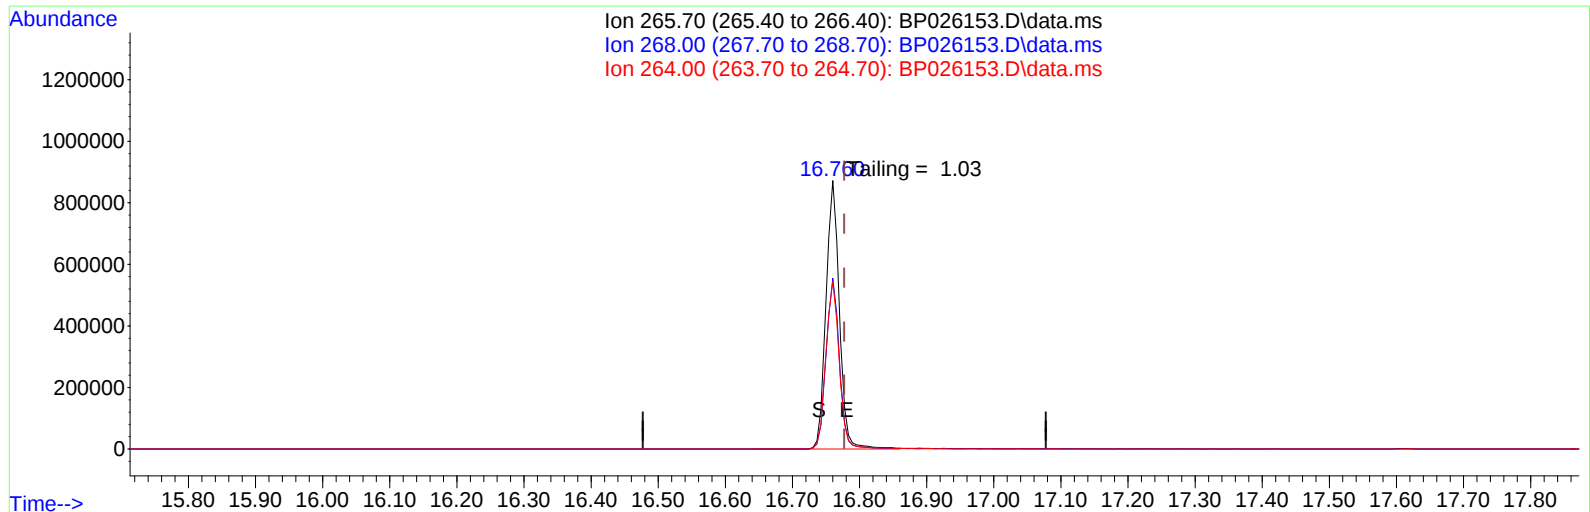

TIC: BP026153.D\data.ms

(70) Pentachlorophenol (C)

16.760min (-0.017) 66392.47 ng




response 1207974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.54
264.00	62.70	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111925\
Data File : BP026153.D
Acq On : 19 Nov 2025 10:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 19 10:25:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

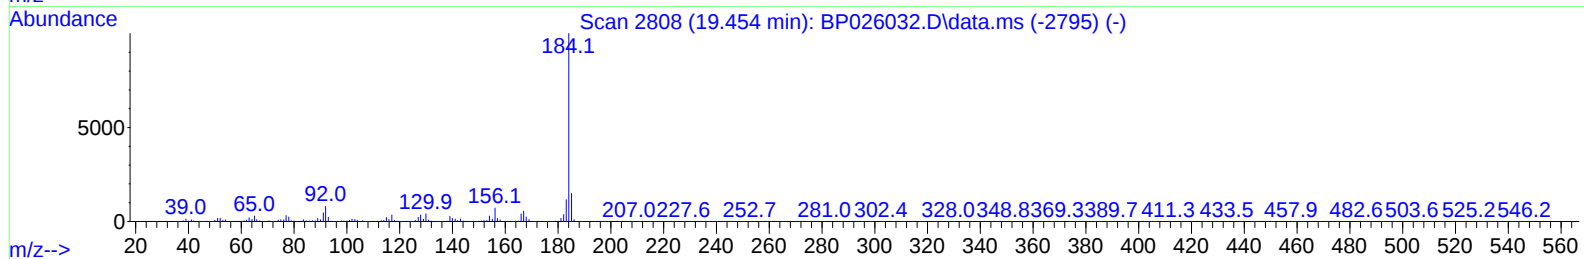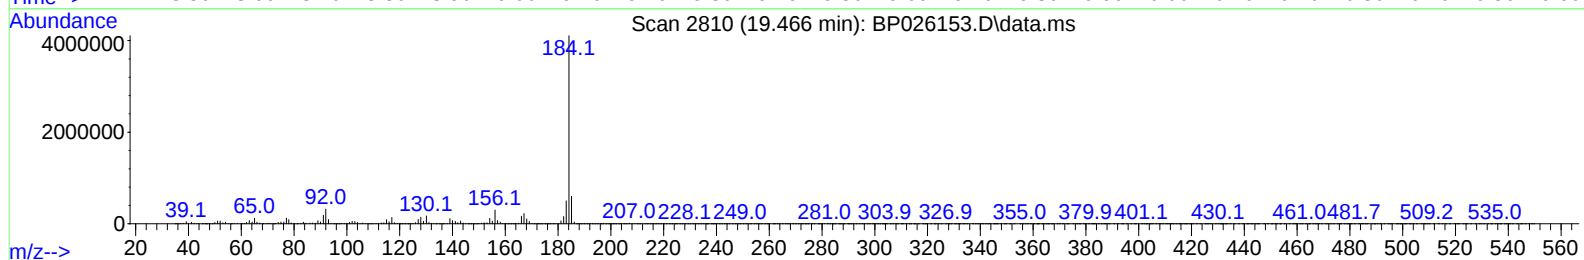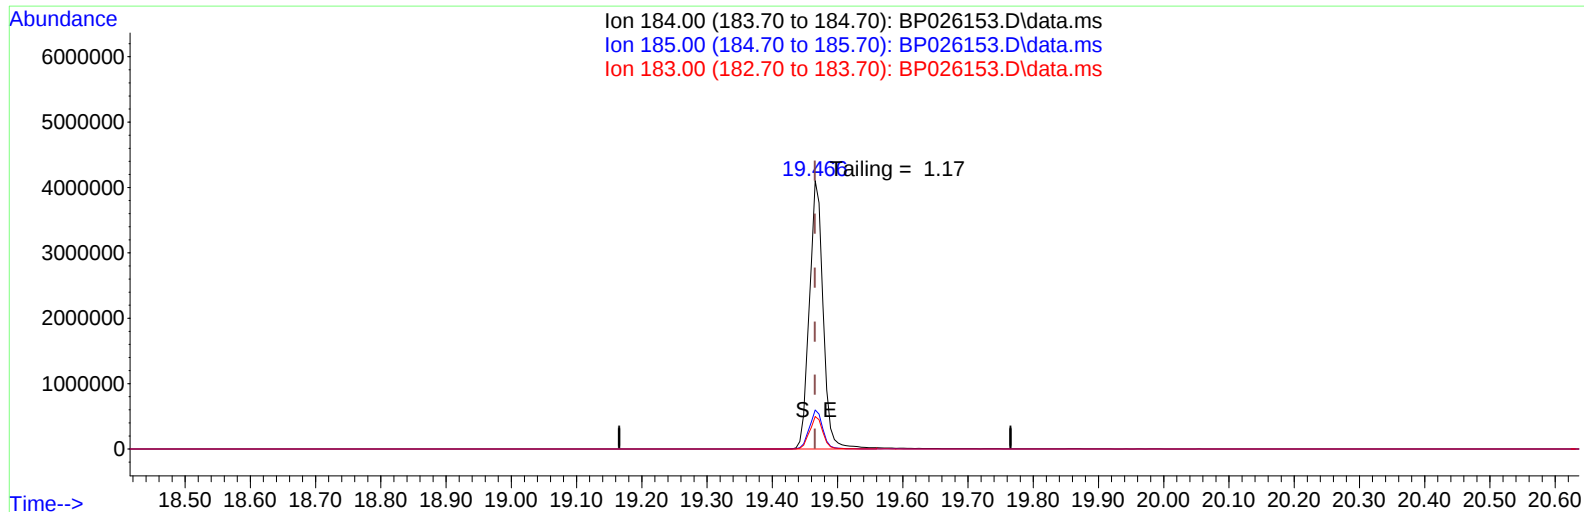

TIC: BP026153.D\data.ms

(77) Benzidine

19.466min (+ 0.000) 1840.91 ng

response 6080695

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.56
183.00	11.30	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/19/2025	BNA_P	<u>BP026153.D</u>
Compound Name	Response	Retention Time
DDT	3033284	20.772
DDD	33941	20.307
DDE	6635	19.866
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40576	3073860	1.32

Instrument :
BNA_P
ClientSampleId :
DFTPP