

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
 Data File : BP026176.D
 Acq On : 20 Nov 2025 15:57
 Operator : RC/JU
 Sample : Q3678-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COMPOSITE-STONE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.825	315	321	335	rVB	847827	1197642	13.97%	2.151%
2	5.284	392	399	412	rBV	3407274	4946840	57.69%	8.883%
3	5.743	472	477	482	rBV	68140	101194	1.18%	0.182%
4	6.843	657	664	678	rBV	3116452	4907472	57.23%	8.813%
5	7.666	796	804	812	rBV	1094970	1783668	20.80%	3.203%
6	8.802	989	997	1010	rBV	1948347	3139326	36.61%	5.637%
7	10.431	1266	1274	1282	rBV	1451460	2380424	27.76%	4.275%
8	12.913	1688	1696	1710	rBV	4300882	6970568	81.29%	12.517%
9	14.307	1926	1933	1943	rBV	1682148	2875267	33.53%	5.163%
10	15.701	2164	2170	2178	rBV	269326	368224	4.29%	0.661%
11	15.819	2184	2190	2204	rBV	3067827	4577469	53.38%	8.220%
12	17.125	2406	2412	2421	rBV	2303210	3039279	35.44%	5.458%
13	17.548	2480	2484	2490	rBV2	75509	109878	1.28%	0.197%
14	18.083	2569	2575	2588	rBV	395851	724064	8.44%	1.300%
15	18.536	2648	2652	2656	rBV2	112839	128073	1.49%	0.230%
16	19.289	2777	2780	2787	rVB4	62436	91918	1.07%	0.165%
17	19.425	2798	2803	2809	rBV2	168441	256839	3.00%	0.461%
18	19.872	2872	2879	2888	rBV	5980046	8574740	100.00%	15.398%
19	20.430	2970	2974	2982	rBV	309852	408710	4.77%	0.734%
20	20.701	3017	3020	3025	rBV4	80372	109629	1.28%	0.197%
21	21.201	3101	3105	3111	rBV2	166779	269589	3.14%	0.484%
22	21.266	3112	3116	3123	rBV2	280724	469338	5.47%	0.843%
23	21.572	3163	3168	3176	rBV	2295522	3491040	40.71%	6.269%
24	23.442	3482	3486	3495	rVB2	246218	492500	5.74%	0.884%
25	24.901	3725	3734	3747	rVB	1507439	4273417	49.84%	7.674%




Sum of corrected areas: 55687108

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026176.D
Acq On : 20 Nov 2025 15:57
Operator : RC/JU
Sample : Q3678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMPOSITE-STONE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

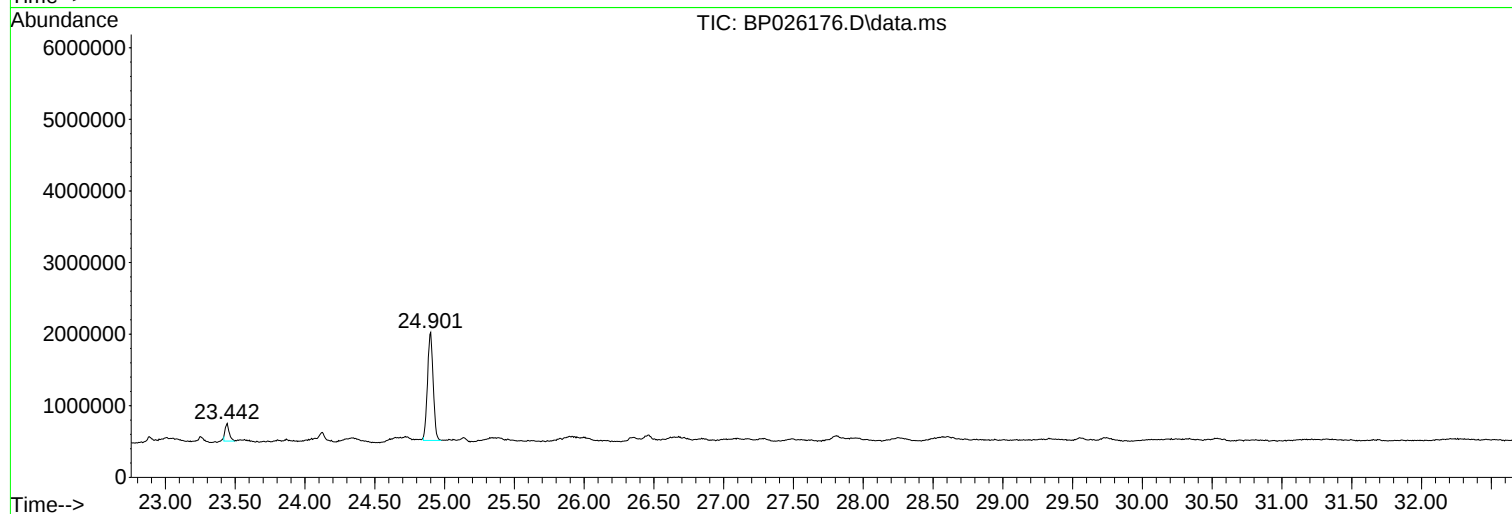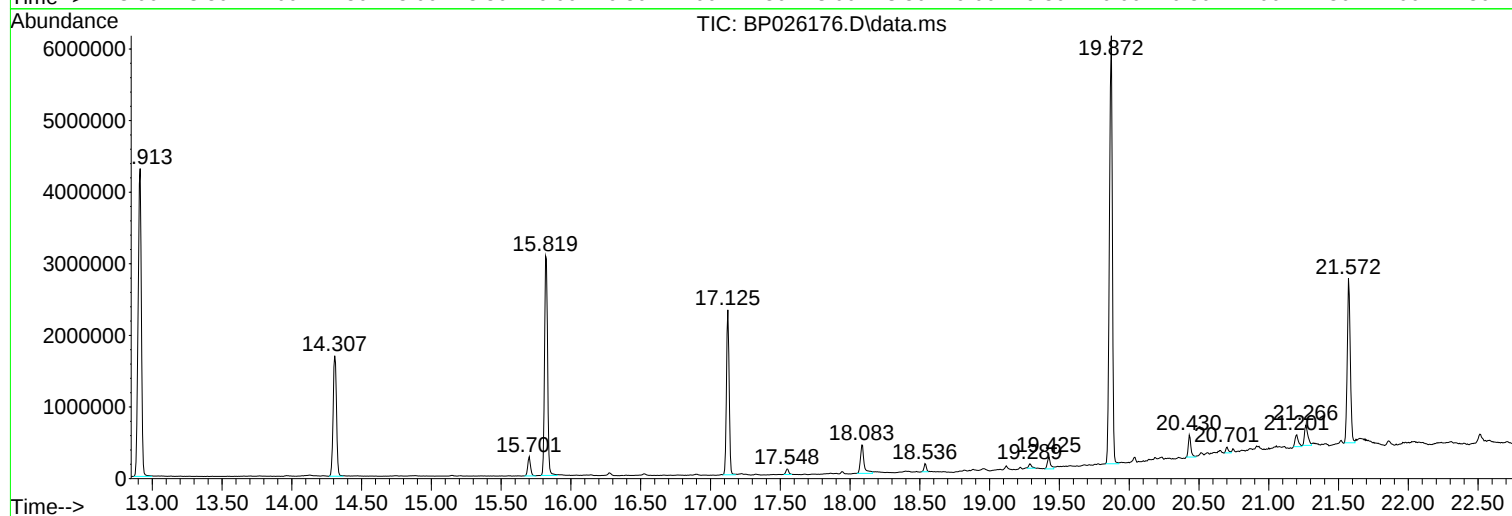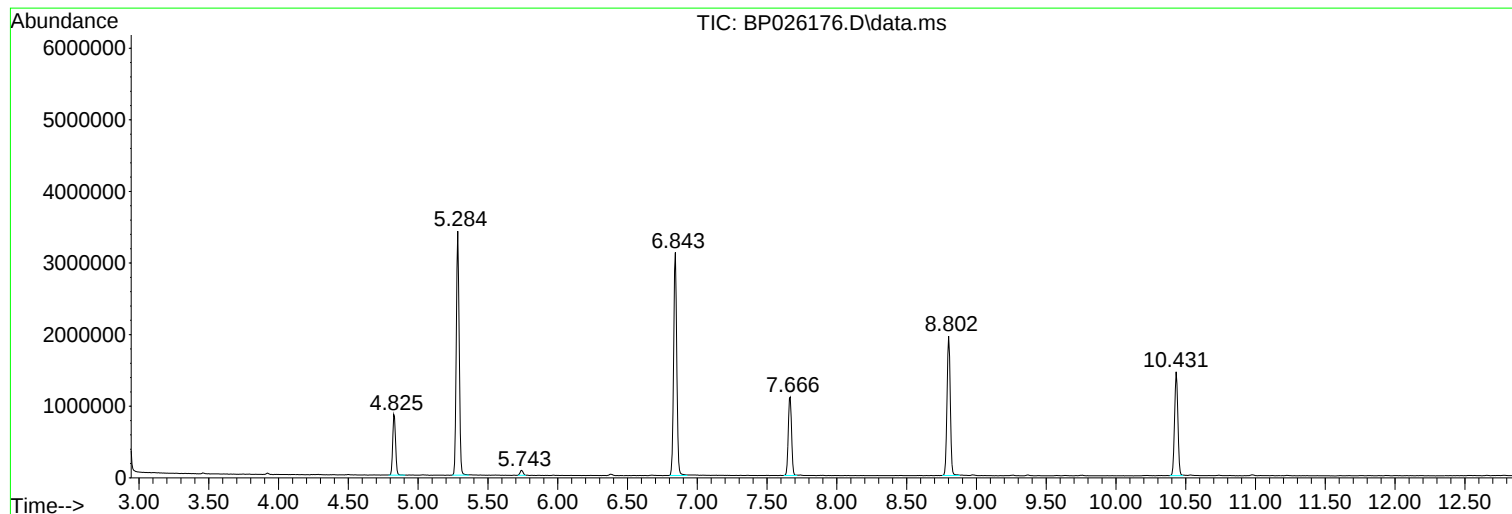

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026176.D
Acq On : 20 Nov 2025 15:57
Operator : RC/JU
Sample : Q3678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMPOSITE-STONE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026176.D
Acq On : 20 Nov 2025 15:57
Operator : RC/JU
Sample : Q3678-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COMPOSITE-STONE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc