


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026167.D
Acq On : 20 Nov 2025 09:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

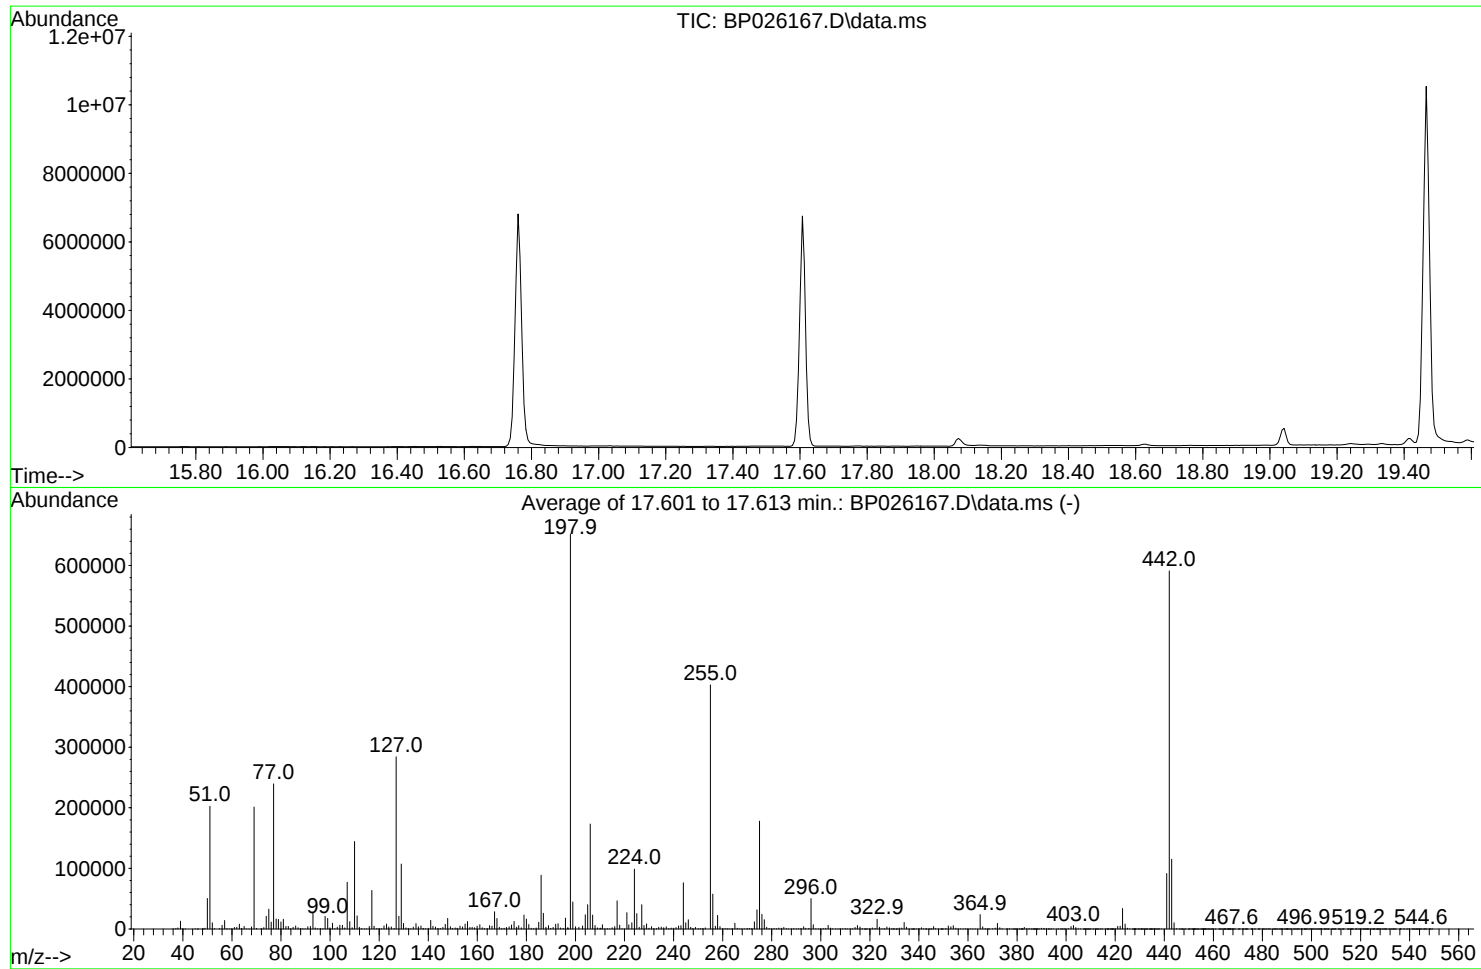




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	3369	PASS
69	69	100	100	100.0	201104	PASS
70	69	0.00	2	0.5	909	PASS
197	198	0.00	2	0.3	2042	PASS
198	198	100	100	100.0	651830	PASS
199	198	5	9	6.8	44554	PASS
365	198	1	100	3.6	23728	PASS
441	443	0.01	150	79.7	91677	PASS
442	442	100	100	100.0	590955	PASS
443	442	15	24	19.5	115061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026167.D
Acq On : 20 Nov 2025 09:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 20 09:56:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

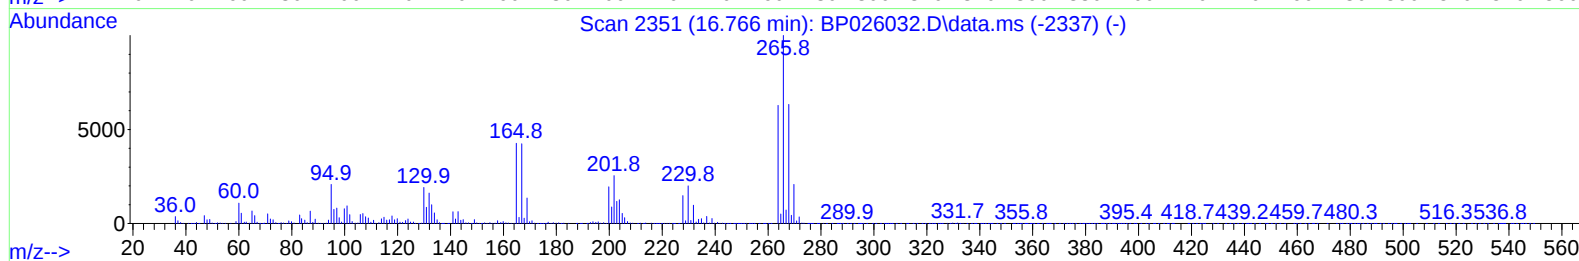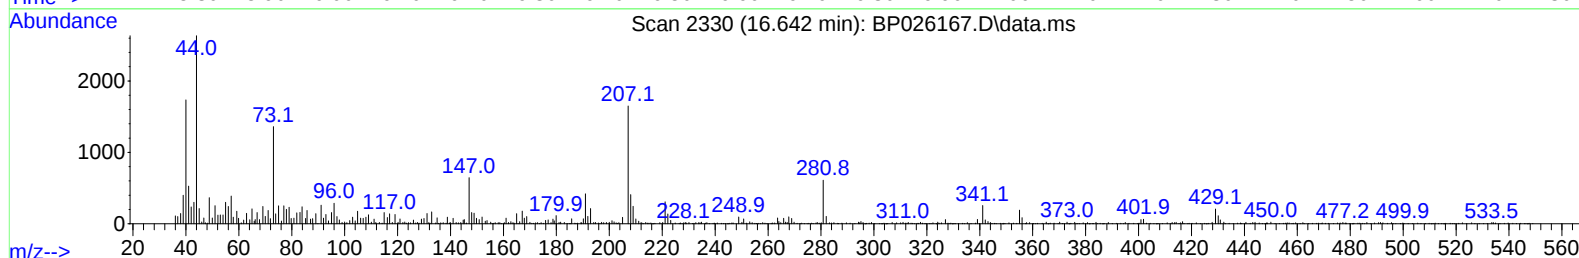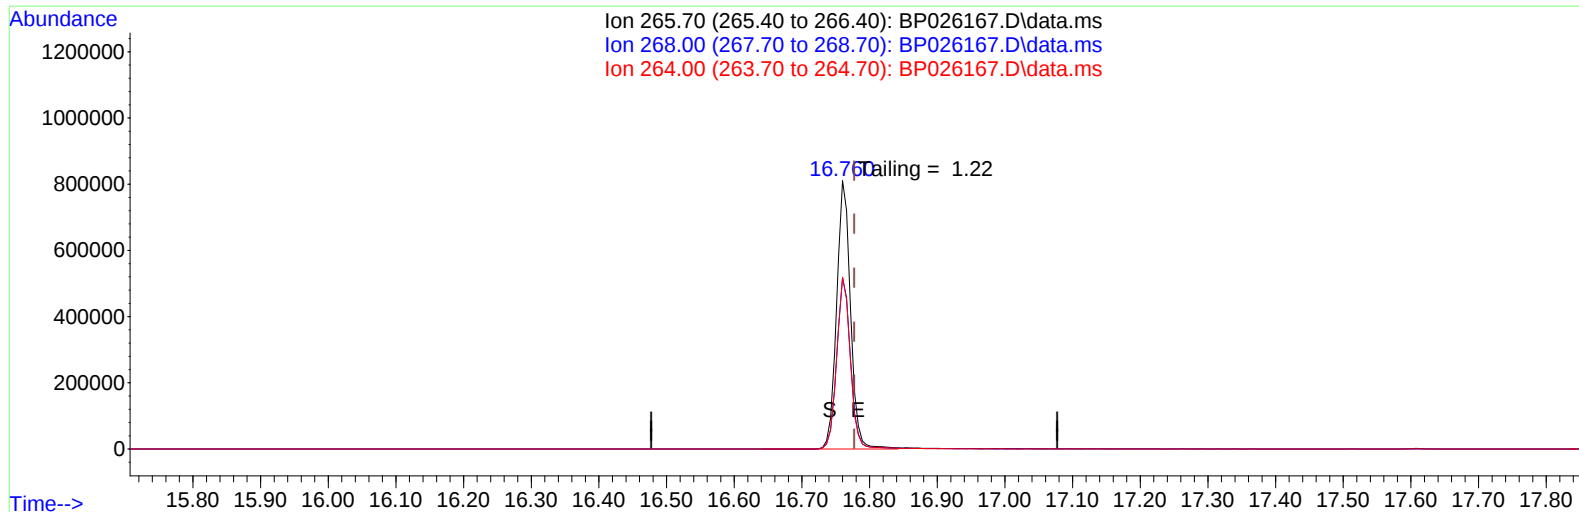

TIC: BP026167.D\data.ms

(70) Pentachlorophenol (C)

16.760min (-0.017) 1011900.89 ng




response 1155234

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.97
264.00	62.70	63.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112025\
Data File : BP026167.D
Acq On : 20 Nov 2025 09:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 20 09:56:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

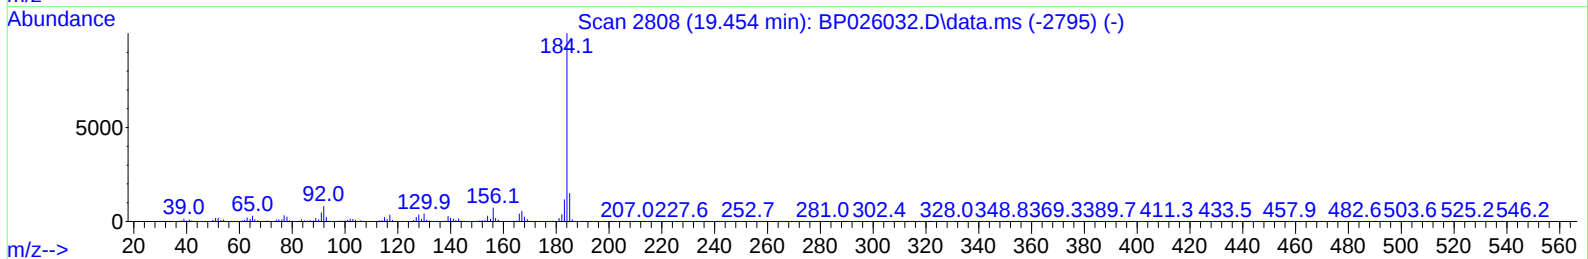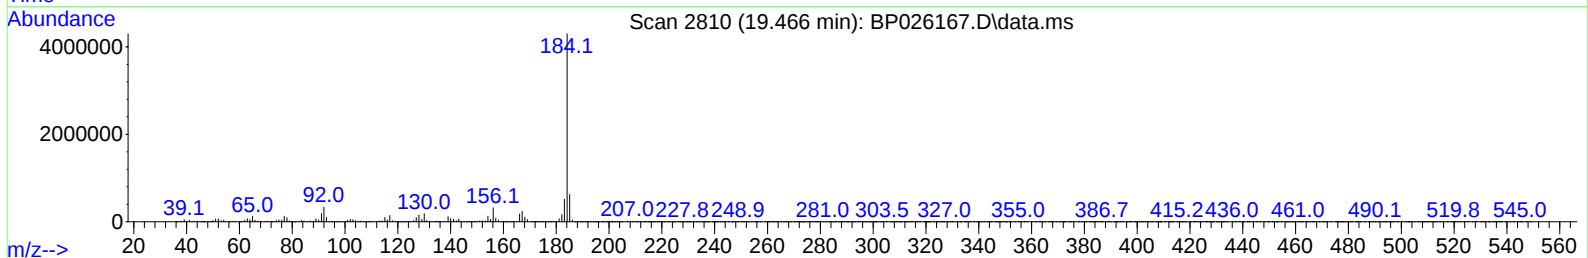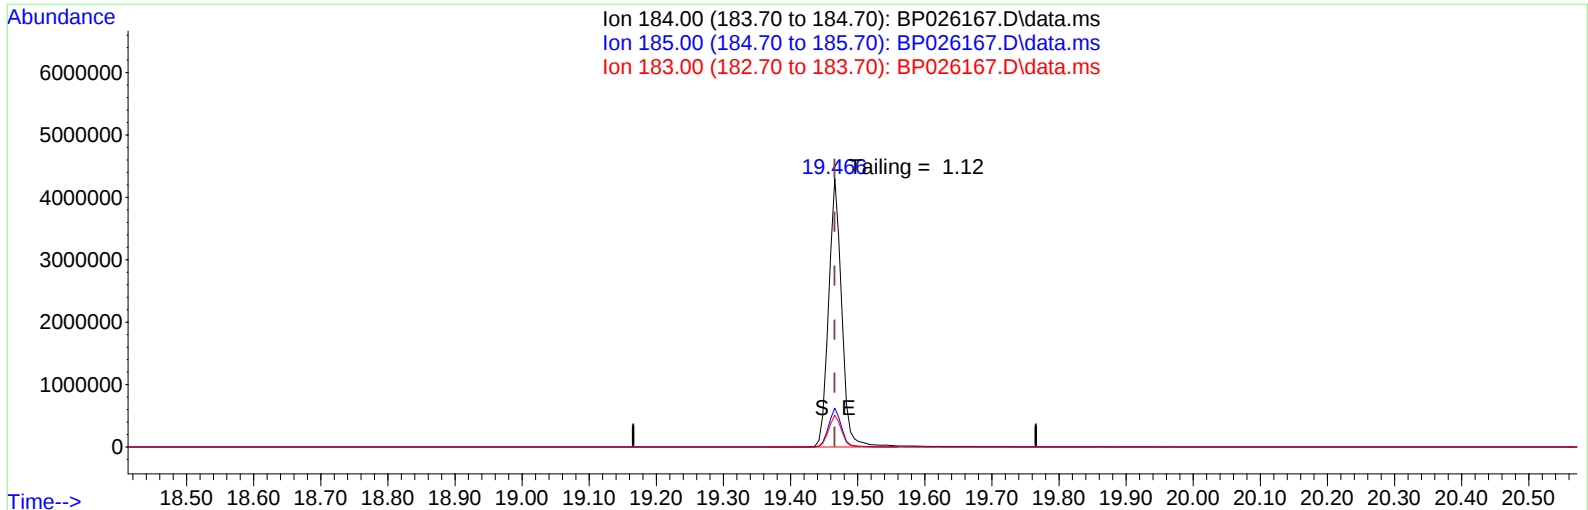

TIC: BP026167.D\data.ms

(77) Benzidine

19.466min (+ 0.000) 1941.39 ng

response 5856650

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.51
183.00	11.30	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/20/2025	BNA_P	<u>BP026167.D</u>
Compound Name	Response	Retention Time
DDT	2907150	20.772
DDD	28938	20.313
DDE	363	19.419
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29301	2936451	1.00

Instrument :
BNA_P
ClientSampleId :
DFTPP