
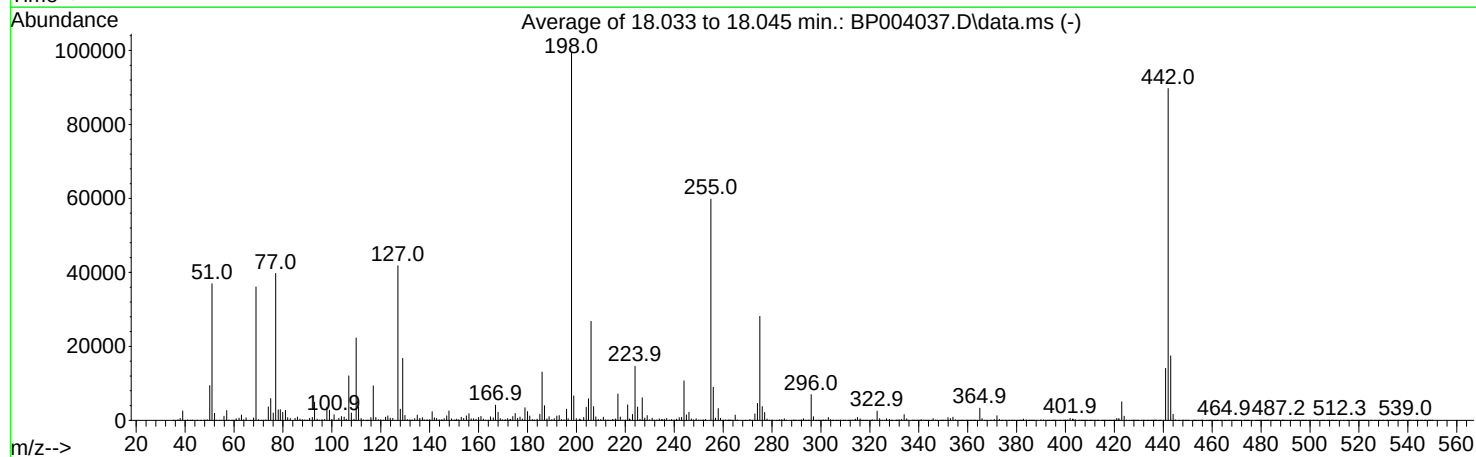


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112120\
 Data File : BP004037.D
 Acq On : 21 Nov 2020 14:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 23 03:48:44 2020

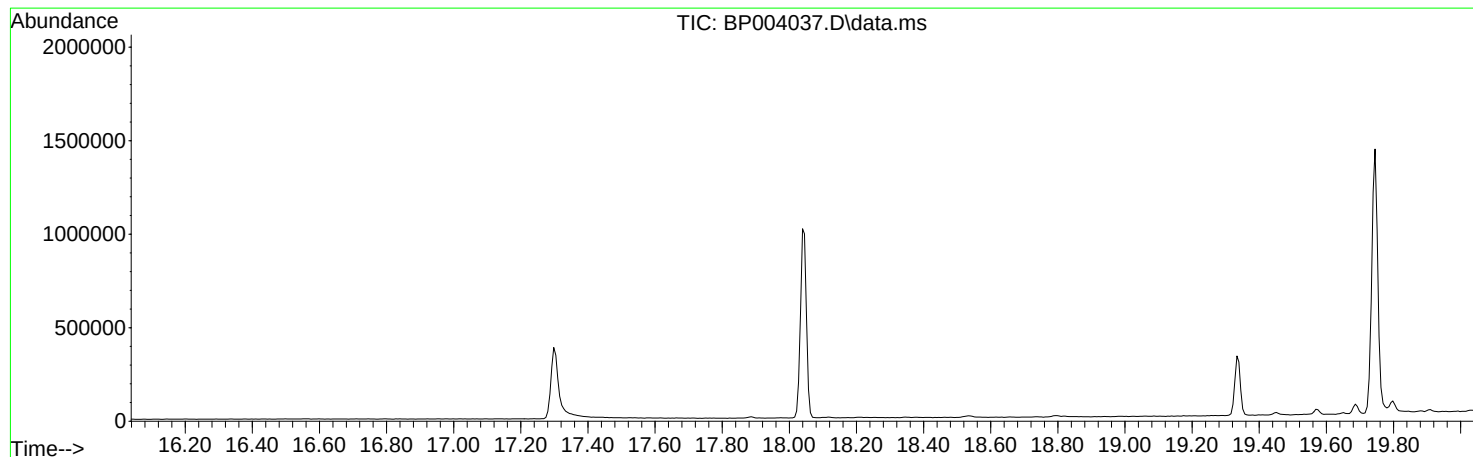

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	36947	PASS
68	69	0.00	2	1.8	646	PASS
69	198	0.00	100	36.3	36091	PASS
70	69	0.00	2	0.5	183	PASS
127	198	10	80	42.0	41799	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99451	PASS
199	198	5	9	6.7	6630	PASS
275	198	10	60	28.3	28106	PASS
365	198	1	100	3.3	3282	PASS
441	198	0.01	100	14.1	14049	PASS
442	442	100	100	100.0	89728	PASS
443	442	15	24	19.4	17436	PASS