
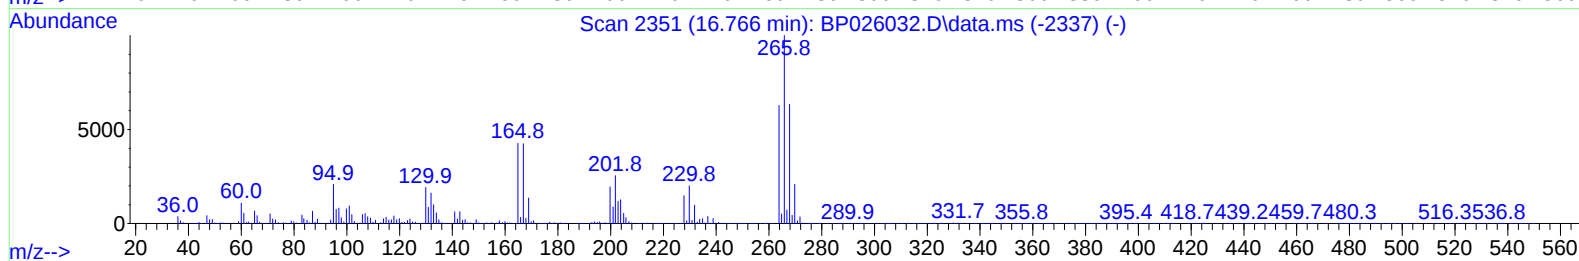
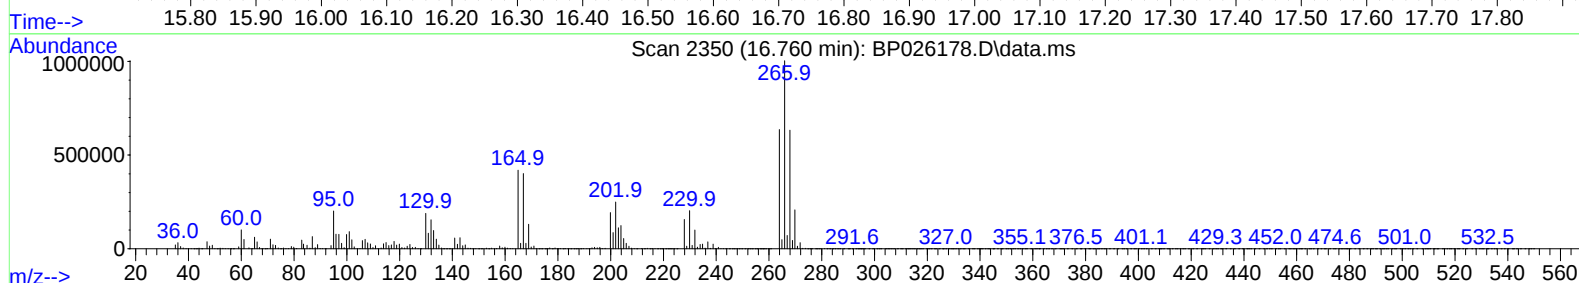


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112125\
Data File : BP026178.D
Acq On : 21 Nov 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 10:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

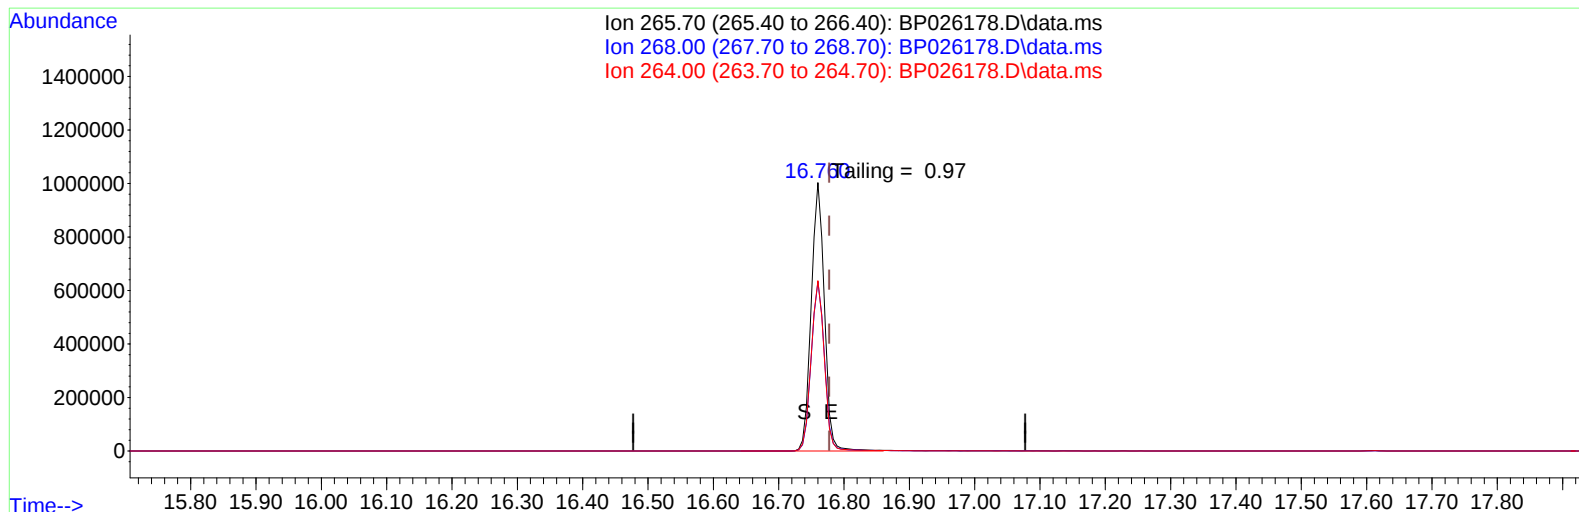

TIC: BP026178.D\data.ms

(70) Pentachlorophenol (C)




16.760min (-0.017) 379922.49 ng

response 1413916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.07
264.00	62.70	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112125\
Data File : BP026178.D
Acq On : 21 Nov 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 10:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

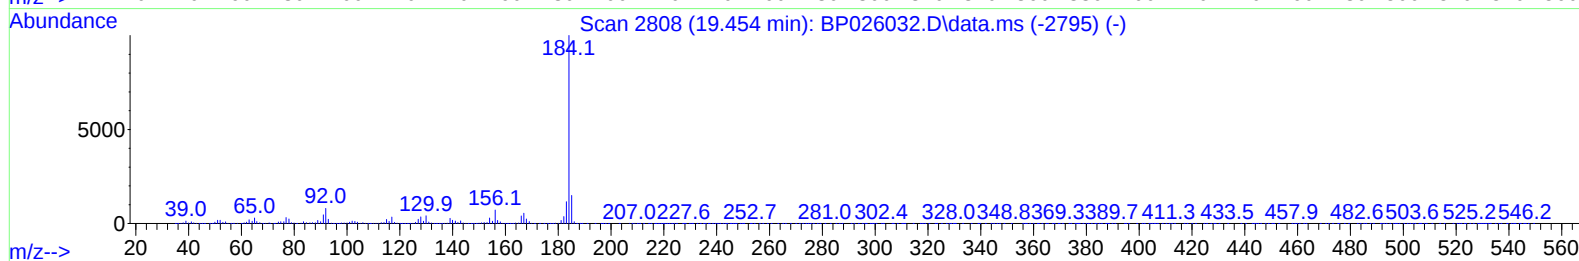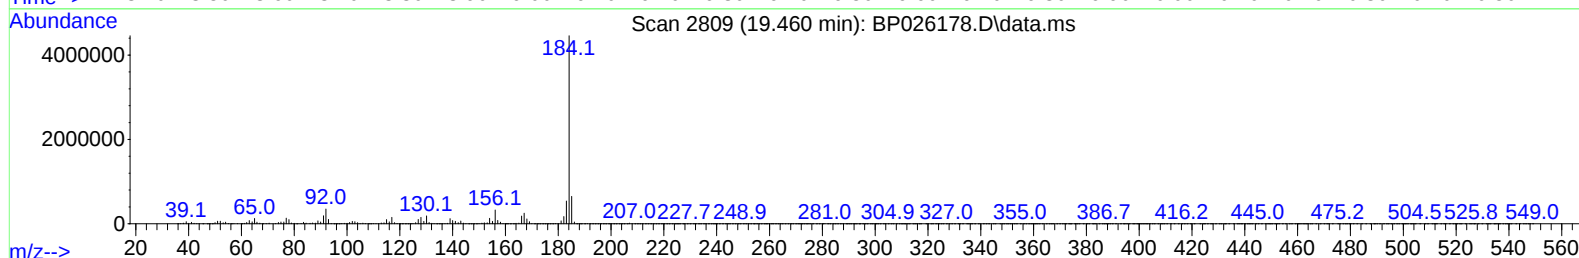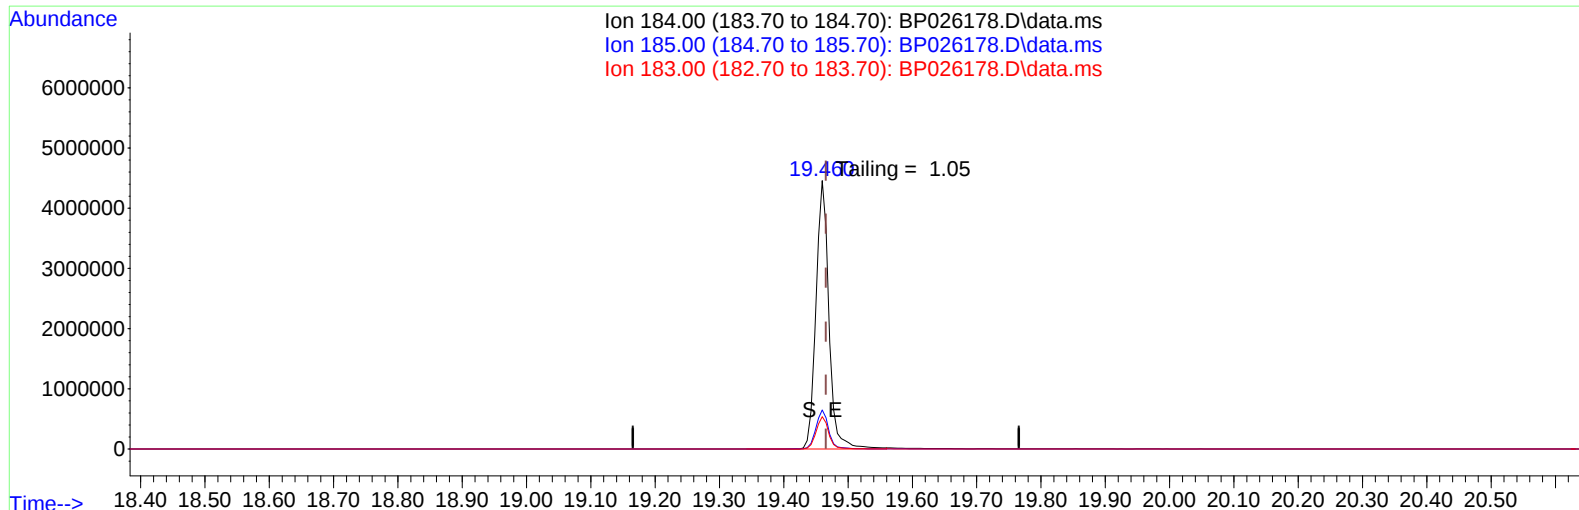

TIC: BP026178.D\data.ms

(77) Benzidine

19.460min (-0.006) 2279.03 ng

response 6316206

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.56
183.00	11.30	12.08
0.00	0.00	0.00