


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112125\
Data File : BP026178.D
Acq On : 21 Nov 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 19 01:25:31 2025

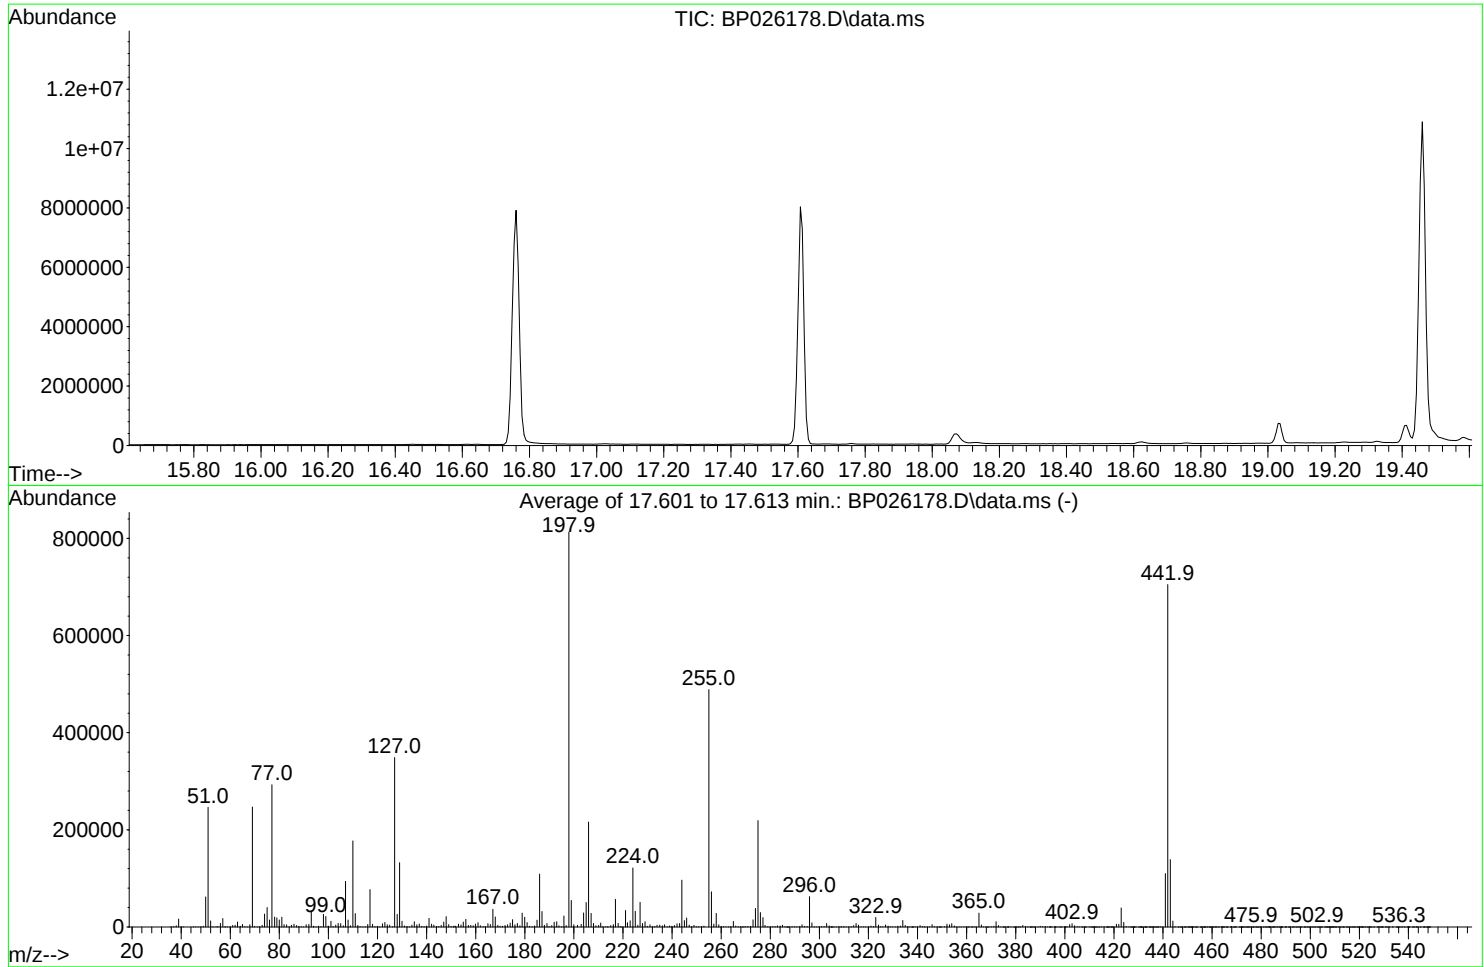


AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	4495	PASS
69	69	100	100	100.0	247056	PASS
70	69	0.00	2	0.5	1120	PASS
197	198	0.00	2	0.3	2705	PASS
198	198	100	100	100.0	813018	PASS
199	198	5	9	6.7	54583	PASS
365	198	1	100	3.5	28504	PASS
441	443	0.01	150	79.2	109796	PASS
442	442	100	100	100.0	704806	PASS
443	442	15	24	19.7	138547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112125\
Data File : BP026178.D
Acq On : 21 Nov 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 21 10:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

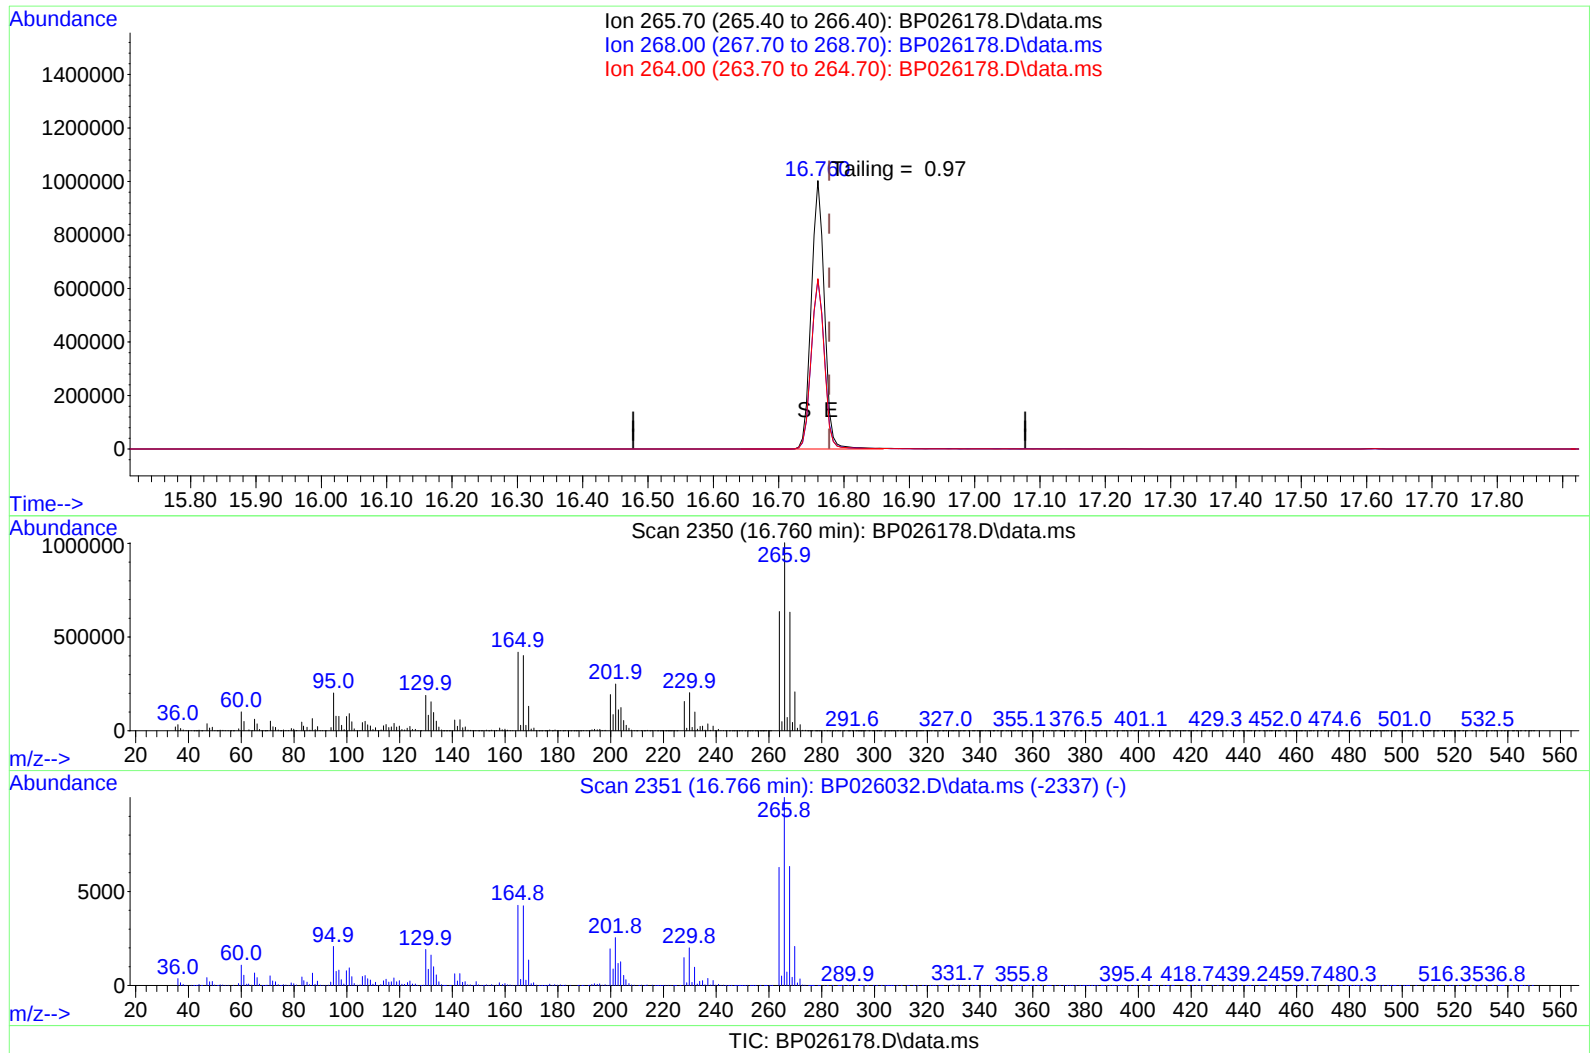

(70) Pentachlorophenol (C)

16.760min (-0.017) 379922.49 ng




response 1413916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.07
264.00	62.70	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112125\
Data File : BP026178.D
Acq On : 21 Nov 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Nov 21 10:05:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration

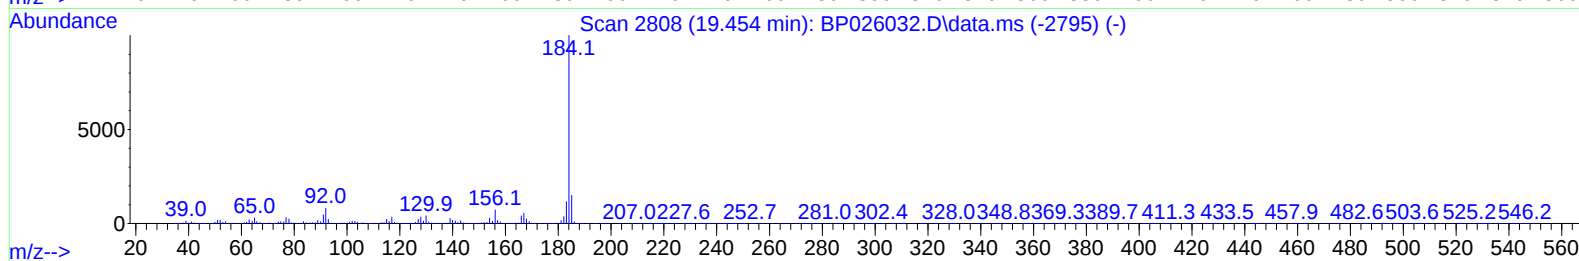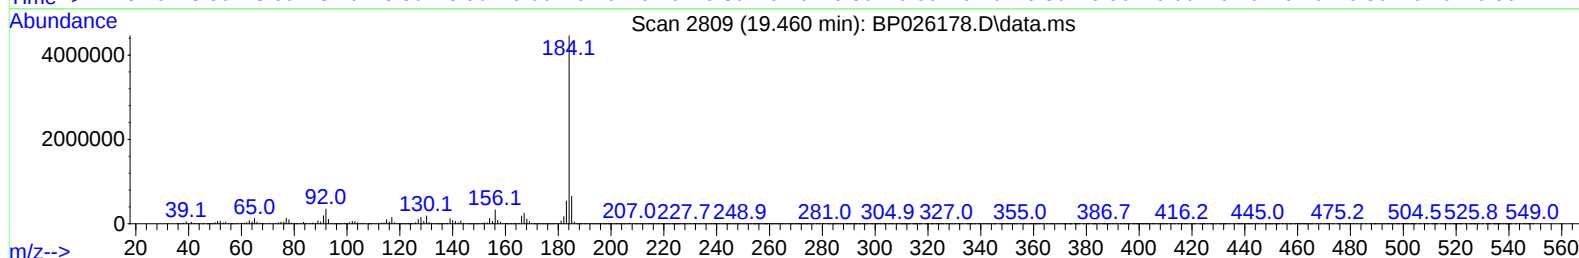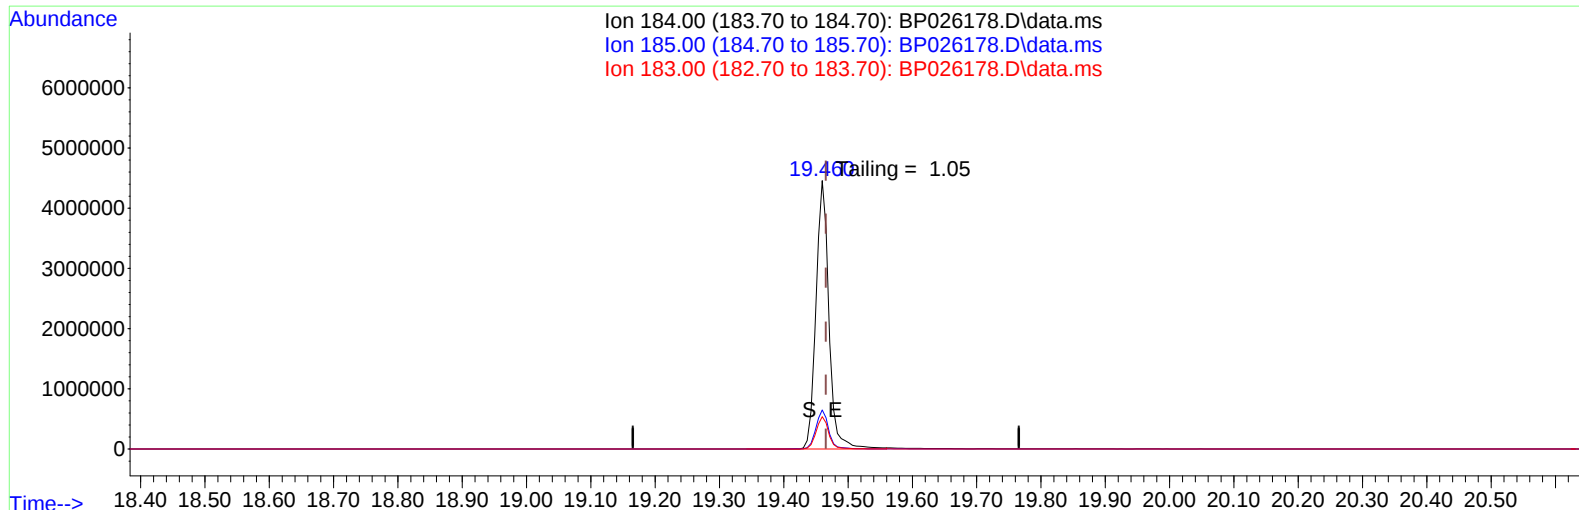

TIC: BP026178.D\data.ms

(77) Benzidine

19.460min (-0.006) 2279.03 ng

response 6316206

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.56
183.00	11.30	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2025	BNA_P	<u>BP026178.D</u>
Compound Name	Response	Retention Time
DDT	3217760	20.76
DDD	42151	20.307
DDE	3096	19.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45247	3263007	1.39

Instrument :
BNA_P
ClientSampleId :
DFTPP