

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018293.D
 Acq On : 23 Nov 2023 01:25
 Operator : MA/JU
 Sample : 05226-22
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG83

Quant Time: Nov 23 02:02:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 22 14:09:55 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	418996	20.000	ng/u1	0.00
20) Naphthalene-d8	10.675	136	1766179	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.504	164	1125942	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.257	188	2183924	20.000	ng/u1	0.00
79) Chrysene-d12	21.357	240	1315168	20.000	ng/u1	0.00
88) Perylene-d12	23.780	264	1406911	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	42288	3.780	ng/uL	0.00
4) Pyridine-d5	3.693	84	89367	2.907	ng/u1	0.00
7) Phenol-d5	7.034	99	283804	7.412	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	663639	28.983	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	656030	20.405	ng/u1	0.00
15) 4-Methylphenol-d8	8.581	113	451341	14.605	ng/u1	0.00
21) Nitrobenzene-d5	9.034	128	419441	29.238	ng/u1	0.00
24) 2-Nitrophenol-d4	9.757	143	365257	27.569	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	763074	23.873	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	683948	15.865	ng/u1	0.00
46) Dimethylphthalate-d6	13.922	166	3058105	30.524	ng/u1	-0.01
49) Acenaphthylene-d8	14.198	160	3299607	28.904	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	71943	5.202	ng/u1	-0.01
60) Fluorene-d10	15.498	176	2487512	29.685	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	220688	23.738	ng/u1	0.00
73) Anthracene-d10	17.357	188	3670734	31.446	ng/u1	0.00
81) Pyrene-d10	19.592	212	3511952	33.552	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.621	264	2625071	32.183	ng/u1	0.00
Target Compounds						
80) Fluoranthene	19.269	202	131017	1.048	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018293.D
Acq On : 23 Nov 2023 01:25
Operator : MA/JU
Sample : 05226-22
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG83

Quant Time: Nov 23 02:02:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 22 14:09:55 2023
Response via : Initial Calibration

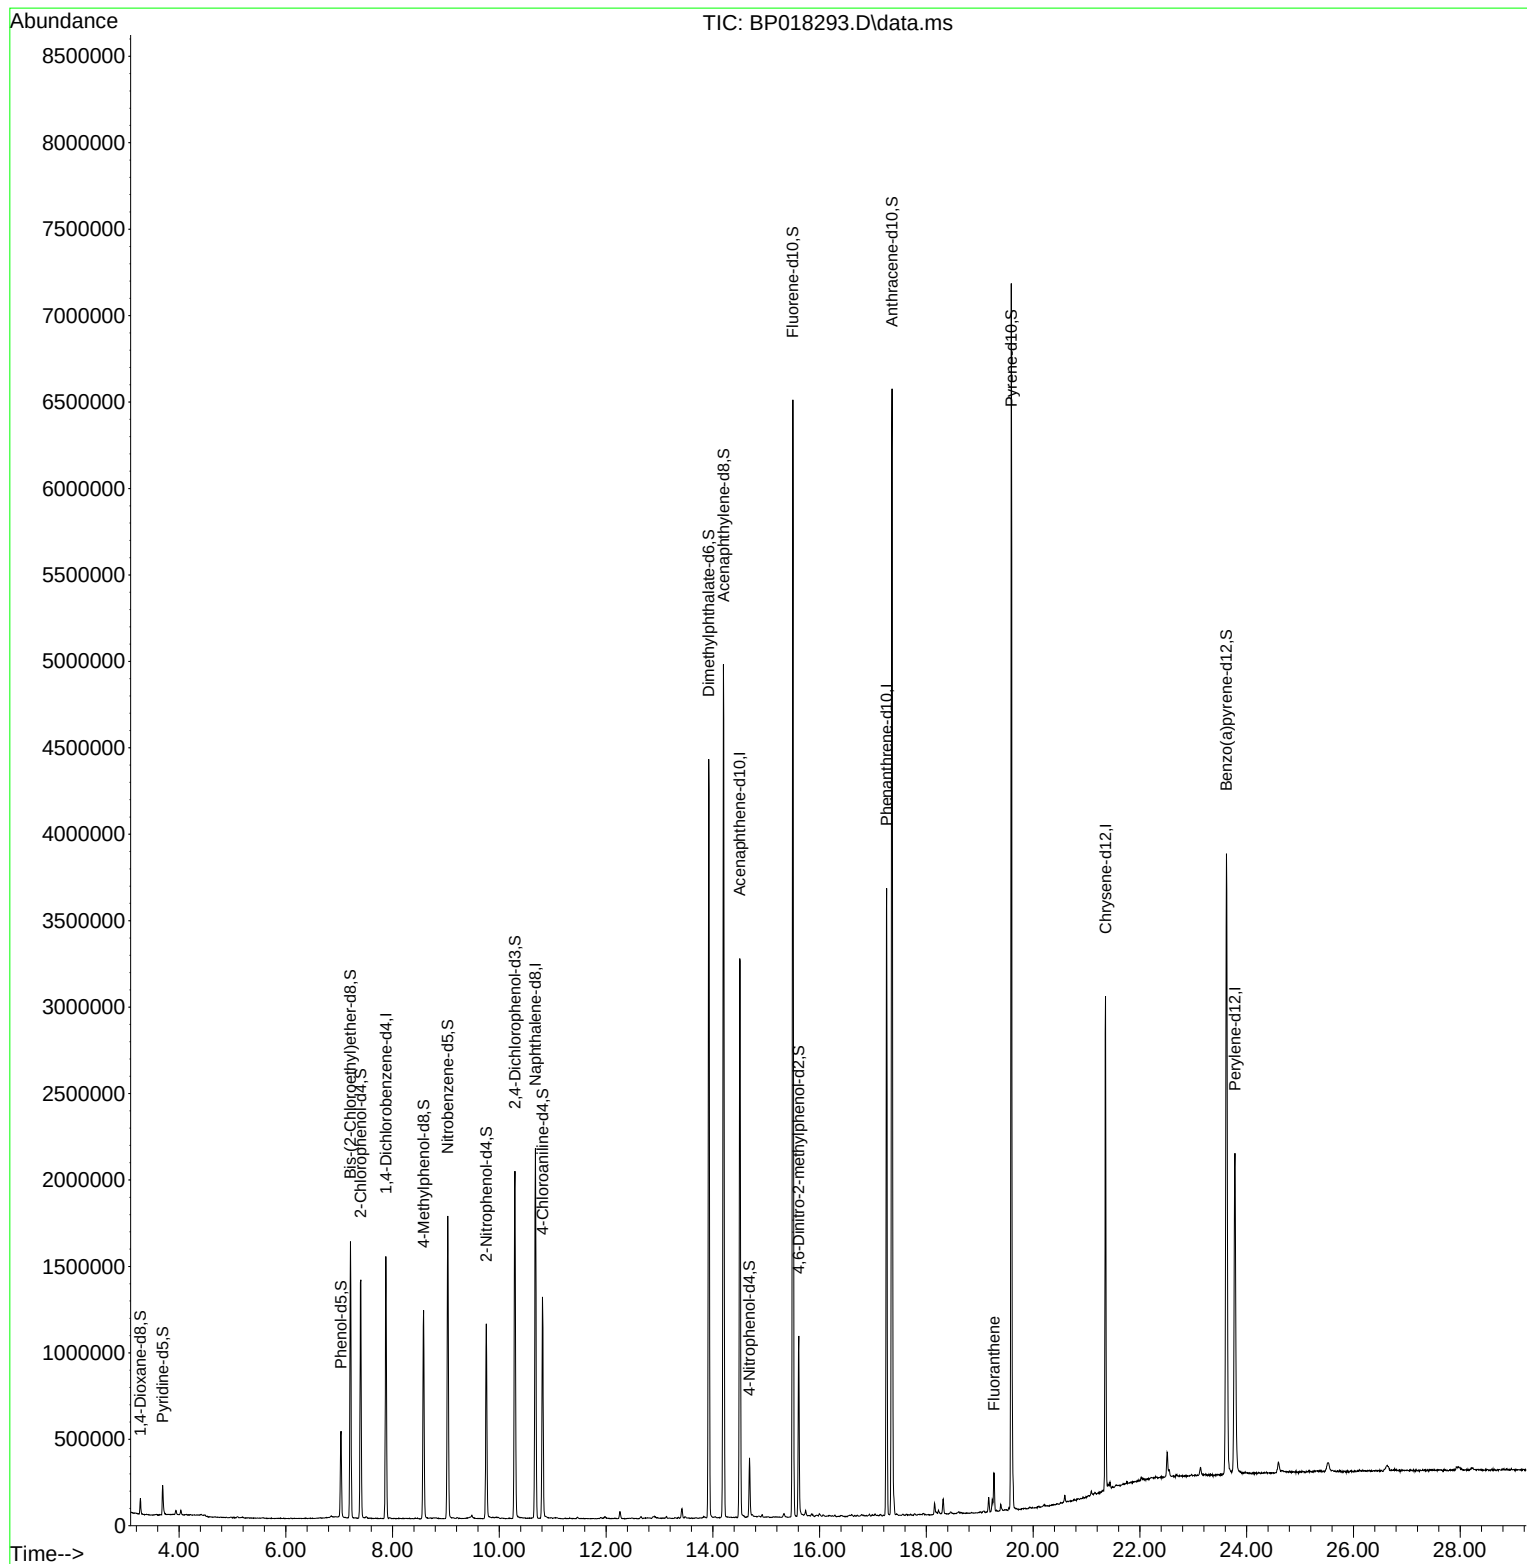

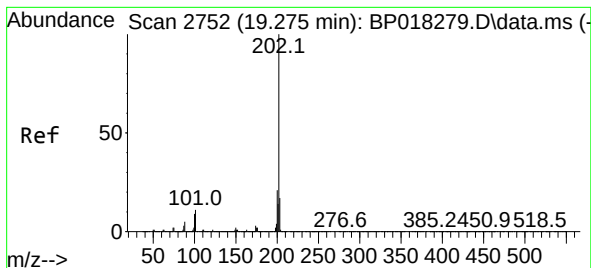

#80

Fluoranthene

Concen: 1.048 ng/ul

RT: 19.269 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP018293.D


Acq: 23 Nov 2023 01:25

Instrument :

BNA_P

ClientSampleId :

YCG83

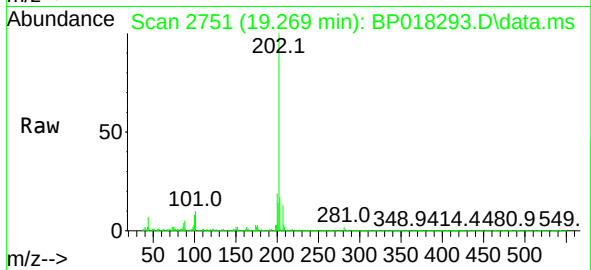

Tgt Ion:202 Resp: 131017

Ion Ratio Lower Upper

202 100

101 9.6 8.6 13.0

100 8.2 6.7 10.1

