

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018276.D
 Acq On : 22 Nov 2023 14:55
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	40	rVB	115086	153850	2.18%	0.189%
2	3.681	97	101	117	rBV	1416820	1952245	27.63%	2.404%
3	4.028	156	160	166	rVB2	20477	33108	0.47%	0.041%
4	4.522	239	244	250	rBV4	11180	26805	0.38%	0.033%
5	7.028	663	670	688	rVB	1459774	2327510	32.95%	2.866%
6	7.205	694	700	709	rVB	1264543	1911308	27.05%	2.353%
7	7.399	726	733	745	rVB	1467872	2326613	32.93%	2.864%
8	7.869	806	813	822	rBV	1160042	1826584	25.85%	2.249%
9	8.299	884	886	892	rVB6	5383	8985	0.13%	0.011%
10	8.575	921	933	946	rBV	1902619	2951344	41.78%	3.634%
11	8.822	968	975	978	rBV9	4138	8992	0.13%	0.011%
12	9.028	1003	1010	1020	rBV	1382051	2253328	31.90%	2.774%
13	9.481	1085	1087	1095	rVB7	8163	13647	0.19%	0.017%
14	9.752	1123	1133	1144	rBV	961270	1580192	22.37%	1.946%
15	10.287	1216	1224	1235	rBV	1786409	2944185	41.67%	3.625%
16	10.675	1279	1290	1300	rBV	1626427	2723018	38.54%	3.353%
17	10.810	1305	1313	1323	rVV	1970480	3282646	46.47%	4.042%
18	10.875	1323	1324	1330	rVB6	5946	9109	0.13%	0.011%
19	11.822	1475	1485	1486	rBV8	14704	31555	0.45%	0.039%
20	12.263	1555	1560	1567	rBV	38715	61602	0.87%	0.076%
21	12.475	1591	1596	1600	rVB8	5751	10269	0.15%	0.013%
22	12.651	1621	1626	1629	rBV7	6346	13704	0.19%	0.017%
23	12.722	1635	1638	1641	rBV4	4960	8374	0.12%	0.010%
24	12.887	1658	1666	1677	rBV2	36864	129178	1.83%	0.159%
25	13.310	1733	1738	1743	rVB9	4020	7556	0.11%	0.009%
26	13.428	1752	1758	1762	rBV2	30142	45039	0.64%	0.055%
27	13.481	1764	1767	1774	rVB8	6487	11246	0.16%	0.014%
28	13.822	1816	1825	1832	rBV2	38305	82326	1.17%	0.101%
29	13.928	1835	1843	1856	rVB	3602986	4823929	68.28%	5.939%
30	14.204	1883	1890	1897	rVB	4000488	5846543	82.76%	7.198%
31	14.440	1923	1930	1933	rBV5	13526	23593	0.33%	0.029%
32	14.510	1933	1942	1948	rVV	2649478	3830108	54.21%	4.716%
33	14.557	1948	1950	1958	rVB	47015	65095	0.92%	0.080%
34	14.693	1964	1973	1987	rBV	1198941	1735523	24.57%	2.137%
35	14.875	2000	2004	2008	rBV6	6456	11157	0.16%	0.014%
36	15.340	2076	2083	2087	rBV2	43233	65203	0.92%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018276.D
 Acq On : 22 Nov 2023 14:55
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.504	2104	2111	2124	rBV	4990748	7064765	100.00%	8.698%
38	15.616	2124	2130	2140	rBV	672502	992301	14.05%	1.222%
39	15.745	2148	2152	2164	rVB4	28771	60284	0.85%	0.074%
40	15.869	2171	2173	2178	rVB6	9021	13152	0.19%	0.016%
41	15.963	2183	2189	2196	rVB2	28045	49481	0.70%	0.061%
42	16.069	2201	2207	2213	rBV10	12896	26074	0.37%	0.032%
43	16.292	2241	2245	2249	rVB6	7734	13228	0.19%	0.016%
44	16.457	2268	2273	2276	rBV7	6402	10004	0.14%	0.012%
45	16.551	2285	2289	2291	rBV5	7556	9754	0.14%	0.012%
46	16.610	2295	2299	2304	rVV3	19984	23731	0.34%	0.029%
47	16.792	2325	2330	2334	rBV4	10010	16394	0.23%	0.020%
48	16.934	2352	2354	2364	rVB9	7213	11457	0.16%	0.014%
49	17.045	2369	2373	2379	rBV6	9456	19082	0.27%	0.023%
50	17.157	2386	2392	2396	rBV2	25339	36226	0.51%	0.045%
51	17.204	2396	2400	2403	rBV6	8292	11678	0.17%	0.014%
52	17.263	2404	2410	2420	rVV	2985085	4179216	59.16%	5.145%
53	17.363	2420	2427	2439	rVB	5041617	6992564	98.98%	8.609%
54	17.639	2469	2474	2475	rBV4	6791	9014	0.13%	0.011%
55	17.669	2475	2479	2484	rVV3	12478	20112	0.28%	0.025%
56	17.716	2484	2487	2493	rVB5	11695	18043	0.26%	0.022%
57	17.863	2509	2512	2516	rVB6	7122	9649	0.14%	0.012%
58	17.951	2523	2527	2532	rBV7	6337	14180	0.20%	0.017%
59	18.169	2558	2564	2567	rBV3	53973	80922	1.15%	0.100%
60	18.239	2573	2576	2581	rVB2	9760	13852	0.20%	0.017%
61	18.669	2646	2649	2654	rVB7	17048	22532	0.32%	0.028%
62	18.781	2665	2668	2671	rBV4	9827	11540	0.16%	0.014%
63	19.075	2715	2718	2719	rBV3	7693	8275	0.12%	0.010%
64	19.181	2732	2736	2742	rVB2	59260	86174	1.22%	0.106%
65	19.245	2743	2747	2751	rBV	51657	68421	0.97%	0.084%
66	19.404	2771	2774	2779	rBV2	32598	44212	0.63%	0.054%
67	19.563	2798	2801	2802	rBV3	14639	16332	0.23%	0.020%
68	19.604	2802	2808	2814	rVV	5016000	6607022	93.52%	8.134%
69	20.610	2975	2979	2984	rVB	149783	177447	2.51%	0.218%
70	21.363	3102	3107	3113	rBV	2266523	2884980	40.84%	3.552%
71	23.633	3486	3493	3509	rVB2	2738844	5370825	76.02%	6.612%
72	23.792	3513	3520	3531	rVB	1504538	3094216	43.80%	3.810%




Sum of corrected areas: 81222608

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018276.D
Acq On : 22 Nov 2023 14:55
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

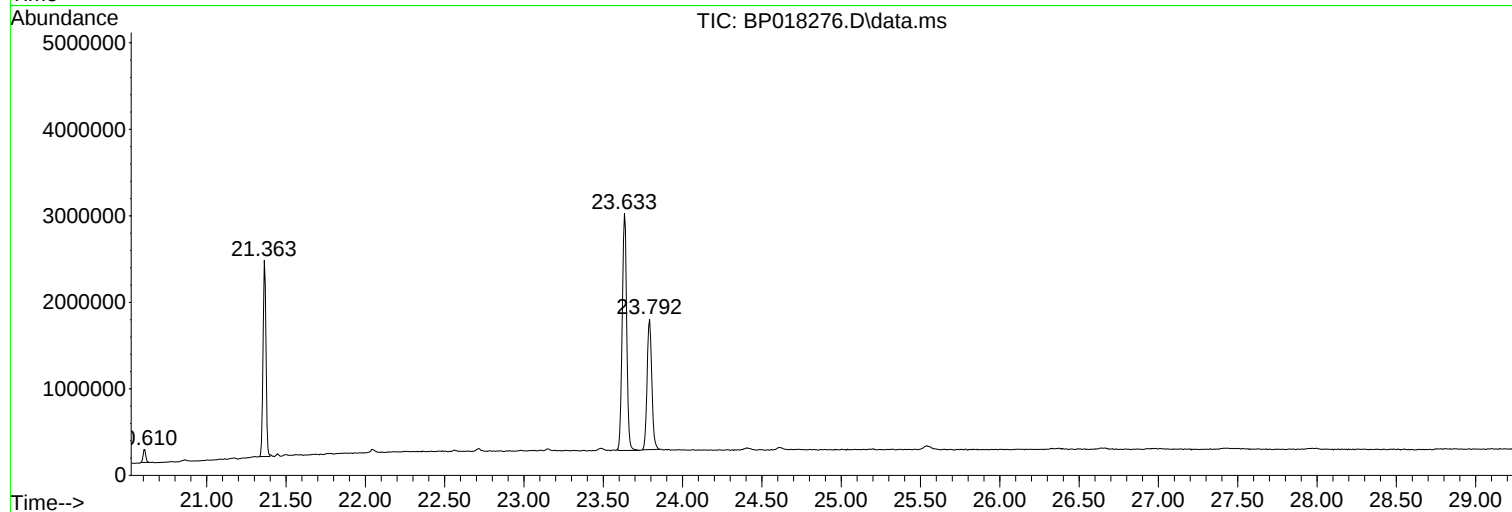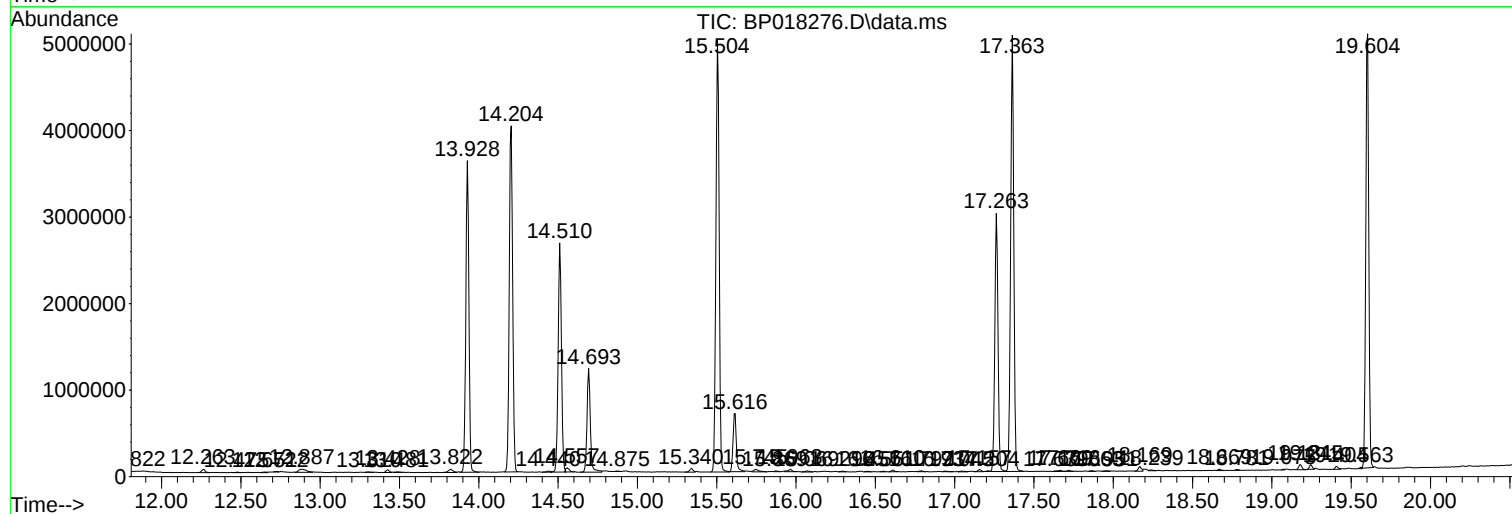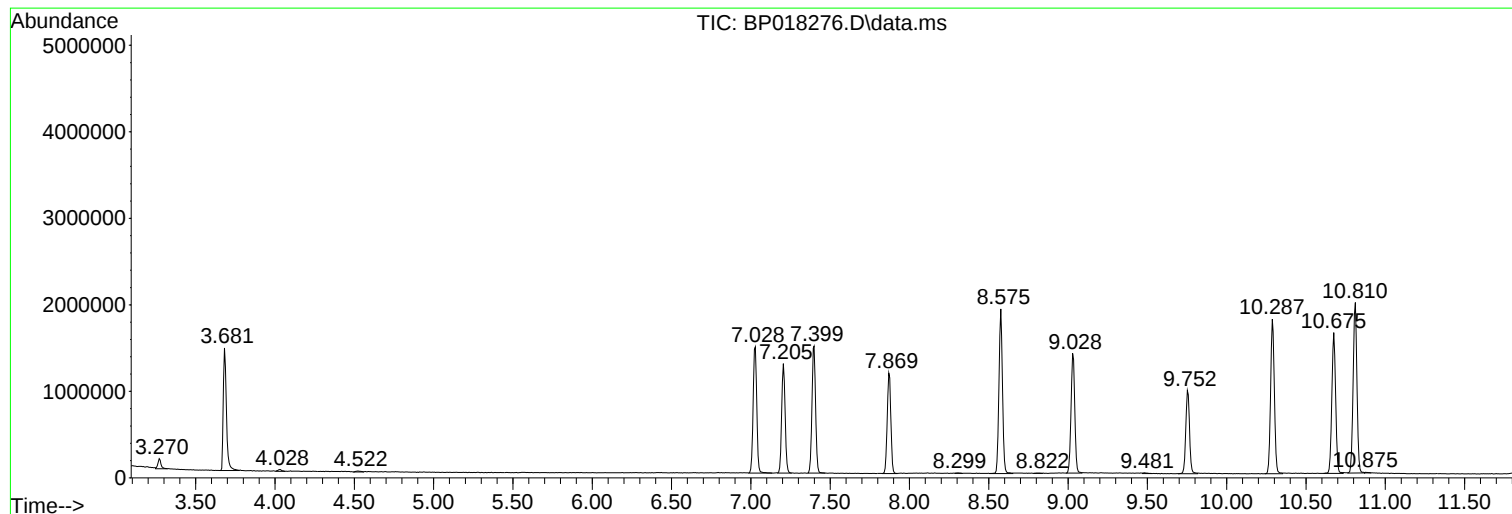

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018276.D
Acq On : 22 Nov 2023 14:55
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018276.D
Acq On : 22 Nov 2023 14:55
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc