

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018277.D
 Acq On : 22 Nov 2023 15:41
 Operator : MA/JU
 Sample : 05268-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	39	rVB	112357	149959	0.98%	0.075%
2	3.687	97	102	116	rBV	1548654	2411610	15.80%	1.210%
3	3.846	126	129	136	rVB3	26506	40160	0.26%	0.020%
4	3.940	141	145	148	rVV	15451	22114	0.14%	0.011%
5	3.981	148	152	155	rVB3	18708	23104	0.15%	0.012%
6	4.028	156	160	165	rVB	32056	38515	0.25%	0.019%
7	4.522	240	244	249	rBV2	12098	24312	0.16%	0.012%
8	5.893	473	477	482	rVB8	9304	17965	0.12%	0.009%
9	7.063	663	676	689	rBV2	6710837	13113549	85.91%	6.577%
10	7.210	694	701	708	rVB	1499348	2217499	14.53%	1.112%
11	7.399	726	733	746	rVV	1737965	2713125	17.77%	1.361%
12	7.505	746	751	759	rVB4	22632	43008	0.28%	0.022%
13	7.875	806	814	821	rBV	1205039	1914008	12.54%	0.960%
14	8.310	881	888	897	rBV	2367684	3765721	24.67%	1.889%
15	8.581	926	934	938	rBV	2205133	3570147	23.39%	1.791%
16	8.640	938	944	955	rVB	6480901	10234299	67.05%	5.133%
17	9.034	1003	1011	1020	rBV	1650100	2635464	17.27%	1.322%
18	9.481	1084	1087	1095	rVB7	15977	30751	0.20%	0.015%
19	9.757	1121	1134	1136	rBV	1171598	1935157	12.68%	0.971%
20	9.787	1136	1139	1144	rVV	1610064	2475331	16.22%	1.241%
21	9.857	1144	1151	1166	rVB	8601422	13967814	91.51%	7.006%
22	10.151	1197	1201	1206	rVB8	11267	16963	0.11%	0.009%
23	10.322	1216	1230	1250	rBV2	7395347	15264426	100.00%	7.656%
24	10.675	1283	1290	1299	rVB	1670188	2827599	18.52%	1.418%
25	10.810	1305	1313	1316	rBV	2090983	3549672	23.25%	1.780%
26	10.851	1316	1320	1332	rVB	4896883	8217076	53.83%	4.121%
27	11.863	1485	1492	1494	rBV8	11710	22360	0.15%	0.011%
28	12.263	1555	1560	1568	rVB2	41836	72671	0.48%	0.036%
29	12.704	1628	1635	1639	rBV10	9734	24395	0.16%	0.012%
30	12.945	1660	1676	1681	rBV	9588999	14950851	97.95%	7.499%
31	13.004	1681	1686	1701	rVB	2888060	4467333	29.27%	2.241%
32	13.422	1752	1757	1762	rVB4	19070	29203	0.19%	0.015%
33	13.828	1820	1826	1834	rBV3	29245	62340	0.41%	0.031%
34	13.928	1836	1843	1852	rVV	3579872	5001883	32.77%	2.509%
35	14.004	1852	1856	1865	rVB4	36604	62574	0.41%	0.031%
36	14.204	1879	1890	1898	rBV	4381868	6429761	42.12%	3.225%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018277.D
 Acq On : 22 Nov 2023 15:41
 Operator : MA/JU
 Sample : 05268-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.510	1935	1942	1948	rBV	2521048	3654898	23.94%	1.833%
38	14.563	1948	1951	1954	rVB2	20696	19872	0.13%	0.010%
39	14.622	1954	1961	1968	rBV	4069081	5684649	37.24%	2.851%
40	14.722	1968	1978	1992	rVB2	5436753	10118995	66.29%	5.075%
41	15.134	2041	2048	2062	rBV	2141267	3167257	20.75%	1.589%
42	15.345	2080	2084	2095	rVB3	28046	53649	0.35%	0.027%
43	15.504	2104	2111	2124	rBV	5231083	7504540	49.16%	3.764%
44	15.633	2124	2133	2149	rBV2	6174821	10083451	66.06%	5.057%
45	15.751	2149	2153	2160	rVB3	32486	63724	0.42%	0.032%
46	15.963	2186	2189	2195	rVB3	22912	34968	0.23%	0.018%
47	16.075	2203	2208	2211	rBV6	13184	17272	0.11%	0.009%
48	16.486	2275	2278	2284	rVB5	20073	25036	0.16%	0.013%
49	16.610	2295	2299	2306	rVB4	14822	22174	0.15%	0.011%
50	16.904	2342	2349	2362	rBV	4064081	5603717	36.71%	2.811%
51	17.157	2389	2392	2397	rVB3	19174	26977	0.18%	0.014%
52	17.263	2404	2410	2420	rVV	2604577	3594117	23.55%	1.803%
53	17.363	2420	2427	2439	rVB	5208344	7096997	46.49%	3.559%
54	17.716	2484	2487	2492	rBV7	11638	18529	0.12%	0.009%
55	17.833	2503	2507	2510	rBV5	20264	25195	0.17%	0.013%
56	17.880	2510	2515	2521	rVB	150310	201212	1.32%	0.101%
57	18.163	2559	2563	2567	rBV4	46665	68994	0.45%	0.035%
58	18.480	2612	2617	2622	rBV	100222	130460	0.85%	0.065%
59	18.669	2646	2649	2655	rVB8	14438	18744	0.12%	0.009%
60	19.180	2731	2736	2742	rVB2	61855	88762	0.58%	0.045%
61	19.245	2742	2747	2751	rBV	59660	88911	0.58%	0.045%
62	19.404	2771	2774	2779	rBV7	32976	45025	0.29%	0.023%
63	19.598	2801	2807	2814	rBV	5200432	6927594	45.38%	3.475%
64	20.604	2975	2978	2984	rVB	134492	150466	0.99%	0.075%
65	21.363	3102	3107	3114	rBV	2295921	2818079	18.46%	1.413%
66	23.633	3485	3493	3505	rBV2	3323439	6547009	42.89%	3.284%
67	23.792	3512	3520	3532	rBV	1531895	3139328	20.57%	1.575%




Sum of corrected areas: 199383320

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018277.D
Acq On : 22 Nov 2023 15:41
Operator : MA/JU
Sample : 05268-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

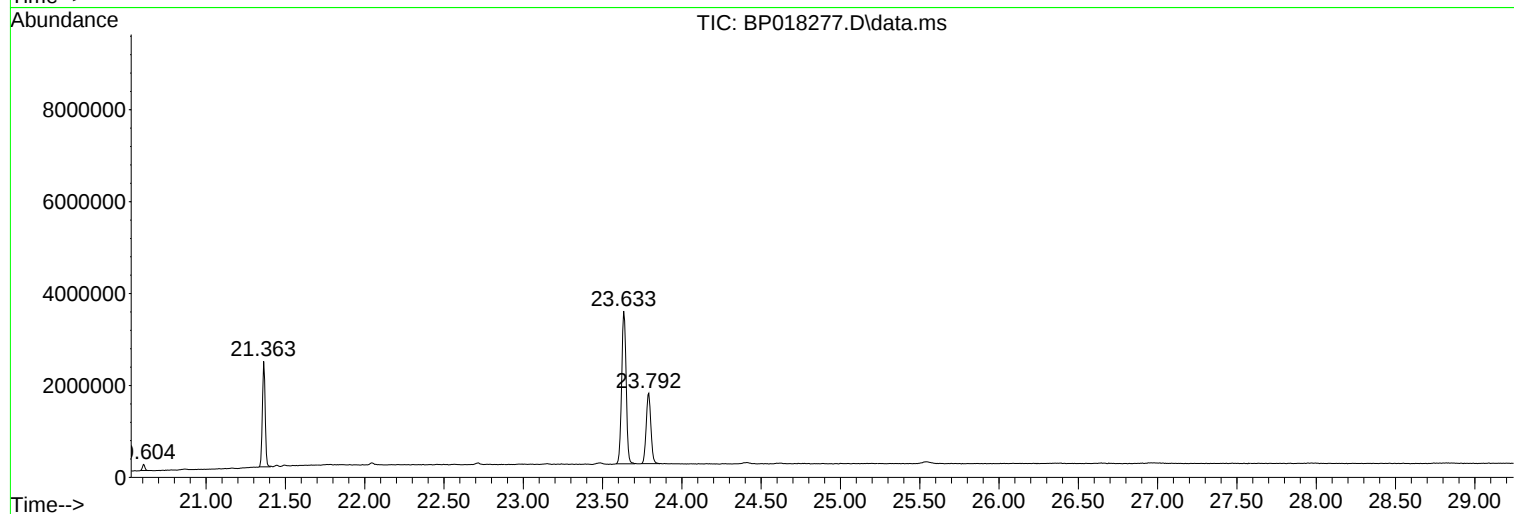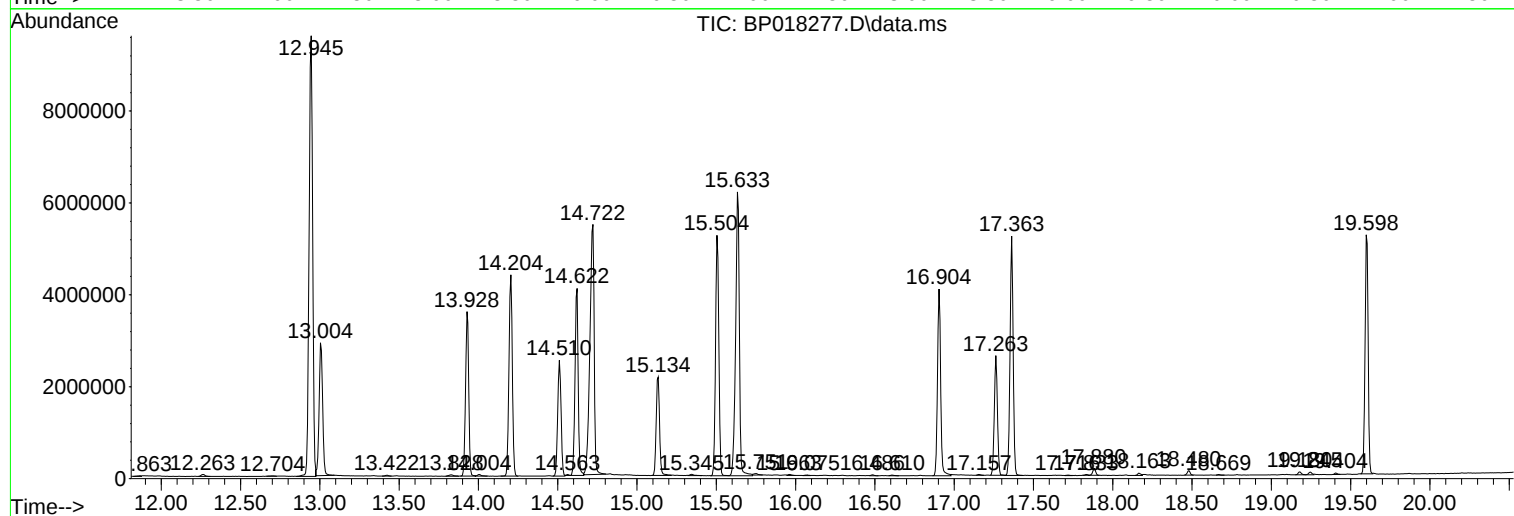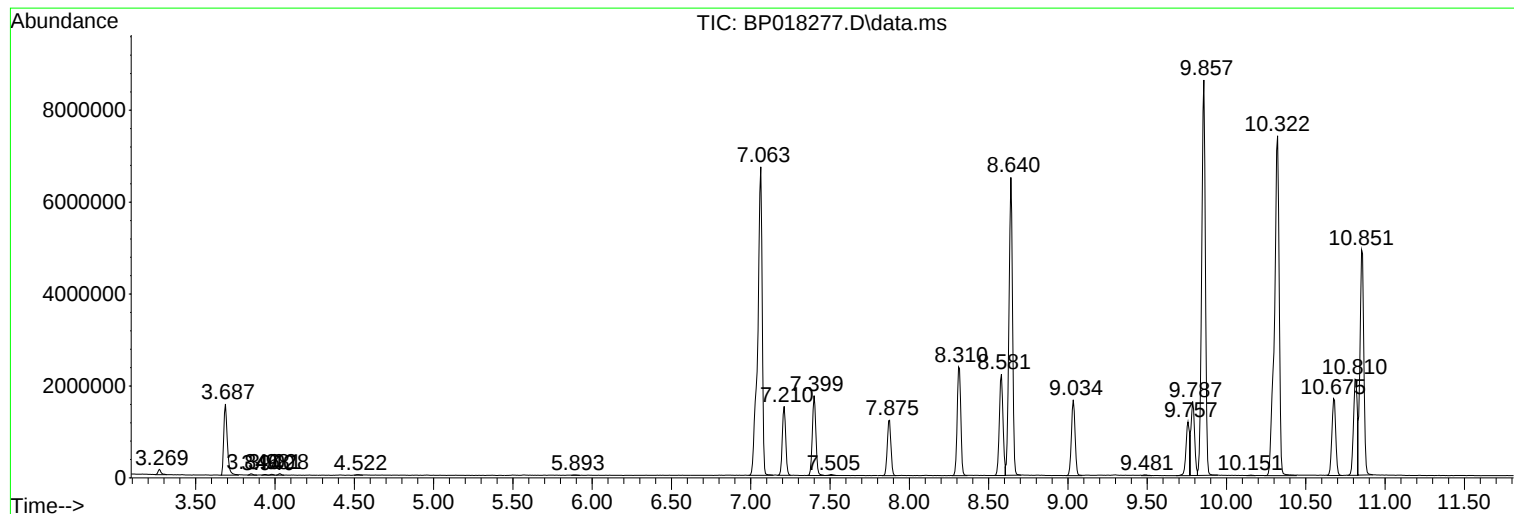

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018277.D
Acq On : 22 Nov 2023 15:41
Operator : MA/JU
Sample : 05268-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018277.D
Acq On : 22 Nov 2023 15:41
Operator : MA/JU
Sample : 05268-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc