

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018278.D
 Acq On : 22 Nov 2023 16:38
 Operator : MA/JU
 Sample : 05268-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKF8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	42	rVB	29679	53672	1.72%	0.107%
2	3.687	98	102	114	rVV	310299	453248	14.53%	0.902%
3	4.028	156	160	164	rBV	22272	27936	0.90%	0.056%
4	5.228	362	364	366	rBV3	3835	4212	0.14%	0.008%
5	6.175	523	525	527	rVB3	4480	3677	0.12%	0.007%
6	6.410	562	565	570	rBV7	3659	5856	0.19%	0.012%
7	7.051	663	674	683	rVB2	1430694	2613836	83.78%	5.199%
8	7.204	693	700	708	rBV	289497	437119	14.01%	0.869%
9	7.393	726	732	742	rBV	320951	513489	16.46%	1.021%
10	7.504	748	751	756	rVB7	5097	8339	0.27%	0.017%
11	7.628	769	772	777	rVV7	3617	4069	0.13%	0.008%
12	7.869	806	813	821	rVV	1014785	1614135	51.74%	3.211%
13	8.140	858	859	865	rBV6	2493	4437	0.14%	0.009%
14	8.310	882	888	896	rBV	473229	709821	22.75%	1.412%
15	8.575	925	933	937	rBV	432661	665695	21.34%	1.324%
16	8.634	937	943	954	rVB	1260931	2008718	64.38%	3.995%
17	8.810	971	973	977	rVB5	3803	3824	0.12%	0.008%
18	8.904	985	989	992	rBV6	4131	5641	0.18%	0.011%
19	9.028	1004	1010	1021	rVB	299864	487739	15.63%	0.970%
20	9.222	1039	1043	1045	rBV5	2772	4048	0.13%	0.008%
21	9.481	1086	1087	1092	rVB5	5410	5362	0.17%	0.011%
22	9.698	1115	1124	1126	rBV9	5446	10092	0.32%	0.020%
23	9.751	1126	1133	1135	rVV	178949	285082	9.14%	0.567%
24	9.781	1135	1138	1143	rVV	256487	420092	13.46%	0.836%
25	9.845	1143	1149	1160	rVV	1806505	2812231	90.14%	5.594%
26	10.316	1217	1229	1238	rBV2	1425618	2963640	94.99%	5.895%
27	10.381	1238	1240	1244	rVB5	2906	5251	0.17%	0.010%
28	10.469	1253	1255	1259	rBV5	2739	4100	0.13%	0.008%
29	10.675	1283	1290	1298	rBV	1448773	2348047	75.26%	4.670%
30	10.734	1298	1300	1303	rVB4	5348	4793	0.15%	0.010%
31	10.810	1305	1313	1316	rVV	417718	758286	24.30%	1.508%
32	10.851	1316	1320	1332	rVB	948081	1543874	49.48%	3.071%
33	11.810	1474	1483	1484	rBV7	12767	20808	0.67%	0.041%
34	11.839	1486	1488	1490	rVV3	4369	5147	0.16%	0.010%
35	11.869	1490	1493	1495	rVV4	3333	5183	0.17%	0.010%
36	11.992	1513	1514	1520	rVB6	4758	5466	0.18%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018278.D
 Acq On : 22 Nov 2023 16:38
 Operator : MA/JU
 Sample : 05268-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKF8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	12.263	1555	1560	1567	rBV3	10436	13855	0.44%	0.028%
38	12.534	1602	1606	1609	rBV6	3665	5975	0.19%	0.012%
39	12.657	1622	1627	1628	rBV4	5336	8187	0.26%	0.016%
40	12.886	1657	1666	1668	rBV3	32311	72851	2.34%	0.145%
41	12.939	1669	1675	1681	rVV	1914519	2915670	93.45%	5.799%
42	13.004	1681	1686	1699	rVB	534547	831493	26.65%	1.654%
43	13.181	1713	1716	1720	rVB6	4081	5755	0.18%	0.011%
44	13.422	1752	1757	1762	rBV2	22144	35021	1.12%	0.070%
45	13.569	1777	1782	1785	rVB6	3208	4770	0.15%	0.009%
46	13.645	1792	1795	1798	rBV4	3776	3994	0.13%	0.008%
47	13.822	1819	1825	1830	rBV2	31170	63751	2.04%	0.127%
48	13.928	1837	1843	1853	rVV	745540	1045768	33.52%	2.080%
49	14.004	1853	1856	1861	rVB7	6782	8293	0.27%	0.016%
50	14.122	1872	1876	1877	rBV4	2927	3603	0.12%	0.007%
51	14.198	1881	1889	1896	rVV	852162	1284012	41.16%	2.554%
52	14.257	1897	1899	1904	rVB6	4810	6288	0.20%	0.013%
53	14.439	1925	1930	1933	rBV6	10619	16055	0.51%	0.032%
54	14.510	1933	1942	1948	rVV	2187145	3119916	100.00%	6.206%
55	14.557	1948	1950	1953	rVV2	36226	40260	1.29%	0.080%
56	14.610	1954	1959	1967	rVV	478405	692311	22.19%	1.377%
57	14.704	1967	1975	1991	rVV2	1094787	1820974	58.37%	3.622%
58	14.910	2008	2010	2016	rVB7	5252	7793	0.25%	0.016%
59	15.033	2027	2031	2032	rBV4	4728	4082	0.13%	0.008%
60	15.063	2032	2036	2038	rVB5	3385	4433	0.14%	0.009%
61	15.128	2042	2047	2054	rBV	389206	553578	17.74%	1.101%
62	15.339	2077	2083	2088	rBV2	30801	47853	1.53%	0.095%
63	15.504	2103	2111	2119	rBV	1109541	1551273	49.72%	3.086%
64	15.628	2123	2132	2144	rBV2	921235	1437957	46.09%	2.860%
65	15.739	2149	2151	2156	rVB6	7733	11142	0.36%	0.022%
66	15.875	2170	2174	2178	rBV7	8578	12537	0.40%	0.025%
67	15.933	2178	2184	2185	rVV5	11083	14001	0.45%	0.028%
68	15.963	2186	2189	2195	rVV	23643	33464	1.07%	0.067%
69	16.027	2197	2200	2201	rVB2	5603	4819	0.15%	0.010%
70	16.069	2201	2207	2210	rBV8	8190	14184	0.45%	0.028%
71	16.163	2221	2223	2225	rBV3	4960	6239	0.20%	0.012%
72	16.245	2233	2237	2239	rBV5	4655	6622	0.21%	0.013%
73	16.292	2243	2245	2247	rVV3	4598	3670	0.12%	0.007%
74	16.398	2260	2263	2270	rBV9	8750	18100	0.58%	0.036%
75	16.486	2276	2278	2282	rVB5	4984	4088	0.13%	0.008%
76	16.610	2294	2299	2304	rBV4	17610	25147	0.81%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018278.D
 Acq On : 22 Nov 2023 16:38
 Operator : MA/JU
 Sample : 05268-01DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCKF8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

77	16.780	2324	2328	2332	rBV5	11297	15948	0.51%	0.032%
78	16.833	2335	2337	2340	rBV4	3418	3818	0.12%	0.008%
79	16.904	2340	2349	2361	rBV	625331	939528	30.11%	1.869%
80	17.045	2370	2373	2380	rVB7	8263	11513	0.37%	0.023%
81	17.104	2380	2383	2388	rBV7	5225	6392	0.20%	0.013%
82	17.157	2388	2392	2397	rBV3	21113	31337	1.00%	0.062%
83	17.210	2398	2401	2403	rVV4	7741	8338	0.27%	0.017%
84	17.263	2404	2410	2417	rVV	2218267	3050022	97.76%	6.067%
85	17.363	2421	2427	2439	rVB	982693	1421355	45.56%	2.827%
86	17.669	2475	2479	2480	rBV4	6273	7234	0.23%	0.014%
87	17.722	2484	2488	2491	rVB5	10619	13032	0.42%	0.026%
88	17.816	2501	2504	2505	rBV3	4957	5140	0.16%	0.010%
89	17.886	2510	2516	2520	rVV7	30100	52524	1.68%	0.104%
90	17.951	2523	2527	2531	rVV6	6301	10122	0.32%	0.020%
91	18.163	2560	2563	2567	rBV4	37104	56074	1.80%	0.112%
92	18.480	2612	2617	2621	rBV5	18904	26120	0.84%	0.052%
93	18.669	2646	2649	2653	rVB6	14170	16922	0.54%	0.034%
94	19.174	2733	2735	2741	rVB5	15806	22022	0.71%	0.044%
95	19.404	2771	2774	2781	rBV7	24845	33778	1.08%	0.067%
96	19.598	2802	2807	2813	rBV	1118607	1362168	43.66%	2.709%
97	20.604	2975	2978	2985	rVB2	96190	116079	3.72%	0.231%
98	21.362	3102	3107	3115	rBV	1908862	2422244	77.64%	4.818%
99	23.633	3487	3493	3505	rVB	635921	1274767	40.86%	2.536%
100	23.792	3513	3520	3535	rVB	1370191	2782305	89.18%	5.534%




Sum of corrected areas: 50275531

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018278.D
Acq On : 22 Nov 2023 16:38
Operator : MA/JU
Sample : 05268-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

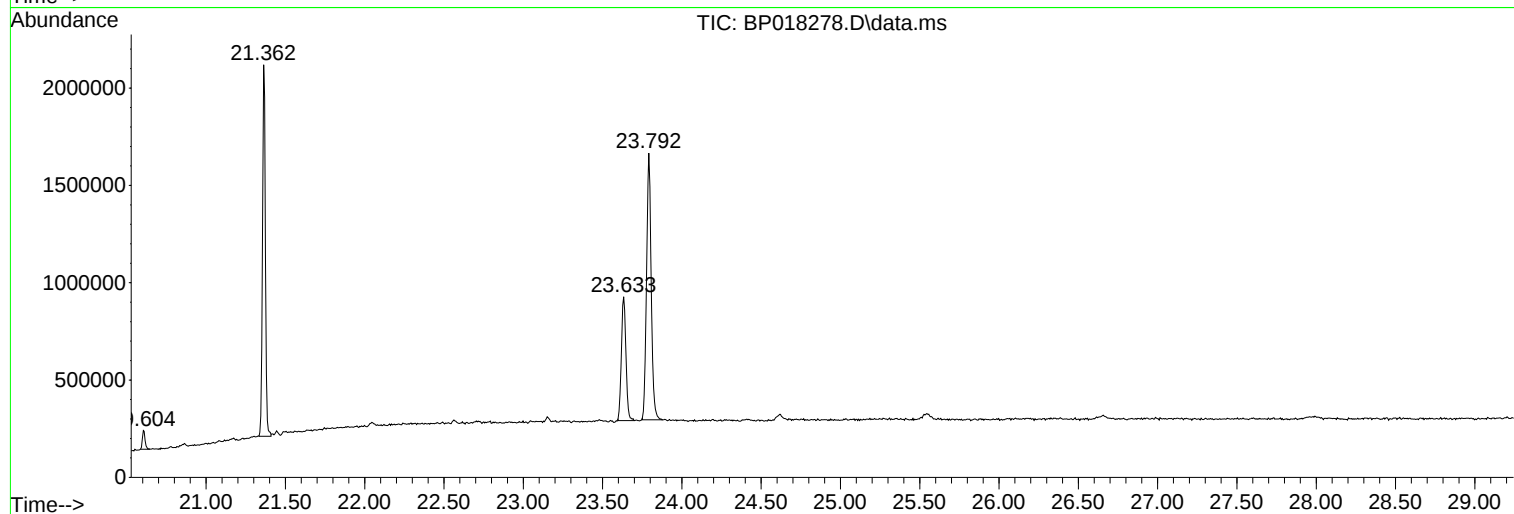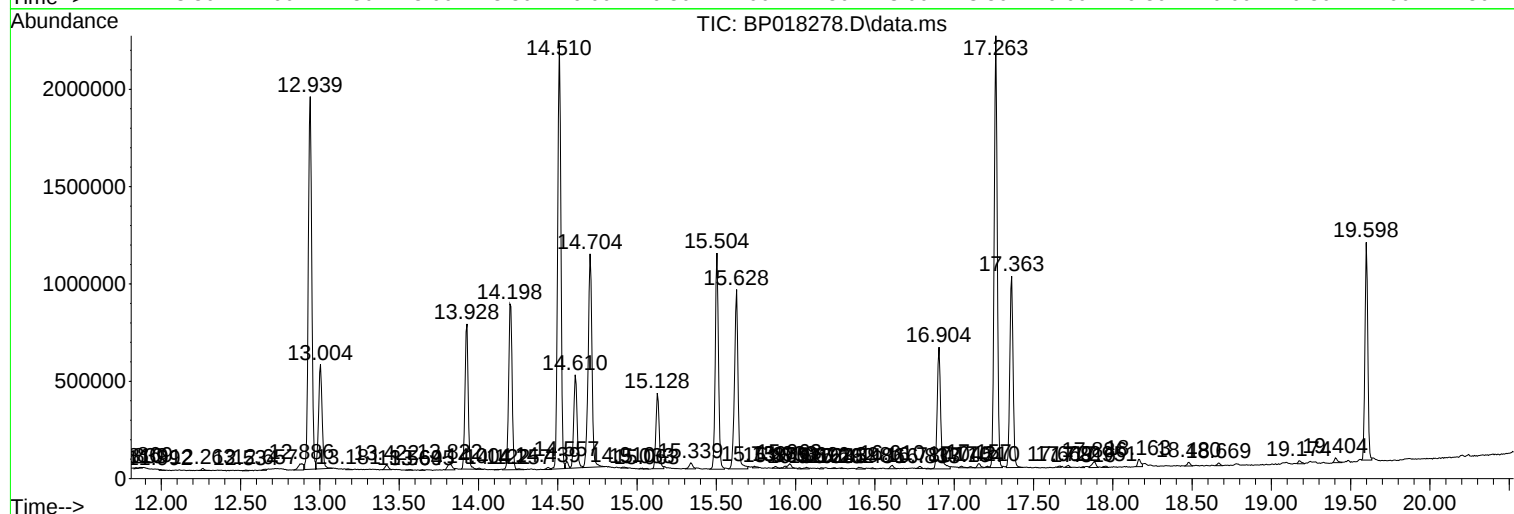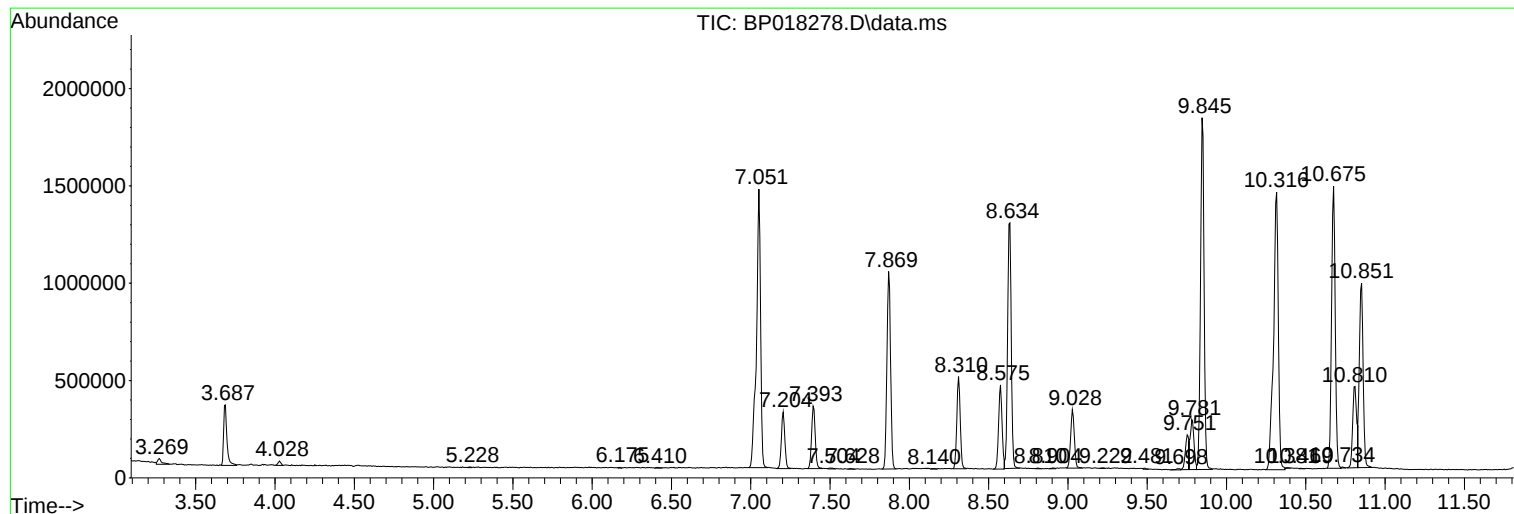

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018278.D
Acq On : 22 Nov 2023 16:38
Operator : MA/JU
Sample : 05268-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018278.D
Acq On : 22 Nov 2023 16:38
Operator : MA/JU
Sample : 05268-01DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCKF8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------