

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018281.D
 Acq On : 22 Nov 2023 18:38
 Operator : MA/JU
 Sample : PB156975BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rVB	108405	134611	1.51%	0.141%
2	3.687	98	102	120	rBV	1496737	2064003	23.11%	2.161%
3	4.034	157	161	168	rVB	25174	36911	0.41%	0.039%
4	7.034	664	671	681	rBV	1604619	2437485	27.30%	2.553%
5	7.210	695	701	711	rVB	1330753	2054702	23.01%	2.152%
6	7.405	727	734	743	rBV	1603654	2449938	27.44%	2.566%
7	7.875	807	814	824	rBV	1348901	2173197	24.34%	2.276%
8	8.581	925	934	945	rBV	2002457	3119506	34.93%	3.267%
9	9.034	999	1011	1025	rBV	1455506	2422324	27.13%	2.537%
10	9.757	1125	1134	1147	rBV	1002430	1651377	18.49%	1.729%
11	10.293	1217	1225	1242	rBV	1918467	3152121	35.30%	3.301%
12	10.681	1283	1291	1299	rVB	1959132	3264891	36.56%	3.419%
13	10.810	1305	1313	1332	rBV	2093029	3601214	40.33%	3.771%
14	11.898	1494	1498	1503	rBV8	6989	14088	0.16%	0.015%
15	12.263	1552	1560	1569	rVB2	41114	75558	0.85%	0.079%
16	12.710	1632	1636	1641	rBV8	4634	11392	0.13%	0.012%
17	12.910	1663	1670	1675	rBV6	14398	30306	0.34%	0.032%
18	13.422	1753	1757	1763	rBV2	39895	63068	0.71%	0.066%
19	13.487	1763	1768	1770	rBV5	6501	10298	0.12%	0.011%
20	13.834	1823	1827	1831	rBV7	10000	15115	0.17%	0.016%
21	13.928	1836	1843	1850	rBV	4026261	5494993	61.54%	5.754%
22	14.204	1882	1890	1898	rBV	4481219	6542630	73.27%	6.851%
23	14.510	1934	1942	1949	rBV	3362080	4801602	53.77%	5.028%
24	14.557	1949	1950	1959	rVB8	11780	19987	0.22%	0.021%
25	14.692	1963	1973	1995	rBV	1467860	2154284	24.12%	2.256%
26	14.928	2007	2013	2018	rVB9	10990	22779	0.26%	0.024%
27	15.345	2080	2084	2087	rVB5	11119	11279	0.13%	0.012%
28	15.504	2104	2111	2120	rBV	5771857	8102272	90.73%	8.485%
29	15.610	2123	2129	2142	rBV	901233	1264225	14.16%	1.324%
30	15.745	2147	2152	2157	rVB3	26581	40434	0.45%	0.042%
31	15.969	2185	2190	2192	rVB5	5826	9509	0.11%	0.010%
32	16.075	2202	2208	2211	rVB6	9638	16834	0.19%	0.018%
33	16.186	2224	2227	2232	rBV7	5542	9356	0.10%	0.010%
34	16.292	2240	2245	2249	rBV7	8742	15609	0.17%	0.016%
35	16.604	2294	2298	2302	rBV7	7345	10362	0.12%	0.011%
36	16.775	2323	2327	2332	rBV7	5575	11237	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018281.D
 Acq On : 22 Nov 2023 18:38
 Operator : MA/JU
 Sample : PB156975BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.933	2351	2354	2362	rVB10	10063	16297	0.18%	0.017%
38	17.045	2368	2373	2376	rBV3	11242	19494	0.22%	0.020%
39	17.151	2386	2391	2396	rBV8	12507	21493	0.24%	0.023%
40	17.257	2403	2409	2419	rBV	4011735	5680350	63.61%	5.948%
41	17.357	2419	2426	2436	rBV2	5857225	8502207	95.21%	8.903%
42	17.633	2469	2473	2477	rBV5	9266	14662	0.16%	0.015%
43	17.857	2508	2511	2519	rBV10	5079	13684	0.15%	0.014%
44	18.163	2560	2563	2566	rBV5	13522	19917	0.22%	0.021%
45	19.174	2730	2735	2741	rVB2	74019	97580	1.09%	0.102%
46	19.239	2742	2746	2751	rVV	74741	91714	1.03%	0.096%
47	19.404	2771	2774	2778	rBV6	8558	13225	0.15%	0.014%
48	19.557	2796	2800	2801	rBV4	17286	22176	0.25%	0.023%
49	19.598	2801	2807	2816	rVB	6705084	8929685	100.00%	9.351%
50	20.604	2975	2978	2982	rVB	39502	46091	0.52%	0.048%
51	21.357	3101	3106	3117	rBV	3357219	4514581	50.56%	4.728%
52	23.627	3484	3492	3507	rBV2	3180049	6137131	68.73%	6.427%
53	23.780	3511	3518	3534	rVB	1911865	4043474	45.28%	4.234%




Sum of corrected areas: 95493258

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018281.D
Acq On : 22 Nov 2023 18:38
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

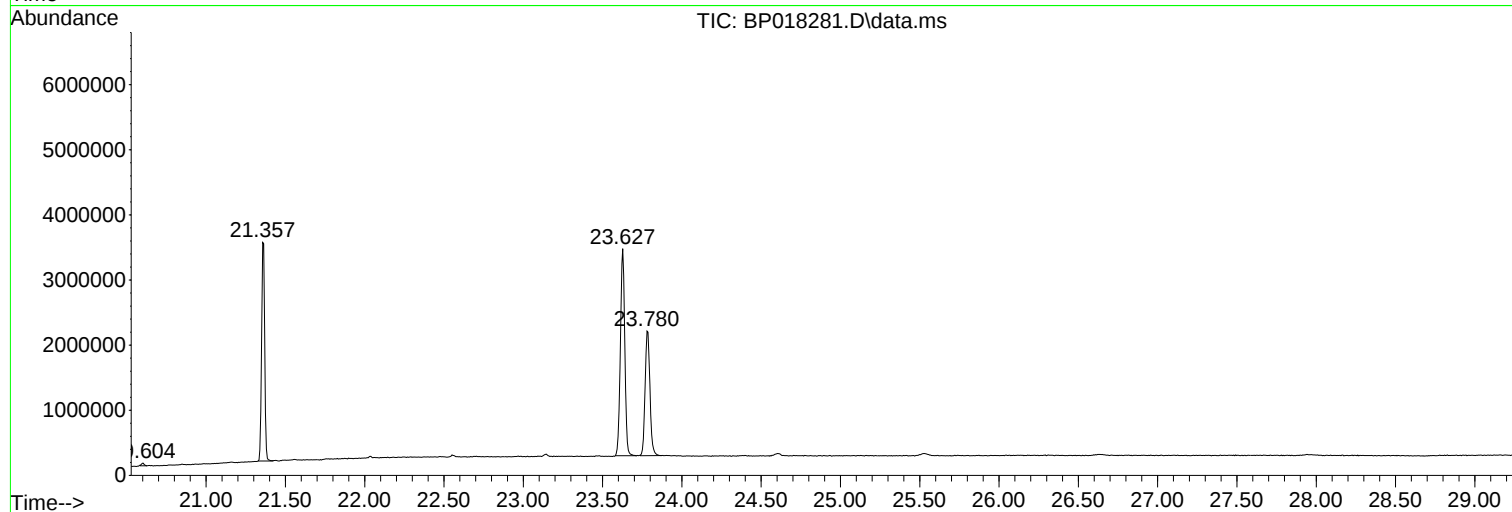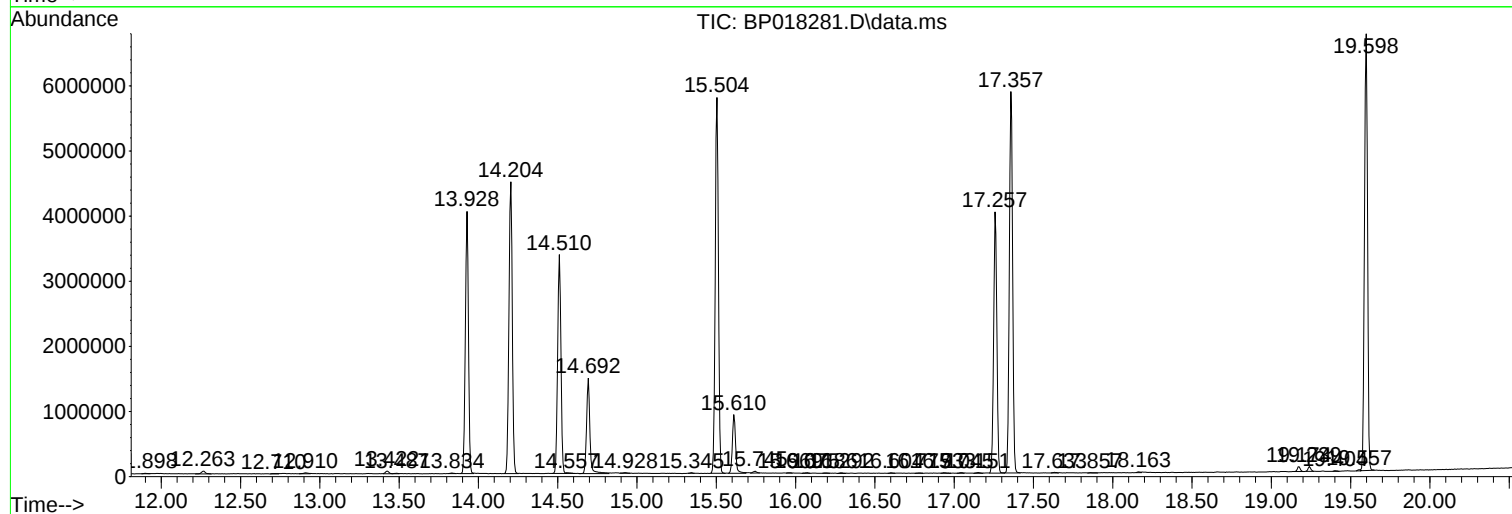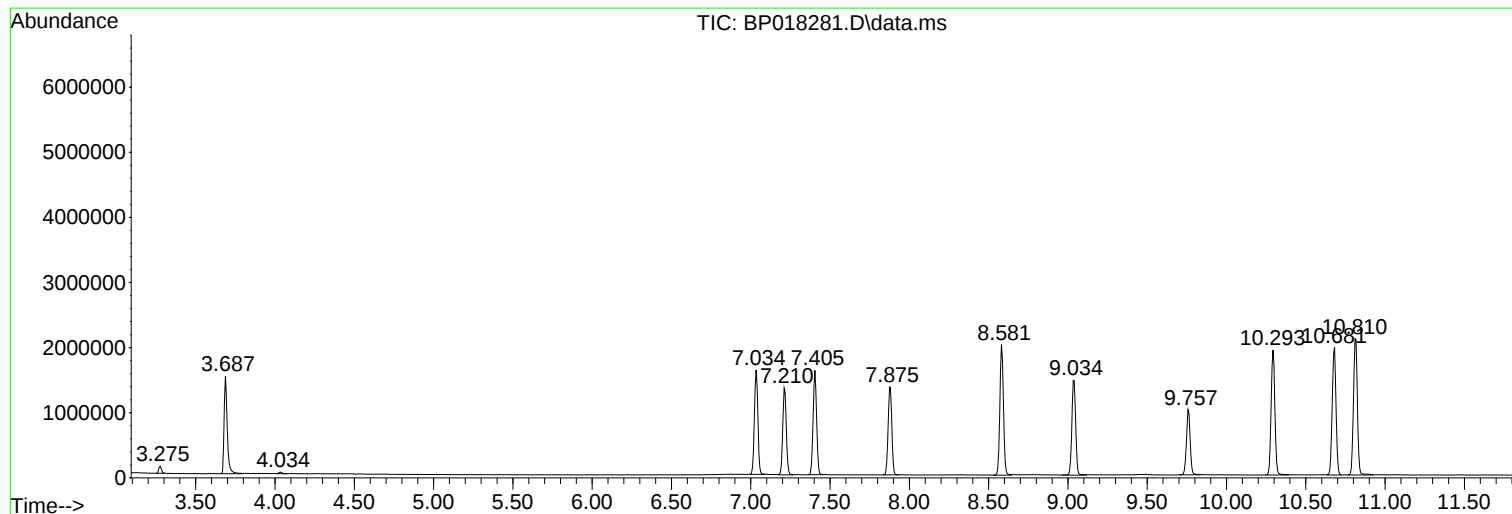

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018281.D
Acq On : 22 Nov 2023 18:38
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018281.D
Acq On : 22 Nov 2023 18:38
Operator : MA/JU
Sample : PB156975BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------