

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018282.D
 Acq On : 22 Nov 2023 19:12
 Operator : MA/JU
 Sample : 05233-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH376

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	36	rBV	95022	114774	0.88%	0.098%
2	3.310	36	38	43	rVB2	17870	21494	0.16%	0.018%
3	3.687	98	102	114	rBV	600081	893971	6.82%	0.766%
4	3.887	132	136	140	rVV3	15000	20787	0.16%	0.018%
5	3.940	141	145	152	rVB	24281	42346	0.32%	0.036%
6	4.034	157	161	166	rVB	21170	30083	0.23%	0.026%
7	6.846	635	639	643	rBV5	10348	17684	0.13%	0.015%
8	7.034	665	671	689	rVB	586990	893435	6.82%	0.766%
9	7.210	694	701	710	rVB	1841353	2932873	22.37%	2.514%
10	7.404	726	734	745	rBV	1759631	2694979	20.56%	2.310%
11	7.510	745	752	759	rVB	10719	27251	0.21%	0.023%
12	7.875	807	814	822	rBV	1366326	2167303	16.53%	1.858%
13	8.581	927	934	943	rBV	1458406	2273779	17.35%	1.949%
14	9.040	1004	1012	1024	rBV	2154537	3527486	26.91%	3.024%
15	9.487	1083	1088	1093	rVB6	10365	20253	0.15%	0.017%
16	9.757	1124	1134	1142	rBV	1472541	2382507	18.17%	2.042%
17	10.292	1218	1225	1240	rBV	2576325	4183289	31.91%	3.586%
18	10.681	1283	1291	1298	rVB	1961669	3309156	25.24%	2.837%
19	10.816	1304	1314	1332	rBV	2637649	4530046	34.56%	3.883%
20	12.263	1554	1560	1566	rBV	55494	83283	0.64%	0.071%
21	12.910	1663	1670	1679	rVB6	11785	35422	0.27%	0.030%
22	13.357	1742	1746	1752	rVV6	9195	13758	0.10%	0.012%
23	13.422	1752	1757	1764	rVV2	50175	81664	0.62%	0.070%
24	13.486	1764	1768	1775	rVB5	12363	20311	0.15%	0.017%
25	13.827	1821	1826	1832	rBV7	12390	24921	0.19%	0.021%
26	13.927	1836	1843	1854	rVV	5734441	7770194	59.27%	6.661%
27	14.204	1881	1890	1899	rBV	6412567	9472631	72.26%	8.121%
28	14.510	1934	1942	1949	rBV	3356230	4867067	37.13%	4.172%
29	14.563	1949	1951	1961	rVB10	16251	37802	0.29%	0.032%
30	14.686	1961	1972	1981	rBV	430600	677765	5.17%	0.581%
31	14.869	1998	2003	2007	rBV8	8196	14271	0.11%	0.012%
32	14.927	2009	2013	2020	rVB7	28115	37475	0.29%	0.032%
33	15.333	2077	2082	2087	rBV7	12164	23062	0.18%	0.020%
34	15.504	2103	2111	2122	rBV	8170413	11692771	89.20%	10.024%
35	15.610	2123	2129	2140	rBV	1491999	2037340	15.54%	1.747%
36	15.739	2148	2151	2156	rVB2	35661	50258	0.38%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018282.D
 Acq On : 22 Nov 2023 19:12
 Operator : MA/JU
 Sample : 05233-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH376

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.292	2241	2245	2249	rVB6	10305	16745	0.13%	0.014%
38	16.939	2351	2355	2363	rVB7	13240	19447	0.15%	0.017%
39	17.039	2368	2372	2376	rBV2	10731	16829	0.13%	0.014%
40	17.145	2385	2390	2395	rBV9	9700	17971	0.14%	0.015%
41	17.257	2402	2409	2419	rBV	3827852	5670567	43.26%	4.861%
42	17.357	2419	2426	2437	rVV2	8322383	12242547	93.39%	10.495%
43	17.633	2469	2473	2476	rVB2	11797	14118	0.11%	0.012%
44	18.163	2558	2563	2572	rBV	241962	375635	2.87%	0.322%
45	18.227	2572	2574	2580	rVB2	15527	25489	0.19%	0.022%
46	18.463	2610	2614	2618	rVB4	17385	21988	0.17%	0.019%
47	19.010	2703	2707	2714	rVB2	35397	49478	0.38%	0.042%
48	19.174	2730	2735	2741	rBV	113219	152754	1.17%	0.131%
49	19.239	2741	2746	2752	rBV	108870	164787	1.26%	0.141%
50	19.398	2769	2773	2782	rBV	171202	255891	1.95%	0.219%
51	19.557	2796	2800	2801	rBV4	20200	22822	0.17%	0.020%
52	19.598	2801	2807	2816	rVB	9974449	13108780	100.00%	11.238%
53	20.598	2975	2977	2983	rVB	48072	52880	0.40%	0.045%
54	21.098	3059	3062	3066	rBV2	59340	68297	0.52%	0.059%
55	21.362	3101	3107	3116	rBV	3435594	4488560	34.24%	3.848%
56	23.627	3484	3492	3506	rBV2	4458396	8920607	68.05%	7.647%
57	23.786	3511	3519	3532	rVB	1907547	3918907	29.90%	3.360%




Sum of corrected areas: 116648590

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018282.D
Acq On : 22 Nov 2023 19:12
Operator : MA/JU
Sample : 05233-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH376

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

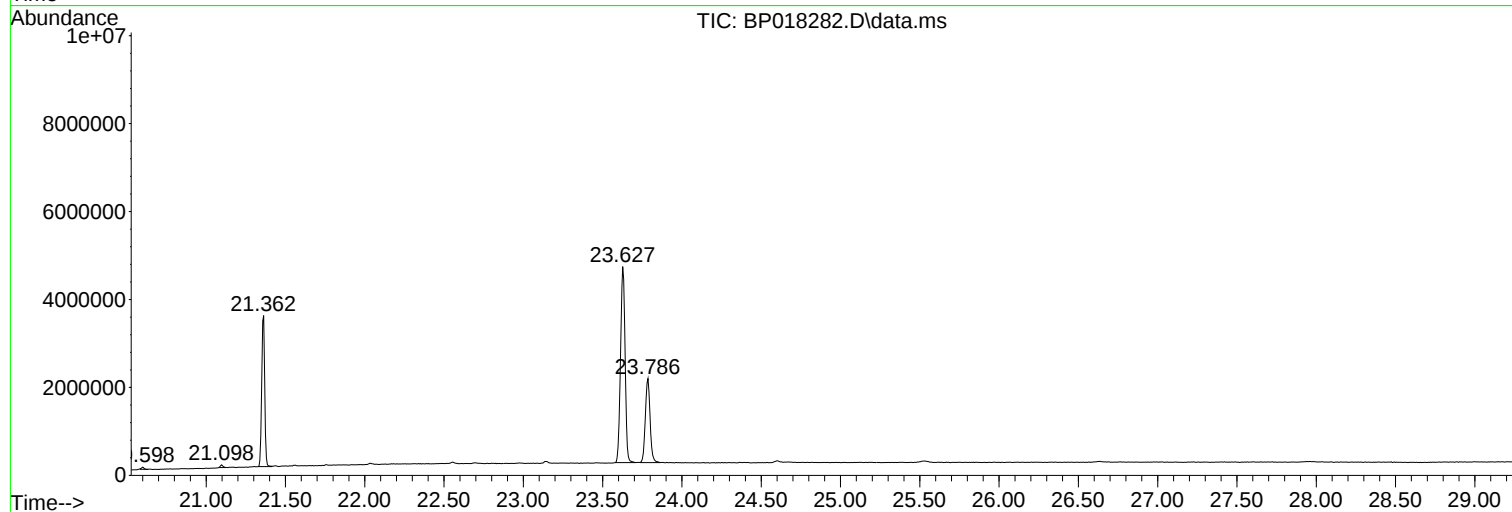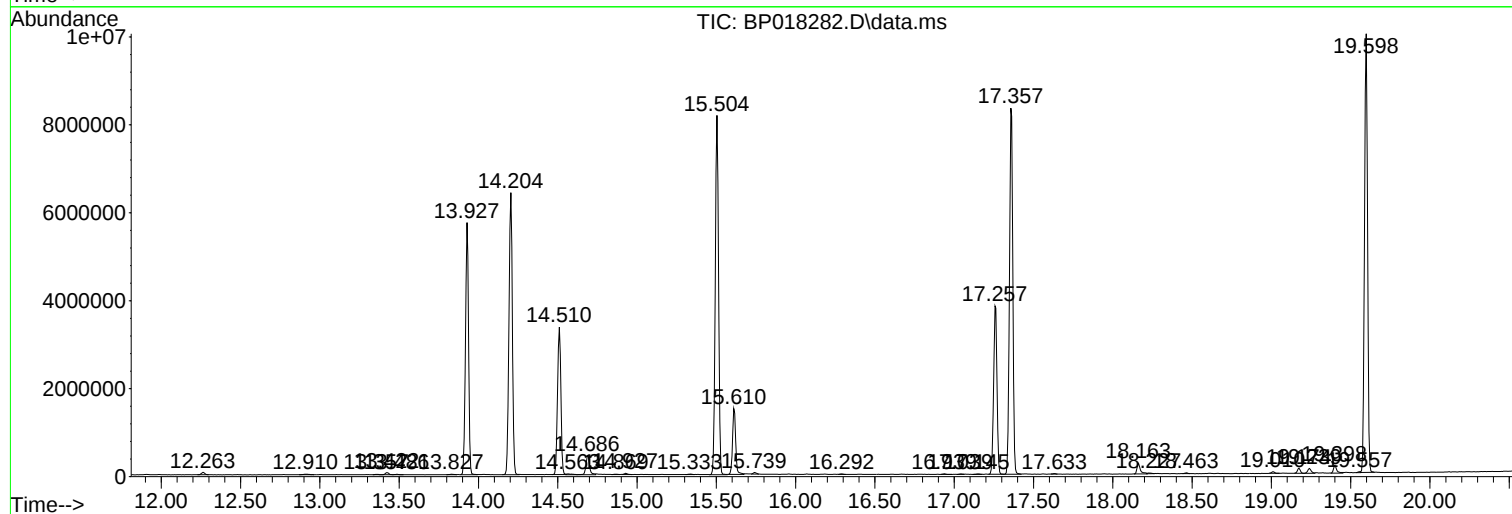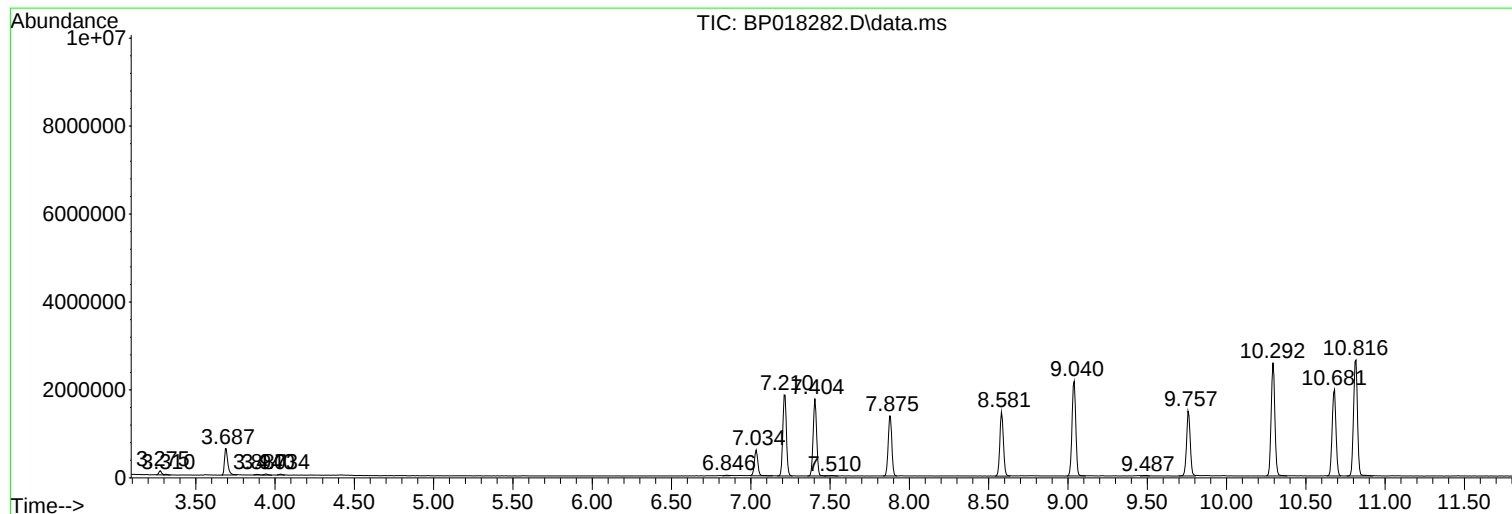

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018282.D
Acq On : 22 Nov 2023 19:12
Operator : MA/JU
Sample : 05233-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH376

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018282.D
Acq On : 22 Nov 2023 19:12
Operator : MA/JU
Sample : 05233-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH376

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
