

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018283.D
 Acq On : 22 Nov 2023 19:46
 Operator : MA/JU
 Sample : 05233-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	36	rBV	76603	102990	0.90%	0.099%
2	3.564	78	81	85	rBV	11741	16493	0.14%	0.016%
3	3.693	99	103	113	rBV	290482	420337	3.67%	0.405%
4	3.887	132	136	139	rBV4	14308	18575	0.16%	0.018%
5	3.940	142	145	151	rVB	19281	30615	0.27%	0.030%
6	4.040	158	162	165	rBV	21404	27824	0.24%	0.027%
7	5.575	418	423	429	rBV10	6095	14571	0.13%	0.014%
8	6.846	636	639	643	rBV6	8368	11567	0.10%	0.011%
9	7.034	664	671	679	rVB	483016	741493	6.47%	0.715%
10	7.211	695	701	710	rVB	1633249	2537070	22.14%	2.445%
11	7.405	726	734	746	rBV	1487595	2309651	20.16%	2.226%
12	7.511	746	752	757	rVB8	8827	20973	0.18%	0.020%
13	7.875	807	814	823	rBV	1415216	2238540	19.54%	2.158%
14	8.581	926	934	952	rBV	1266281	1949144	17.01%	1.879%
15	9.034	1003	1011	1019	rBV	1840141	3033334	26.47%	2.924%
16	9.463	1072	1084	1085	rBV	6783	15721	0.14%	0.015%
17	9.493	1085	1089	1093	rVB7	10380	17019	0.15%	0.016%
18	9.757	1126	1134	1147	rBV	1262463	2017045	17.60%	1.944%
19	10.293	1217	1225	1238	rBV	2201453	3579731	31.24%	3.450%
20	10.681	1278	1291	1298	rVB	1979923	3410368	29.76%	3.287%
21	10.810	1304	1313	1321	rBV	1795020	2998540	26.17%	2.890%
22	11.904	1493	1499	1506	rBV7	9824	20537	0.18%	0.020%
23	12.263	1554	1560	1569	rVB	47402	85262	0.74%	0.082%
24	12.910	1663	1670	1674	rBV6	16253	30734	0.27%	0.030%
25	13.422	1751	1757	1764	rBV	42733	72184	0.63%	0.070%
26	13.487	1764	1768	1774	rVB5	9279	17533	0.15%	0.017%
27	13.828	1820	1826	1831	rBV9	10664	20931	0.18%	0.020%
28	13.928	1836	1843	1849	rBV	5069456	6790014	59.25%	6.545%
29	14.204	1879	1890	1899	rBV	5433820	8123237	70.89%	7.830%
30	14.510	1935	1942	1948	rBV	3409483	4956338	43.25%	4.777%
31	14.563	1948	1951	1958	rVB7	12703	25764	0.22%	0.025%
32	14.687	1966	1972	1979	rBV	369556	547139	4.77%	0.527%
33	14.869	1999	2003	2007	rVB7	8428	13216	0.12%	0.013%
34	14.928	2007	2013	2019	rBV8	25492	40355	0.35%	0.039%
35	15.334	2078	2082	2087	rBV8	12087	17067	0.15%	0.016%
36	15.504	2104	2111	2119	rBV	7083211	10056492	87.76%	9.693%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018283.D
 Acq On : 22 Nov 2023 19:46
 Operator : MA/JU
 Sample : 05233-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.610	2123	2129	2143	rVV	1279050	1785487	15.58%	1.721%
38	15.739	2147	2151	2163	rVB	36124	68004	0.59%	0.066%
39	16.063	2203	2206	2212	rBV6	9274	15841	0.14%	0.015%
40	16.181	2220	2226	2230	rBV9	5927	14482	0.13%	0.014%
41	16.292	2242	2245	2250	rVB7	10554	14731	0.13%	0.014%
42	16.934	2351	2354	2358	rVB5	10090	13782	0.12%	0.013%
43	17.039	2366	2372	2376	rBV5	12850	22546	0.20%	0.022%
44	17.151	2386	2391	2395	rBV8	10995	16230	0.14%	0.016%
45	17.257	2403	2409	2418	rVB	4008485	5674841	49.52%	5.470%
46	17.357	2419	2426	2436	rBV2	7832735	10841561	94.61%	10.450%
47	17.628	2469	2472	2476	rBV	9243	12564	0.11%	0.012%
48	17.951	2522	2527	2531	rBV8	10940	20913	0.18%	0.020%
49	18.157	2558	2562	2572	rBV	213318	349684	3.05%	0.337%
50	18.457	2609	2613	2620	rBV5	16999	25710	0.22%	0.025%
51	19.010	2703	2707	2712	rVB2	28836	39867	0.35%	0.038%
52	19.175	2730	2735	2740	rVB2	100611	133143	1.16%	0.128%
53	19.239	2740	2746	2751	rBV	98619	158810	1.39%	0.153%
54	19.398	2769	2773	2782	rBV	177288	253787	2.21%	0.245%
55	19.551	2796	2799	2801	rBV4	26800	29542	0.26%	0.028%
56	19.598	2801	2807	2813	rVV	8532800	11459123	100.00%	11.045%
57	20.598	2974	2977	2983	rVB	84882	92938	0.81%	0.090%
58	21.092	3059	3061	3067	rVB5	34781	49011	0.43%	0.047%
59	21.357	3101	3106	3117	rBV	3561876	4383750	38.26%	4.225%
60	23.627	3484	3492	3507	rVB	4024278	7954975	69.42%	7.668%
61	23.780	3511	3518	3530	rVB	1943938	3987275	34.80%	3.843%




Sum of corrected areas: 103747001

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018283.D
Acq On : 22 Nov 2023 19:46
Operator : MA/JU
Sample : 05233-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

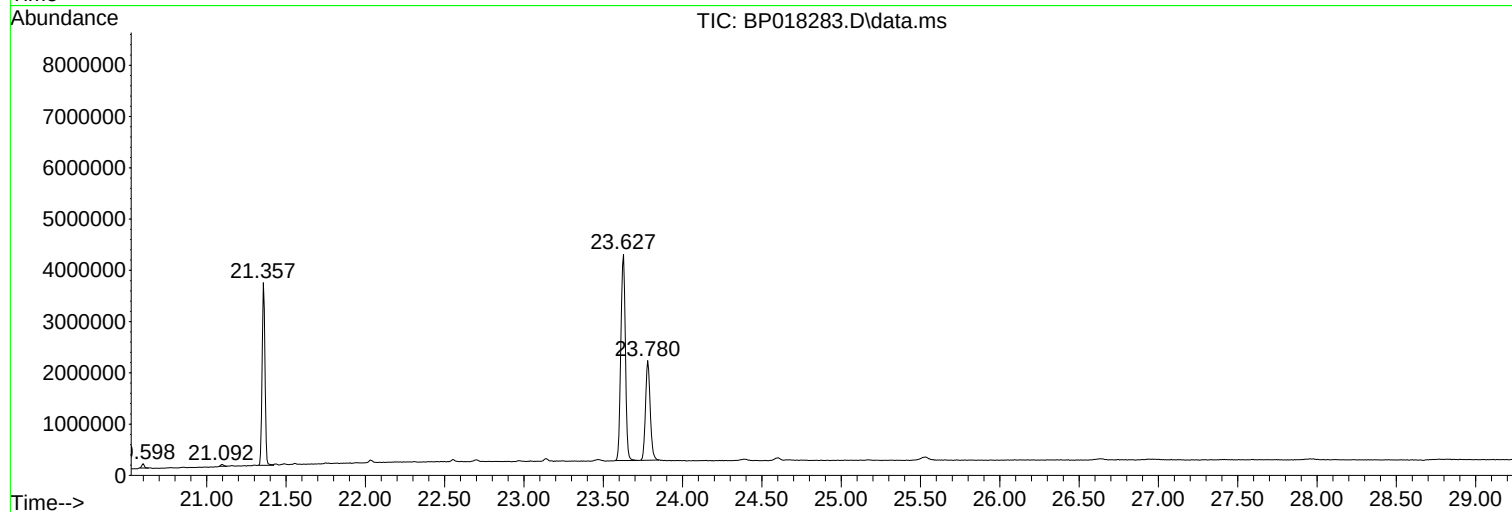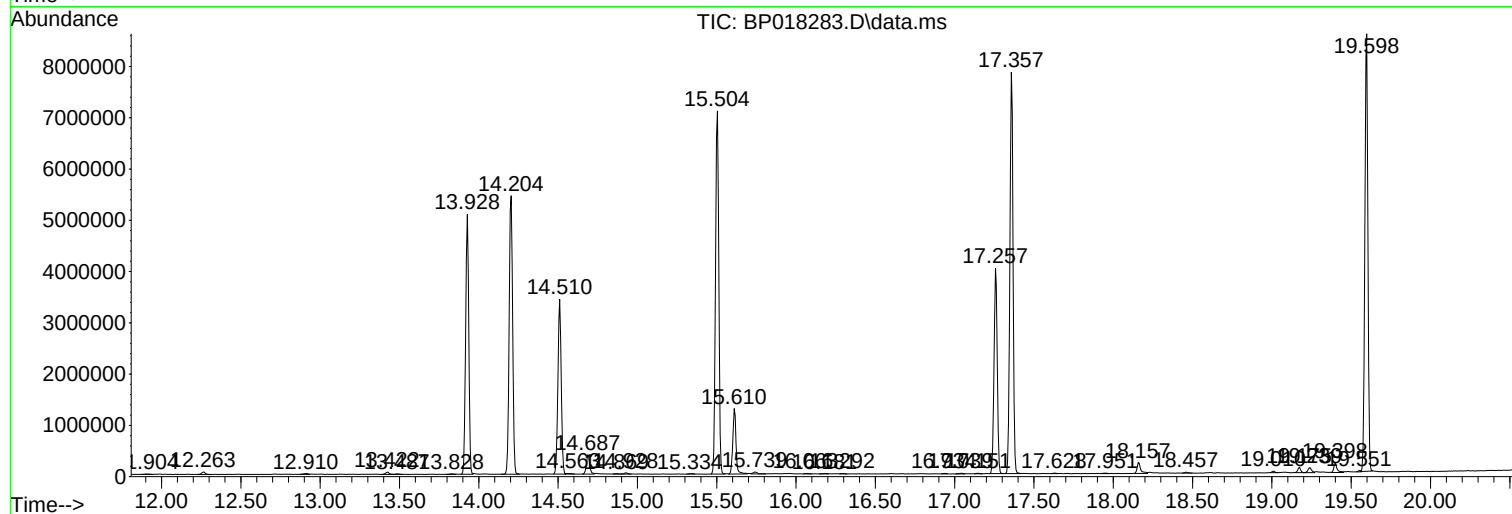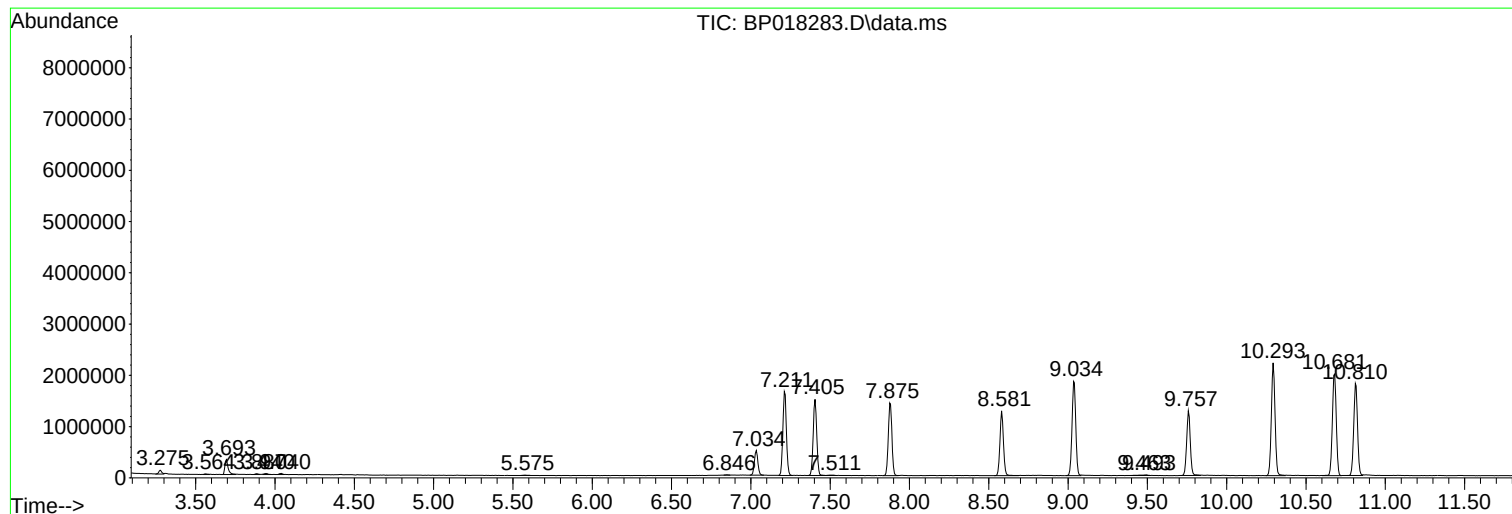

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018283.D
Acq On : 22 Nov 2023 19:46
Operator : MA/JU
Sample : 05233-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018283.D
Acq On : 22 Nov 2023 19:46
Operator : MA/JU
Sample : 05233-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH377

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------