

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018285.D
 Acq On : 22 Nov 2023 20:54
 Operator : MA/JU
 Sample : 05226-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	98287	122680	0.96%	0.110%
2	3.693	98	103	115	rBV	411739	595353	4.65%	0.531%
3	3.940	140	145	153	rVV2	23027	42520	0.33%	0.038%
4	4.034	157	161	166	rVB	24489	33076	0.26%	0.030%
5	7.034	665	671	680	rVB	571323	875373	6.84%	0.781%
6	7.210	694	701	709	rBV	1764907	2687205	20.99%	2.399%
7	7.405	725	734	744	rBV	1607342	2499729	19.53%	2.231%
8	7.516	748	753	758	rVB9	10039	17768	0.14%	0.016%
9	7.875	808	814	822	rBV	1396575	2180061	17.03%	1.946%
10	8.581	925	934	943	rBV	1428530	2193120	17.13%	1.958%
11	9.034	1004	1011	1021	rBV	1953288	3201070	25.01%	2.857%
12	9.487	1082	1088	1098	rVB4	17353	40377	0.32%	0.036%
13	9.757	1127	1134	1143	rBV	1386339	2136937	16.70%	1.908%
14	10.293	1217	1225	1236	rBV	2380498	3859639	30.15%	3.445%
15	10.675	1279	1290	1298	rBV	2005677	3348935	26.16%	2.989%
16	10.810	1304	1313	1322	rBV	2209685	3730995	29.15%	3.331%
17	11.987	1507	1513	1520	rVB8	14990	28184	0.22%	0.025%
18	12.263	1555	1560	1570	rVB	48077	82172	0.64%	0.073%
19	12.881	1660	1665	1675	rBV2	49575	107257	0.84%	0.096%
20	13.128	1700	1707	1713	rVB	44280	67671	0.53%	0.060%
21	13.357	1741	1746	1752	rVB9	8722	13001	0.10%	0.012%
22	13.422	1752	1757	1762	rVV	34763	54898	0.43%	0.049%
23	13.481	1764	1767	1773	rVB5	10450	17183	0.13%	0.015%
24	13.828	1822	1826	1833	rBV9	11033	21701	0.17%	0.019%
25	13.928	1836	1843	1849	rBV	5555695	7473139	58.39%	6.671%
26	14.204	1881	1890	1897	rBV	6054529	8766643	68.49%	7.826%
27	14.510	1934	1942	1949	rBV	3270455	4856861	37.95%	4.336%
28	14.581	1952	1954	1959	rVB6	11751	14564	0.11%	0.013%
29	14.687	1965	1972	1988	rBV	461741	703337	5.49%	0.628%
30	14.922	2008	2012	2018	rVV8	21591	34809	0.27%	0.031%
31	15.004	2022	2026	2032	rVB5	15537	26179	0.20%	0.023%
32	15.334	2076	2082	2088	rBV8	13952	27523	0.22%	0.025%
33	15.504	2102	2111	2122	rBV	7615866	11142168	87.05%	9.946%
34	15.610	2123	2129	2143	rVV	1597630	2123599	16.59%	1.896%
35	15.739	2147	2151	2157	rVB2	36332	58635	0.46%	0.052%
36	16.069	2202	2207	2212	rVB7	10196	17411	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018285.D
 Acq On : 22 Nov 2023 20:54
 Operator : MA/JU
 Sample : 05226-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG87

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.286	2241	2244	2248	rVB5	12585	17747	0.14%	0.016%
38	16.604	2293	2298	2304	rVB9	7820	14855	0.12%	0.013%
39	16.933	2350	2354	2358	rBV6	14023	19490	0.15%	0.017%
40	17.151	2387	2391	2395	rVB6	9579	14786	0.12%	0.013%
41	17.257	2402	2409	2417	rBV	3927584	5435843	42.47%	4.852%
42	17.357	2419	2426	2438	rVV2	8541247	12323795	96.28%	11.001%
43	17.557	2456	2460	2465	rBV3	8411	14436	0.11%	0.013%
44	17.628	2465	2472	2476	rBV2	13988	27559	0.22%	0.025%
45	18.157	2558	2562	2572	rBV2	136882	217646	1.70%	0.194%
46	18.463	2608	2614	2621	rBV8	16375	36499	0.29%	0.033%
47	19.010	2703	2707	2713	rVB4	29321	42785	0.33%	0.038%
48	19.169	2730	2734	2739	rBV	109923	148295	1.16%	0.132%
49	19.239	2741	2746	2751	rVV	99853	143656	1.12%	0.128%
50	19.398	2769	2773	2778	rBV2	96883	119379	0.93%	0.107%
51	19.551	2796	2799	2800	rBV3	18661	19179	0.15%	0.017%
52	19.598	2801	2807	2813	rVV	9491761	12799643	100.00%	11.426%
53	20.598	2974	2977	2983	rVB2	56741	65530	0.51%	0.058%
54	21.092	3058	3061	3064	rBV3	49826	60045	0.47%	0.054%
55	21.357	3101	3106	3116	rBV	3219000	4021892	31.42%	3.590%
56	23.627	3484	3492	3509	rVB2	4839803	9433059	73.70%	8.421%
57	23.780	3511	3518	3530	rVB	1809464	3845728	30.05%	3.433%




Sum of corrected areas: 112023620

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018285.D
Acq On : 22 Nov 2023 20:54
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

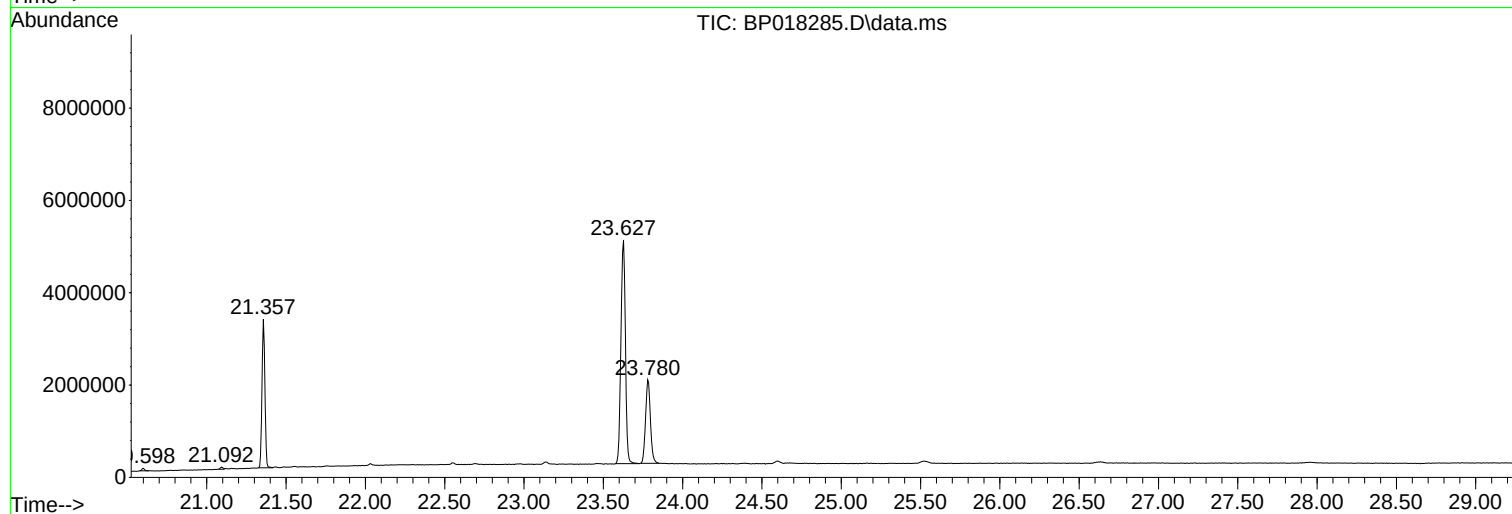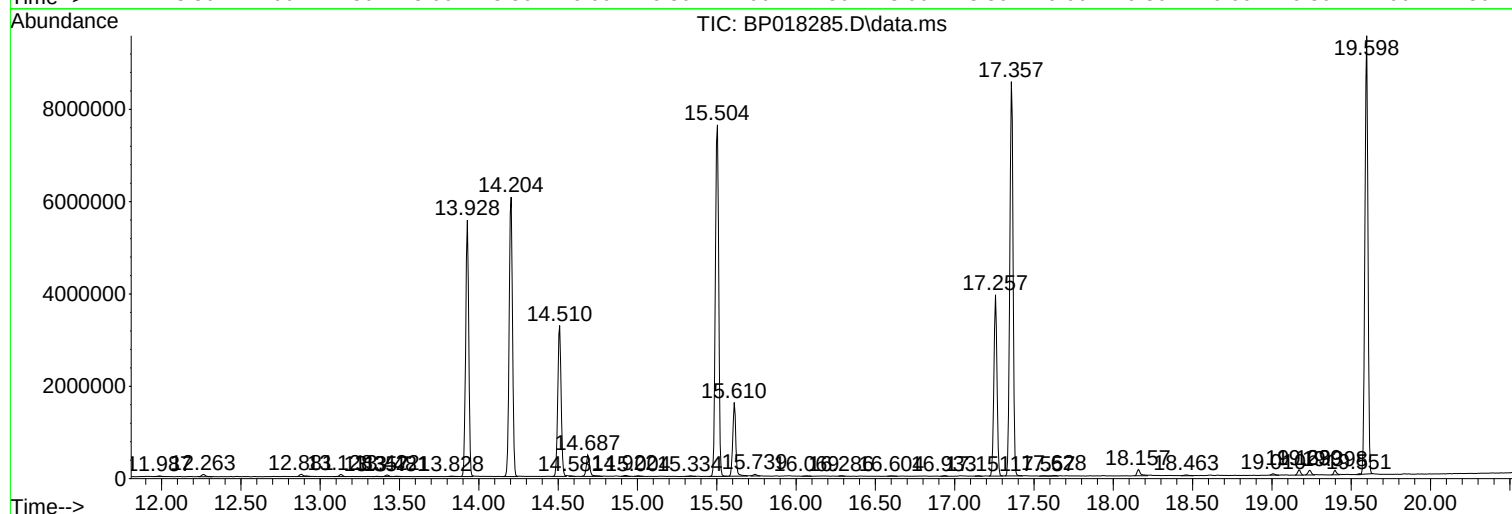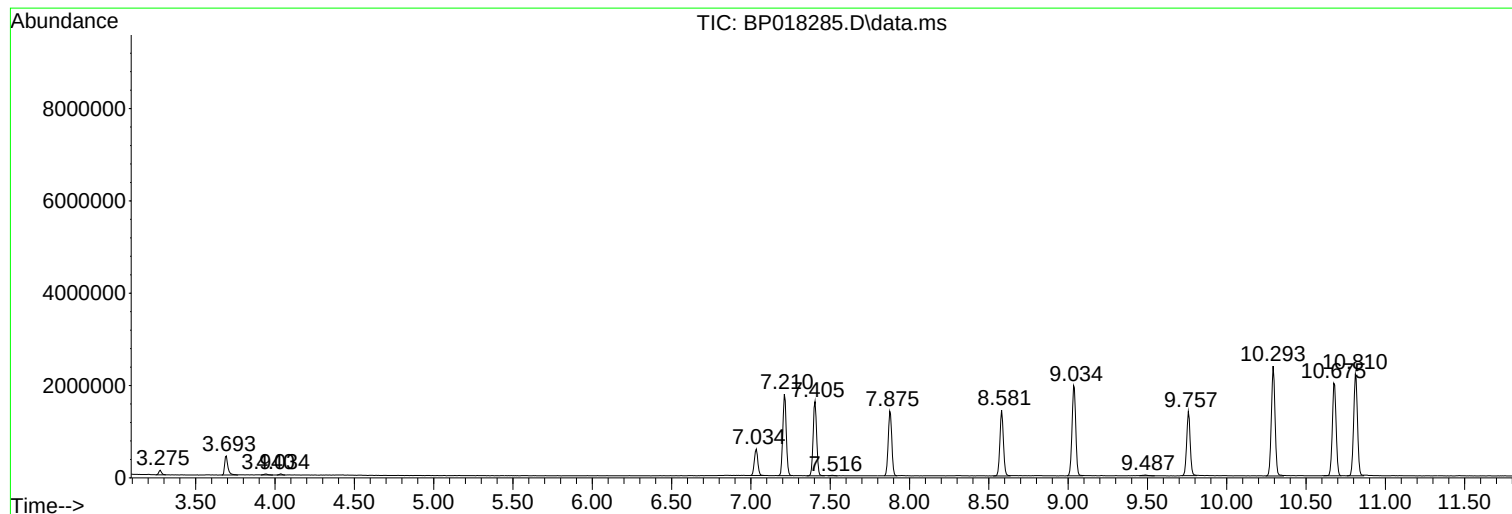

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018285.D
Acq On : 22 Nov 2023 20:54
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018285.D
Acq On : 22 Nov 2023 20:54
Operator : MA/JU
Sample : 05226-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG87

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
