

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018289.D
 Acq On : 22 Nov 2023 23:10
 Operator : MA/JU
 Sample : 05226-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	38	rVB	99000	120385	1.09%	0.111%
2	3.564	78	81	84	rBV3	9370	13993	0.13%	0.013%
3	3.687	98	102	118	rBV	585166	874475	7.90%	0.806%
4	3.940	141	145	150	rVB2	26878	41018	0.37%	0.038%
5	4.034	157	161	167	rBV	27035	39111	0.35%	0.036%
6	4.970	315	320	328	rVB4	22837	42509	0.38%	0.039%
7	5.575	418	423	426	rBV7	7718	13688	0.12%	0.013%
8	6.275	538	542	546	rBV5	11585	18718	0.17%	0.017%
9	6.852	635	640	643	rBV7	6691	11293	0.10%	0.010%
10	7.034	665	671	688	rVB	583611	927445	8.38%	0.855%
11	7.211	694	701	711	rVB	1948876	2965582	26.79%	2.734%
12	7.405	725	734	743	rBV	1698740	2678948	24.20%	2.470%
13	7.875	806	814	823	rBV	1517737	2370794	21.41%	2.186%
14	7.946	823	826	833	rVB5	9590	18056	0.16%	0.017%
15	8.469	911	915	923	rVB5	16740	29512	0.27%	0.027%
16	8.581	927	934	945	rBV	1493387	2293527	20.72%	2.115%
17	9.034	1003	1011	1021	rBV	2138119	3508795	31.69%	3.235%
18	9.481	1084	1087	1095	rVB4	18641	38432	0.35%	0.035%
19	9.758	1124	1134	1142	rBV	1451782	2318100	20.94%	2.137%
20	10.293	1217	1225	1239	rBV	2485119	4048635	36.57%	3.733%
21	10.675	1282	1290	1299	rVB	2117339	3536748	31.94%	3.261%
22	10.810	1303	1313	1326	rBV	2274727	3874225	34.99%	3.572%
23	11.463	1419	1424	1427	rBV7	6978	13067	0.12%	0.012%
24	11.893	1494	1497	1504	rBV9	5894	13046	0.12%	0.012%
25	11.981	1504	1512	1518	rBV2	25936	43709	0.39%	0.040%
26	12.263	1554	1560	1567	rVB2	55509	90421	0.82%	0.083%
27	12.881	1660	1665	1668	rBV2	19326	32886	0.30%	0.030%
28	13.134	1704	1708	1713	rVB5	14902	20969	0.19%	0.019%
29	13.422	1751	1757	1761	rBV3	42223	67730	0.61%	0.062%
30	13.481	1763	1767	1771	rVB4	10210	12667	0.11%	0.012%
31	13.834	1822	1827	1830	rBV7	9137	16472	0.15%	0.015%
32	13.928	1835	1843	1855	rVV	5128651	7239360	65.39%	6.674%
33	14.199	1881	1889	1899	rBV	5845593	8815547	79.62%	8.128%
34	14.510	1932	1942	1948	rBV	3197932	4887167	44.14%	4.506%
35	14.687	1963	1972	1979	rBV	362896	538690	4.87%	0.497%
36	14.928	2006	2013	2020	rVB	19557	35037	0.32%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018289.D
 Acq On : 22 Nov 2023 23:10
 Operator : MA/JU
 Sample : 05226-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	15.334	2076	2082	2087	rBV6	14794	26621	0.24%	0.025%
38	15.498	2103	2110	2120	rBV	7466966	10770806	97.28%	9.930%
39	15.610	2123	2129	2142	rBV	1282454	1768747	15.98%	1.631%
40	15.740	2147	2151	2158	rVB	35522	59856	0.54%	0.055%
41	16.063	2202	2206	2213	rBV8	10345	19720	0.18%	0.018%
42	16.287	2239	2244	2247	rVB7	9966	15828	0.14%	0.015%
43	16.769	2322	2326	2331	rBV8	7559	14020	0.13%	0.013%
44	16.928	2351	2353	2359	rVB7	10936	17149	0.15%	0.016%
45	17.040	2368	2372	2377	rBV3	16745	25843	0.23%	0.024%
46	17.145	2385	2390	2395	rBV9	10047	15480	0.14%	0.014%
47	17.257	2402	2409	2415	rBV	3687673	5222385	47.17%	4.815%
48	17.357	2418	2426	2436	rBV	7954378	11071590	100.00%	10.208%
49	17.563	2457	2461	2466	rVB6	6887	11701	0.11%	0.011%
50	17.628	2466	2472	2475	rBV2	12471	17714	0.16%	0.016%
51	17.945	2522	2526	2530	rBV4	15129	23681	0.21%	0.022%
52	18.157	2557	2562	2569	rBV	146385	209445	1.89%	0.193%
53	18.451	2608	2612	2617	rBV6	16384	25241	0.23%	0.023%
54	19.169	2730	2734	2740	rVB	97430	129093	1.17%	0.119%
55	19.239	2741	2746	2750	rBV	80382	112552	1.02%	0.104%
56	19.398	2769	2773	2781	rBV2	70477	102913	0.93%	0.095%
57	19.551	2796	2799	2800	rBV2	14137	12806	0.12%	0.012%
58	19.592	2800	2806	2823	rVB	8237459	10709416	96.73%	9.874%
59	19.828	2842	2846	2849	rBV	38255	50416	0.46%	0.046%
60	20.598	2973	2977	2981	rVB	89547	103327	0.93%	0.095%
61	21.092	3057	3061	3065	rBV4	83528	118033	1.07%	0.109%
62	21.357	3101	3106	3115	rBV	2929361	3657384	33.03%	3.372%
63	23.622	3483	3491	3506	rBV2	4307280	8629385	77.94%	7.956%
64	23.780	3510	3518	3528	rBV	1895499	3913152	35.34%	3.608%




Sum of corrected areas: 108465061

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018289.D
Acq On : 22 Nov 2023 23:10
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

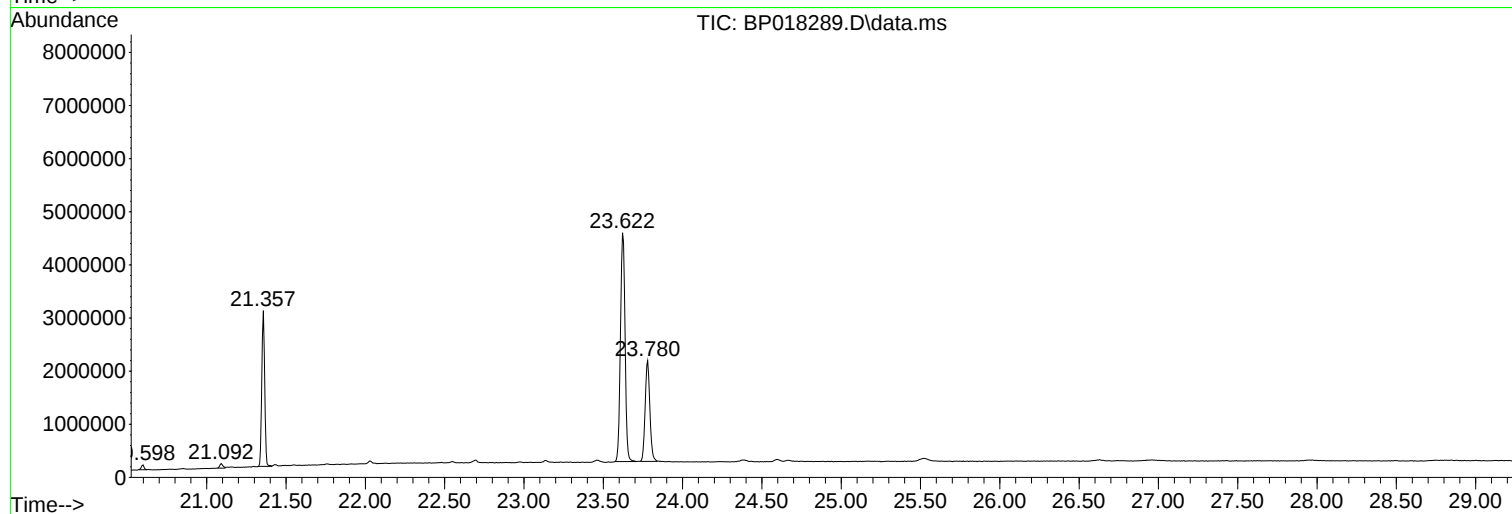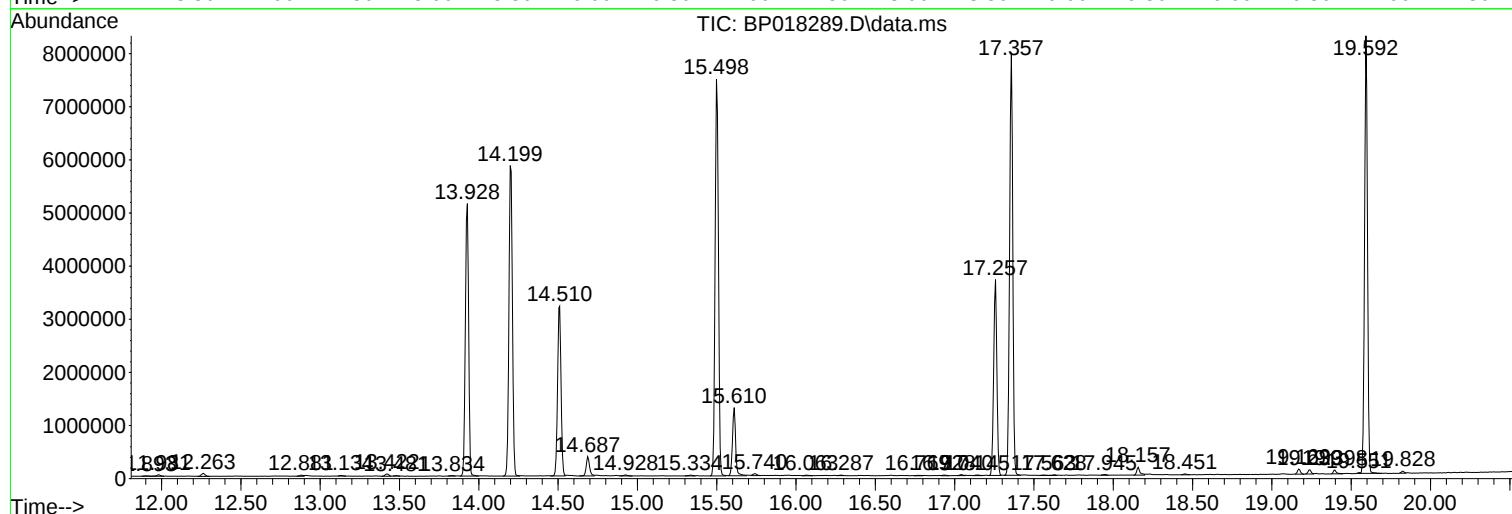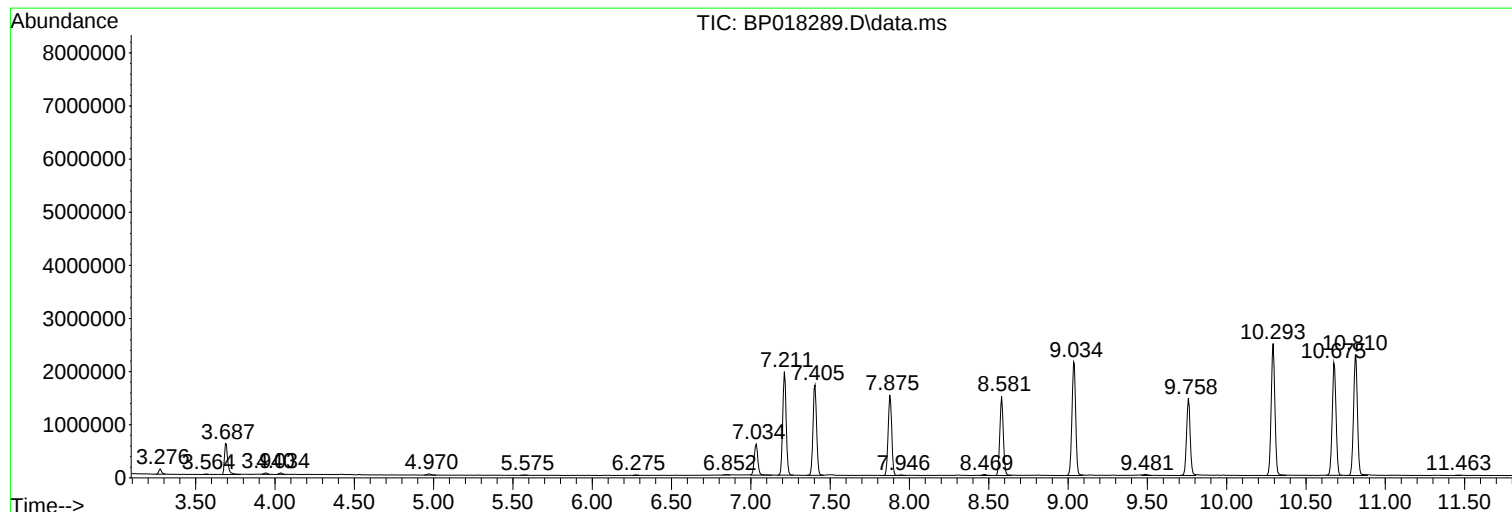

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018289.D
Acq On : 22 Nov 2023 23:10
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018289.D
Acq On : 22 Nov 2023 23:10
Operator : MA/JU
Sample : 05226-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
