

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018292.D
 Acq On : 23 Nov 2023 00:52
 Operator : MA/JU
 Sample : 05226-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	38	rVB	95854	120845	1.15%	0.116%
2	3.687	99	102	114	rBV	584091	839457	7.99%	0.807%
3	3.940	141	145	154	rVB2	29507	50692	0.48%	0.049%
4	4.034	157	161	168	rVB	25521	39828	0.38%	0.038%
5	4.411	223	225	232	rVB7	8687	11880	0.11%	0.011%
6	5.093	338	341	348	rVB9	8241	11534	0.11%	0.011%
7	5.187	352	357	362	rVB4	13120	19792	0.19%	0.019%
8	6.846	634	639	642	rBV7	6875	13566	0.13%	0.013%
9	7.034	665	671	678	rVB	578415	881868	8.40%	0.847%
10	7.211	694	701	712	rVB	1894792	2846027	27.09%	2.735%
11	7.405	725	734	743	rBV	1644718	2613584	24.88%	2.511%
12	7.516	746	753	755	rVB7	9079	16131	0.15%	0.016%
13	7.875	805	814	822	rBV	1499969	2287531	21.78%	2.198%
14	8.475	912	916	922	rVB9	5747	11060	0.11%	0.011%
15	8.581	922	934	945	rBV	1456093	2284024	21.74%	2.195%
16	9.034	1003	1011	1023	rBV	2063800	3335699	31.75%	3.205%
17	9.216	1036	1042	1046	rVB9	8998	11148	0.11%	0.011%
18	9.487	1080	1088	1096	rVB	55408	101875	0.97%	0.098%
19	9.758	1124	1134	1148	rBV	1359407	2216694	21.10%	2.130%
20	9.969	1169	1170	1180	rVB10	6255	11087	0.11%	0.011%
21	10.293	1215	1225	1240	rBV	2385211	3873523	36.87%	3.722%
22	10.422	1242	1247	1251	rVB7	9032	17140	0.16%	0.016%
23	10.675	1277	1290	1298	rBV	2020940	3397297	32.34%	3.264%
24	10.810	1305	1313	1324	rBV	2465292	4032092	38.38%	3.874%
25	11.457	1419	1423	1427	rBV7	9042	11377	0.11%	0.011%
26	11.904	1494	1499	1504	rBV8	7066	14249	0.14%	0.014%
27	11.981	1507	1512	1517	rVV2	31112	47821	0.46%	0.046%
28	12.263	1553	1560	1567	rBV2	49885	83011	0.79%	0.080%
29	12.651	1620	1626	1631	rVB7	10732	21073	0.20%	0.020%
30	12.710	1631	1636	1640	rBV7	9412	18455	0.18%	0.018%
31	12.875	1658	1664	1666	rBV5	11549	16885	0.16%	0.016%
32	13.128	1703	1707	1713	rVB7	14096	22854	0.22%	0.022%
33	13.422	1751	1757	1763	rVV	71555	109892	1.05%	0.106%
34	13.481	1763	1767	1774	rVB5	11689	17390	0.17%	0.017%
35	13.822	1820	1825	1830	rBV8	10142	17785	0.17%	0.017%
36	13.922	1836	1842	1848	rBV	4966317	6931096	65.98%	6.660%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018292.D
 Acq On : 23 Nov 2023 00:52
 Operator : MA/JU
 Sample : 05226-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	14.198	1880	1889	1897	rBV	5513145	8278081	78.80%	7.954%
38	14.504	1932	1941	1948	rBV	3093942	4600824	43.80%	4.421%
39	14.687	1967	1972	1987	rVV	362333	544389	5.18%	0.523%
40	14.869	1996	2003	2007	rVV10	5950	12434	0.12%	0.012%
41	14.928	2009	2013	2020	rVB9	24741	37171	0.35%	0.036%
42	15.140	2046	2049	2054	rBV5	9295	15911	0.15%	0.015%
43	15.334	2076	2082	2089	rBV3	28266	56594	0.54%	0.054%
44	15.498	2103	2110	2119	rBV	6923570	10326571	98.30%	9.923%
45	15.610	2122	2129	2143	rVV	1216295	1712972	16.31%	1.646%
46	15.740	2147	2151	2157	rVB2	34579	58478	0.56%	0.056%
47	15.869	2170	2173	2177	rBV6	8894	13582	0.13%	0.013%
48	16.069	2202	2207	2211	rBV6	8089	11571	0.11%	0.011%
49	16.281	2240	2243	2249	rVB6	8800	12298	0.12%	0.012%
50	16.410	2262	2265	2272	rVB8	10341	19178	0.18%	0.018%
51	16.934	2351	2354	2358	rVB6	10226	14373	0.14%	0.014%
52	17.039	2367	2372	2377	rBV4	10066	20099	0.19%	0.019%
53	17.145	2385	2390	2392	rBV6	9248	14022	0.13%	0.013%
54	17.257	2402	2409	2415	rBV	3412708	4801844	45.71%	4.614%
55	17.357	2419	2426	2436	rVV	7475619	10504660	100.00%	10.094%
56	17.445	2439	2441	2445	rVB5	9498	11537	0.11%	0.011%
57	17.557	2457	2460	2465	rVB3	11099	13599	0.13%	0.013%
58	17.634	2469	2473	2476	rVB2	8029	10745	0.10%	0.010%
59	17.910	2516	2520	2524	rBV	36853	49821	0.47%	0.048%
60	18.157	2557	2562	2567	rBV2	76850	115319	1.10%	0.111%
61	18.228	2571	2574	2579	rVB	24558	30791	0.29%	0.030%
62	18.463	2609	2614	2618	rBV8	10418	19241	0.18%	0.018%
63	19.010	2700	2707	2708	rBV7	11615	22947	0.22%	0.022%
64	19.033	2708	2711	2714	rVB	26159	28480	0.27%	0.027%
65	19.169	2729	2734	2740	rBV2	87980	118797	1.13%	0.114%
66	19.233	2741	2745	2750	rBV	76377	112318	1.07%	0.108%
67	19.392	2768	2772	2779	rBV3	58366	84940	0.81%	0.082%
68	19.545	2796	2798	2800	rBV3	14312	15855	0.15%	0.015%
69	19.592	2800	2806	2817	rVB	7730111	10080014	95.96%	9.686%
70	20.592	2974	2976	2980	rVB3	44679	48260	0.46%	0.046%
71	21.357	3101	3106	3113	rBV	2691349	3389808	32.27%	3.257%
72	23.621	3483	3491	3506	rBV2	4445013	8719283	83.00%	8.378%
73	23.780	3510	3518	3534	rVB	1784338	3787753	36.06%	3.640%




Sum of corrected areas: 104070822

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018292.D
Acq On : 23 Nov 2023 00:52
Operator : MA/JU
Sample : 05226-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

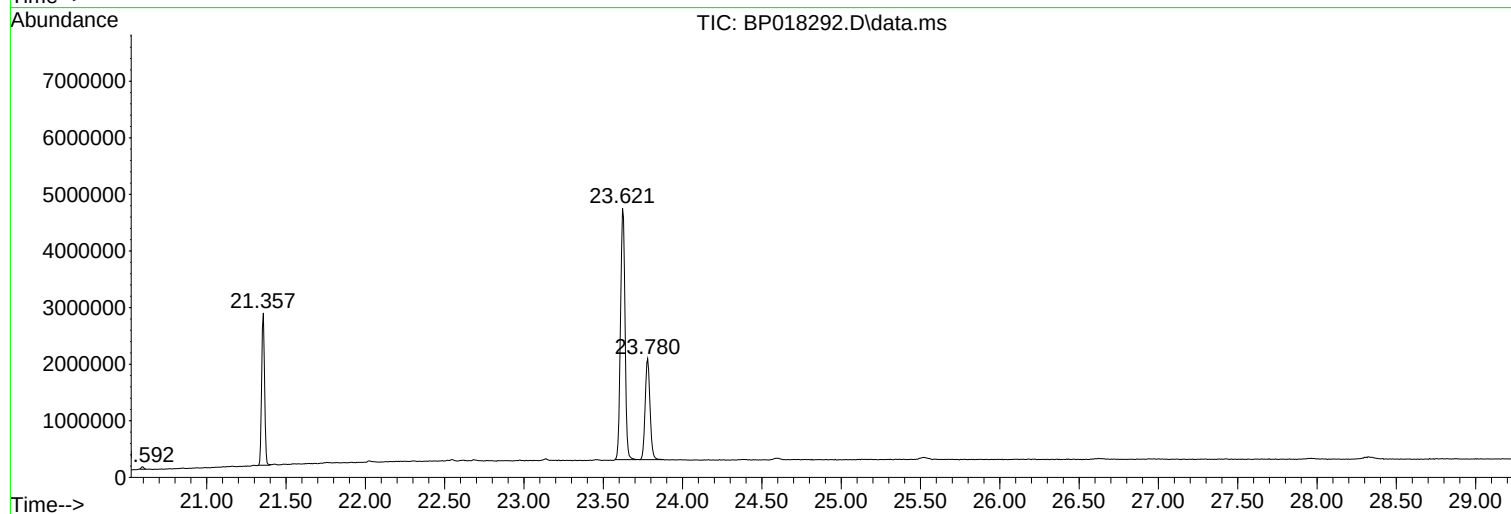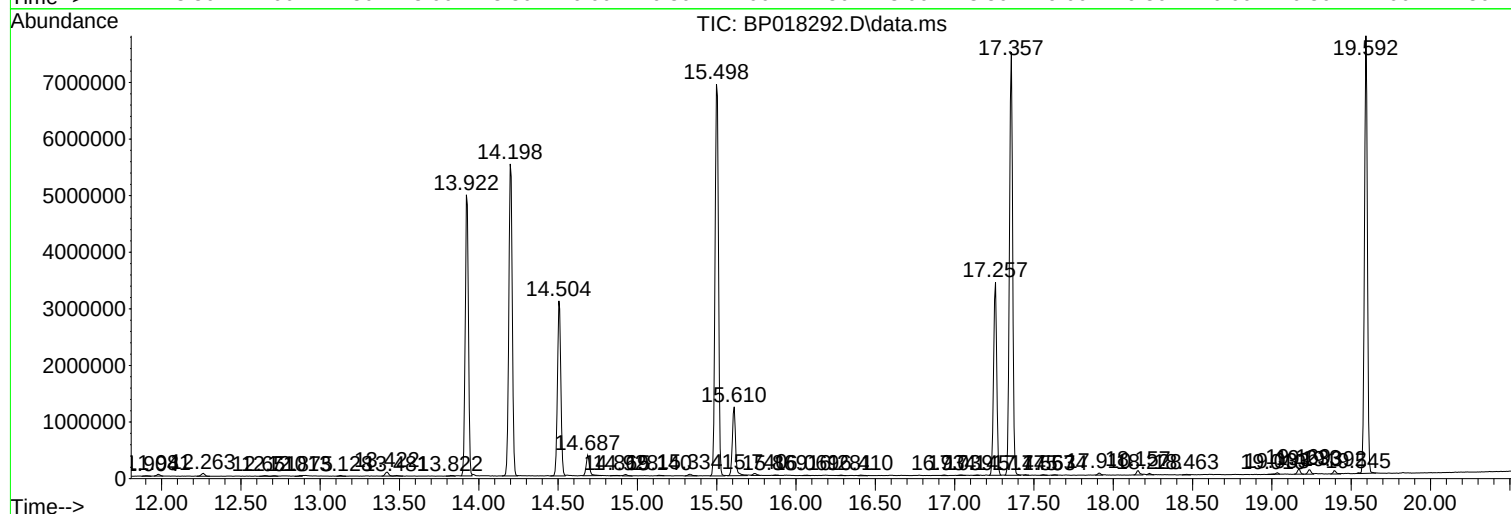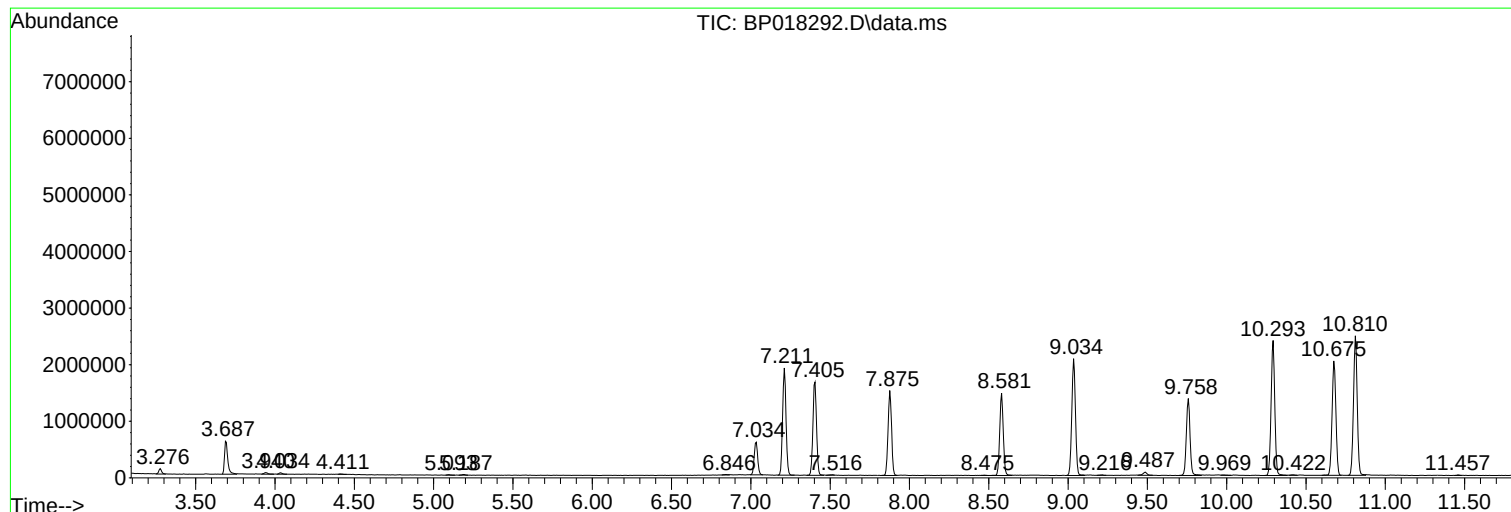

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018292.D
Acq On : 23 Nov 2023 00:52
Operator : MA/JU
Sample : 05226-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018292.D
Acq On : 23 Nov 2023 00:52
Operator : MA/JU
Sample : 05226-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------