

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018297.D
 Acq On : 23 Nov 2023 03:41
 Operator : MA/JU
 Sample : PB156976BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	40	rVB	131048	167247	1.75%	0.159%
2	3.687	98	102	117	rBV	1723628	2403168	25.20%	2.283%
3	4.034	158	161	170	rVB	24675	40079	0.42%	0.038%
4	4.528	240	245	248	rBV5	7106	14792	0.16%	0.014%
5	6.840	631	638	639	rBV7	6506	11383	0.12%	0.011%
6	7.034	664	671	679	rBV	1830915	2821504	29.59%	2.681%
7	7.210	694	701	709	rVB	1573647	2395330	25.12%	2.276%
8	7.405	724	734	744	rBV	1790192	2907757	30.49%	2.763%
9	7.875	804	814	823	rBV	1433882	2275753	23.87%	2.162%
10	8.581	926	934	943	rBV	2361075	3704729	38.85%	3.520%
11	9.034	1003	1011	1021	rBV	1788166	2825424	29.63%	2.684%
12	9.487	1085	1088	1094	rVB8	9442	14050	0.15%	0.013%
13	9.757	1123	1134	1143	rBV	1247867	2031696	21.31%	1.930%
14	10.293	1215	1225	1238	rBV	2281080	3768999	39.53%	3.581%
15	10.675	1283	1290	1299	rVB	2050027	3418457	35.85%	3.248%
16	10.810	1304	1313	1322	rBV	2533497	4142720	43.45%	3.936%
17	12.257	1553	1559	1567	rVB	48981	82632	0.87%	0.079%
18	12.904	1663	1669	1675	rBV9	11059	23596	0.25%	0.022%
19	13.416	1751	1756	1762	rBV	47373	74292	0.78%	0.071%
20	13.481	1762	1767	1773	rVB7	7096	14409	0.15%	0.014%
21	13.828	1822	1826	1828	rBV3	8088	11705	0.12%	0.011%
22	13.922	1835	1842	1854	rBV	4569450	6317177	66.25%	6.002%
23	14.198	1879	1889	1896	rBV	5278283	7619229	79.90%	7.239%
24	14.504	1933	1941	1948	rBV	3442422	4977286	52.20%	4.729%
25	14.692	1966	1973	1987	rBV	1562580	2336953	24.51%	2.220%
26	14.863	2000	2002	2006	rVB4	8454	10054	0.11%	0.010%
27	14.922	2008	2012	2016	rVB7	11892	18625	0.20%	0.018%
28	15.498	2103	2110	2122	rBV	6662161	9294887	97.48%	8.831%
29	15.610	2122	2129	2146	rVV	1078370	1544563	16.20%	1.468%
30	15.739	2146	2151	2157	rVB2	30034	52262	0.55%	0.050%
31	16.069	2204	2207	2211	rVB5	8214	9996	0.10%	0.009%
32	16.181	2220	2226	2231	rBV10	4939	11395	0.12%	0.011%
33	16.281	2240	2243	2250	rVB9	10001	15399	0.16%	0.015%
34	16.933	2351	2354	2357	rVB5	10473	11851	0.12%	0.011%
35	17.033	2366	2371	2374	rBV3	11842	18188	0.19%	0.017%
36	17.145	2386	2390	2394	rVB7	6671	10246	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018297.D
 Acq On : 23 Nov 2023 03:41
 Operator : MA/JU
 Sample : PB156976BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.257	2402	2409	2416	rBV	3962088	5634015	59.08%	5.353%
38	17.357	2419	2426	2440	rVB	6774187	9476407	99.38%	9.004%
39	17.628	2469	2472	2475	rBV2	7733	9838	0.10%	0.009%
40	18.151	2558	2561	2567	rBV8	17464	36861	0.39%	0.035%
41	19.169	2730	2734	2740	rVB2	76667	106262	1.11%	0.101%
42	19.233	2741	2745	2751	rVV	76581	100714	1.06%	0.096%
43	19.392	2770	2772	2776	rVB4	12524	13409	0.14%	0.013%
44	19.545	2795	2798	2800	rBV3	26466	28297	0.30%	0.027%
45	19.592	2800	2806	2816	rVB	7245470	9535446	100.00%	9.060%
46	20.592	2973	2976	2982	rVB	56827	67342	0.71%	0.064%
47	21.357	3101	3106	3112	rBV	3322425	4069832	42.68%	3.867%
48	23.621	3483	3491	3505	rVB2	3514071	6817444	71.50%	6.477%
49	23.774	3510	3517	3529	rVB	1928682	3957139	41.50%	3.760%




Sum of corrected areas: 105250839

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018297.D
Acq On : 23 Nov 2023 03:41
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

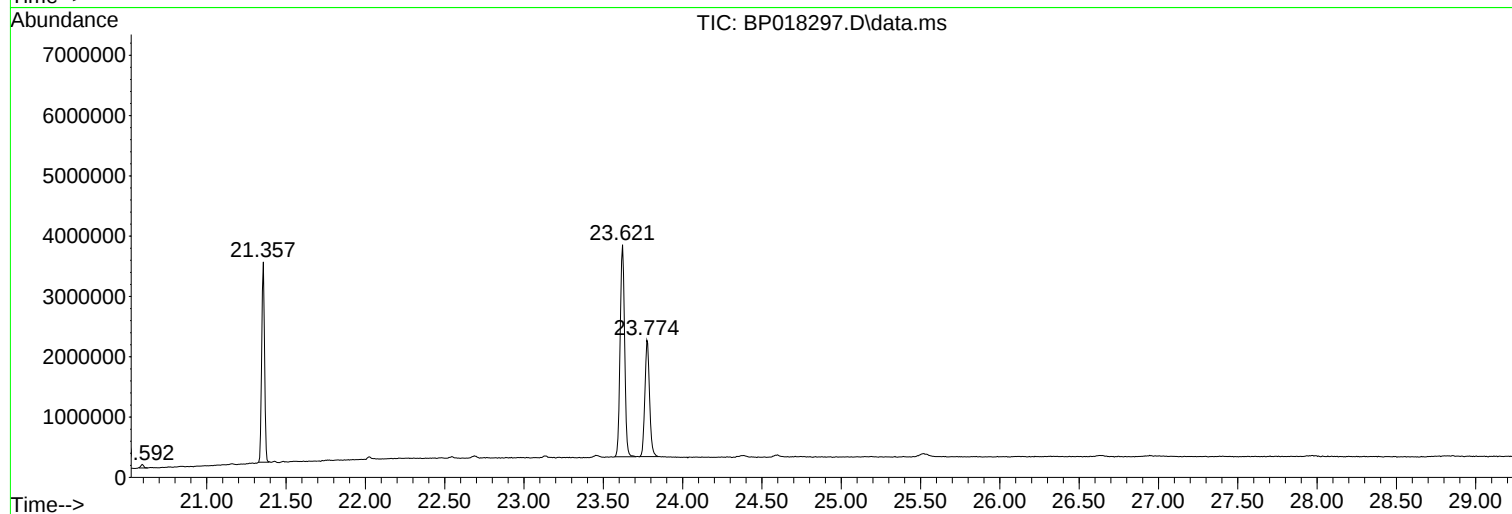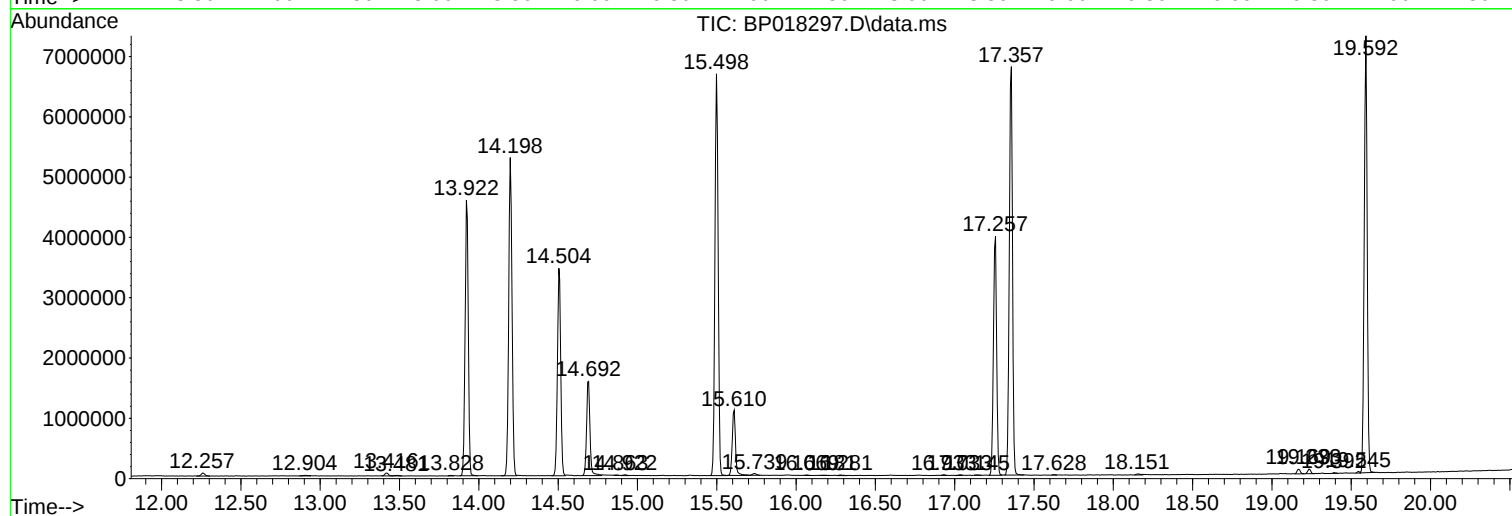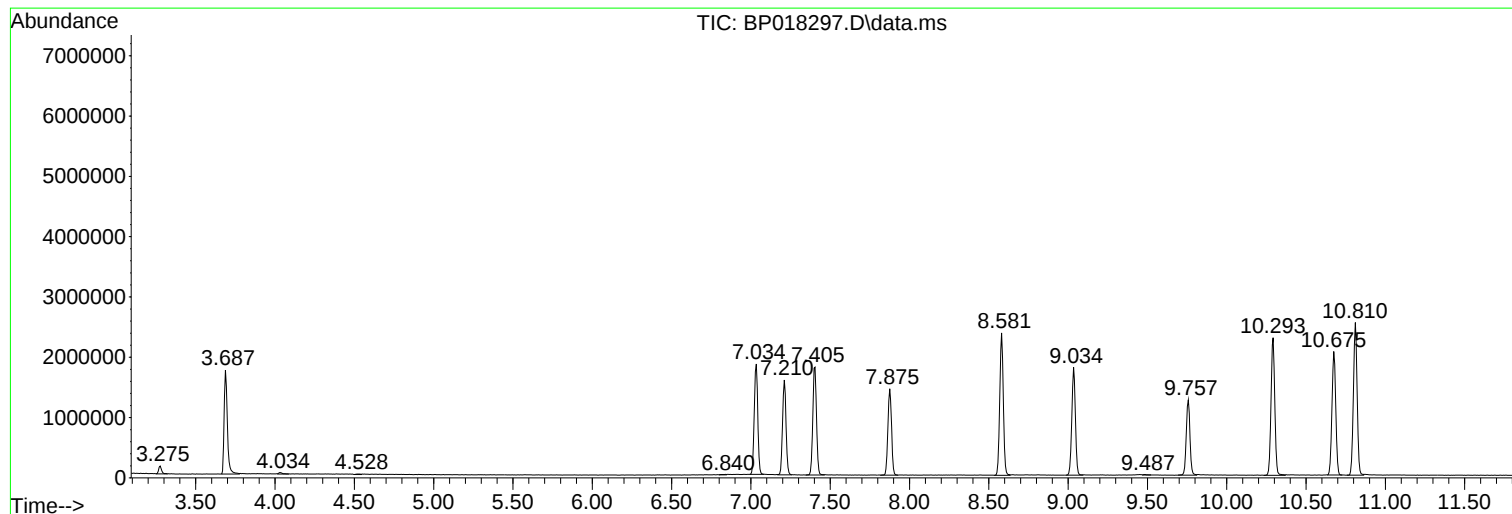

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018297.D
Acq On : 23 Nov 2023 03:41
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018297.D
Acq On : 23 Nov 2023 03:41
Operator : MA/JU
Sample : PB156976BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------