

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018299.D
 Acq On : 23 Nov 2023 05:23
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	41	rVB	127927	164149	1.84%	0.159%
2	3.687	98	102	114	rBV	1649677	2287668	25.64%	2.214%
3	4.034	157	161	167	rVB	26053	38290	0.43%	0.037%
4	4.540	241	247	248	rBV3	9774	11663	0.13%	0.011%
5	7.034	663	671	685	rVB	1750115	2740982	30.72%	2.652%
6	7.210	694	701	711	rVB	1502532	2305182	25.84%	2.231%
7	7.399	726	733	744	rBV	1768291	2782353	31.18%	2.692%
8	7.875	805	814	825	rBV	1645528	2516688	28.21%	2.435%
9	8.581	926	934	947	rBV	2229371	3516138	39.41%	3.402%
10	9.034	1003	1011	1025	rBV	1690866	2704881	30.32%	2.617%
11	9.757	1121	1134	1147	rBV	1176064	1927903	21.61%	1.865%
12	10.293	1214	1225	1236	rBV	2192062	3595210	40.29%	3.479%
13	10.675	1282	1290	1299	rVB	2289303	3756046	42.10%	3.634%
14	10.810	1305	1313	1330	rBV	2416527	3979472	44.60%	3.851%
15	11.898	1488	1498	1500	rBV	6929	12076	0.14%	0.012%
16	11.975	1507	1511	1519	rVB10	6357	13990	0.16%	0.014%
17	12.263	1554	1560	1568	rVB	46740	75858	0.85%	0.073%
18	12.904	1661	1669	1679	rBV9	12055	33187	0.37%	0.032%
19	13.416	1750	1756	1762	rBV2	47886	82546	0.93%	0.080%
20	13.481	1764	1767	1773	rVB7	7943	11371	0.13%	0.011%
21	13.822	1821	1825	1832	rBV7	8211	16226	0.18%	0.016%
22	13.922	1835	1842	1853	rBV	4328413	5967819	66.89%	5.775%
23	14.198	1881	1889	1899	rBV	5045524	7207488	80.78%	6.974%
24	14.504	1934	1941	1948	rBV	3773614	5438383	60.95%	5.262%
25	14.687	1965	1972	1989	rBV	1462923	2198136	24.64%	2.127%
26	14.922	2008	2012	2017	rVB7	9660	13854	0.16%	0.013%
27	15.334	2079	2082	2086	rVB6	7553	9099	0.10%	0.009%
28	15.498	2103	2110	2118	rBV	6290331	8812087	98.76%	8.527%
29	15.604	2122	2128	2140	rBV	973451	1414042	15.85%	1.368%
30	15.739	2146	2151	2156	rVB2	28382	44277	0.50%	0.043%
31	15.945	2184	2186	2191	rVB6	6760	9545	0.11%	0.009%
32	16.069	2202	2207	2213	rVB10	6583	10825	0.12%	0.010%
33	16.592	2292	2296	2300	rBV5	5077	9371	0.11%	0.009%
34	16.928	2350	2353	2358	rVB7	9993	13271	0.15%	0.013%
35	17.039	2368	2372	2377	rBV2	10686	16549	0.19%	0.016%
36	17.257	2402	2409	2418	rBV	4219297	6109636	68.48%	5.912%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018299.D
 Acq On : 23 Nov 2023 05:23
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.351	2419	2425	2438	rVV2	6174278	8882787	99.56%	8.595%
38	18.151	2556	2561	2565	rBV8	21258	37670	0.42%	0.036%
39	19.169	2730	2734	2738	rBV	77358	96380	1.08%	0.093%
40	19.233	2741	2745	2751	rBV	68776	95198	1.07%	0.092%
41	19.592	2800	2806	2812	rBV	6894184	8922295	100.00%	8.633%
42	20.592	2973	2976	2981	rVB3	43176	49128	0.55%	0.048%
43	21.357	3100	3106	3115	rBV	3419663	4494941	50.38%	4.349%
44	23.621	3483	3491	3507	rVB	3289147	6524692	73.13%	6.313%
45	23.774	3510	3517	3532	rVB	2093710	4398022	49.29%	4.256%




Sum of corrected areas: 103347374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018299.D
Acq On : 23 Nov 2023 05:23
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

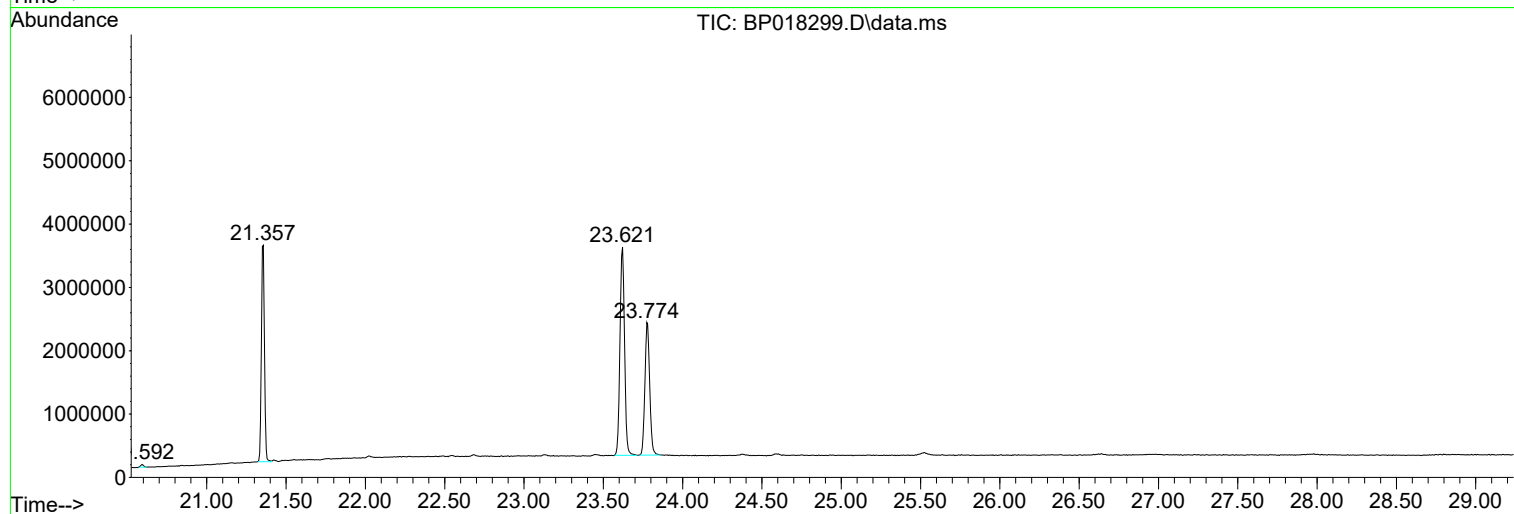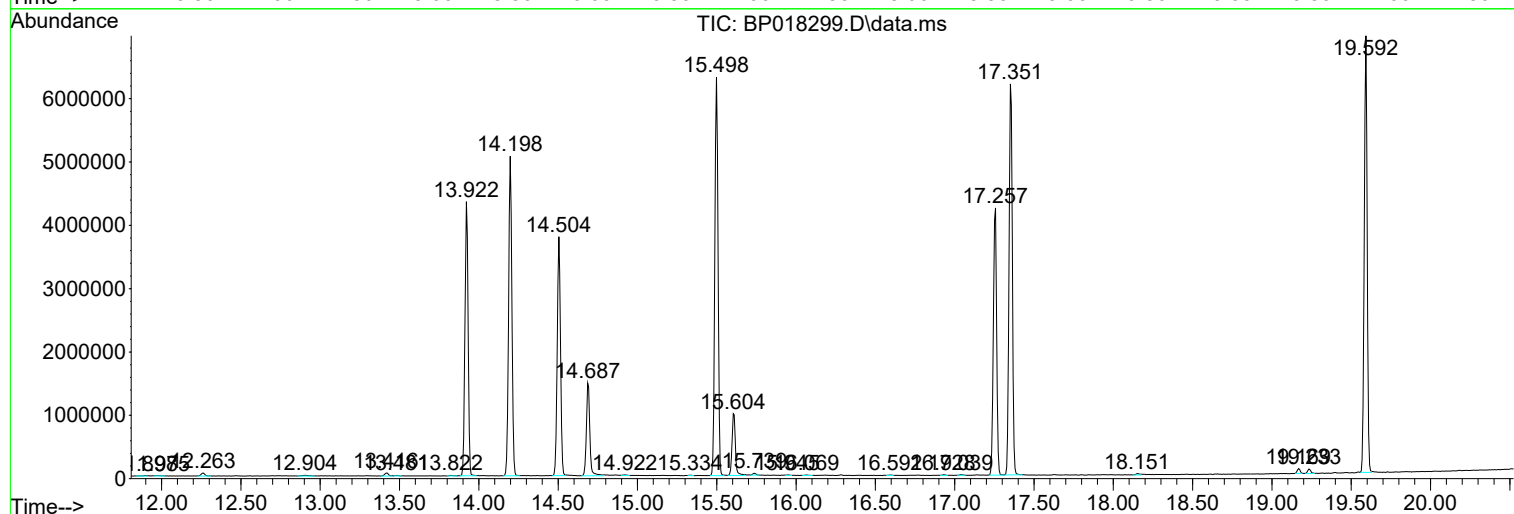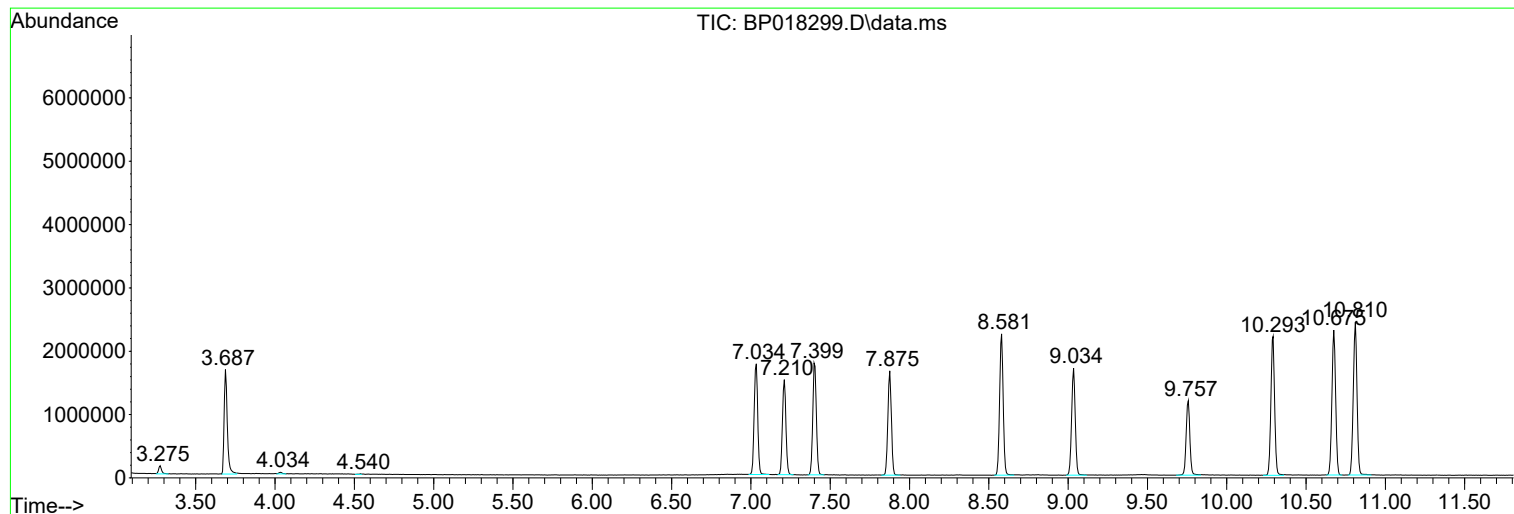

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018299.D
Acq On : 23 Nov 2023 05:23
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018299.D
Acq On : 23 Nov 2023 05:23
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------