

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018300.D
 Acq On : 23 Nov 2023 05:57
 Operator : MA/JU
 Sample : PB157217BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	40	rVB	165979	207811	1.77%	0.162%
2	3.687	98	102	120	rBV	2202956	3055343	26.02%	2.378%
3	4.034	157	161	167	rVB2	25681	36134	0.31%	0.028%
4	4.264	196	200	203	rVB6	15562	20617	0.18%	0.016%
5	4.675	268	270	274	rVB5	10200	11807	0.10%	0.009%
6	7.034	664	671	683	rBV	2407061	3694355	31.46%	2.875%
7	7.210	694	701	710	rVB	2047323	3116902	26.54%	2.426%
8	7.405	725	734	748	rBV	2337153	3774830	32.15%	2.937%
9	7.875	807	814	822	rBV	1726589	2632119	22.42%	2.048%
10	8.581	926	934	947	rBV	3022713	4735850	40.33%	3.685%
11	9.034	1003	1011	1027	rBV	2245745	3655196	31.13%	2.844%
12	9.757	1123	1134	1147	rBV	1637852	2625177	22.36%	2.043%
13	10.287	1216	1224	1236	rBV	2929607	4808785	40.95%	3.742%
14	10.675	1282	1290	1302	rVB	2350688	3907821	33.28%	3.041%
15	10.810	1305	1313	1324	rBV	3125370	5239655	44.62%	4.077%
16	11.893	1493	1497	1503	rBV9	6546	14333	0.12%	0.011%
17	11.975	1505	1511	1516	rVB9	5098	11786	0.10%	0.009%
18	12.257	1554	1559	1566	rBV2	58045	99082	0.84%	0.077%
19	12.898	1661	1668	1679	rBV2	10363	28074	0.24%	0.022%
20	13.416	1751	1756	1762	rBV	63405	103920	0.88%	0.081%
21	13.481	1762	1767	1772	rVV4	9453	15504	0.13%	0.012%
22	13.922	1835	1842	1856	rVV	5627556	7826099	66.65%	6.090%
23	14.198	1879	1889	1898	rBV	6340503	9456227	80.53%	7.359%
24	14.504	1934	1941	1948	rBV	3769782	5493451	46.78%	4.275%
25	14.692	1965	1973	1986	rBV	2060373	2983155	25.40%	2.321%
26	14.922	2008	2012	2017	rVB7	12828	20440	0.17%	0.016%
27	15.334	2078	2082	2088	rVB8	8093	12270	0.10%	0.010%
28	15.498	2103	2110	2118	rBV	8028383	11477295	97.74%	8.931%
29	15.610	2122	2129	2143	rVV	1503373	2042757	17.40%	1.590%
30	15.739	2147	2151	2156	rVB2	37399	60019	0.51%	0.047%
31	15.945	2180	2186	2190	rBV9	6462	14094	0.12%	0.011%
32	16.063	2202	2206	2212	rVB6	9775	17975	0.15%	0.014%
33	16.281	2239	2243	2247	rVB8	8798	12753	0.11%	0.010%
34	16.928	2350	2353	2358	rVB4	11309	14987	0.13%	0.012%
35	17.039	2366	2372	2378	rBV2	12093	17642	0.15%	0.014%
36	17.139	2385	2389	2395	rVB7	9984	17200	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018300.D
 Acq On : 23 Nov 2023 05:57
 Operator : MA/JU
 Sample : PB157217BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK217

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.257	2402	2409	2416	rBV	4332382	6196696	52.77%	4.822%
38	17.357	2419	2426	2436	rBV	7853469	11319634	96.40%	8.809%
39	18.151	2557	2561	2566	rBV6	19529	35959	0.31%	0.028%
40	18.457	2609	2613	2621	rBV4	21327	36788	0.31%	0.029%
41	19.004	2702	2706	2713	rBV3	30816	49005	0.42%	0.038%
42	19.169	2730	2734	2740	rBV	100422	131823	1.12%	0.103%
43	19.233	2740	2745	2750	rBV	95751	131241	1.12%	0.102%
44	19.392	2770	2772	2777	rVB5	13571	17546	0.15%	0.014%
45	19.592	2800	2806	2816	rVB	9195075	11742643	100.00%	9.138%
46	21.357	3101	3106	3116	rVB	3568130	4456409	37.95%	3.468%
47	23.621	3483	3491	3506	rBV2	4303217	8648759	73.65%	6.730%
48	23.780	3511	3518	3530	rVB	2144370	4477117	38.13%	3.484%




Sum of corrected areas: 128505085

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018300.D
Acq On : 23 Nov 2023 05:57
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

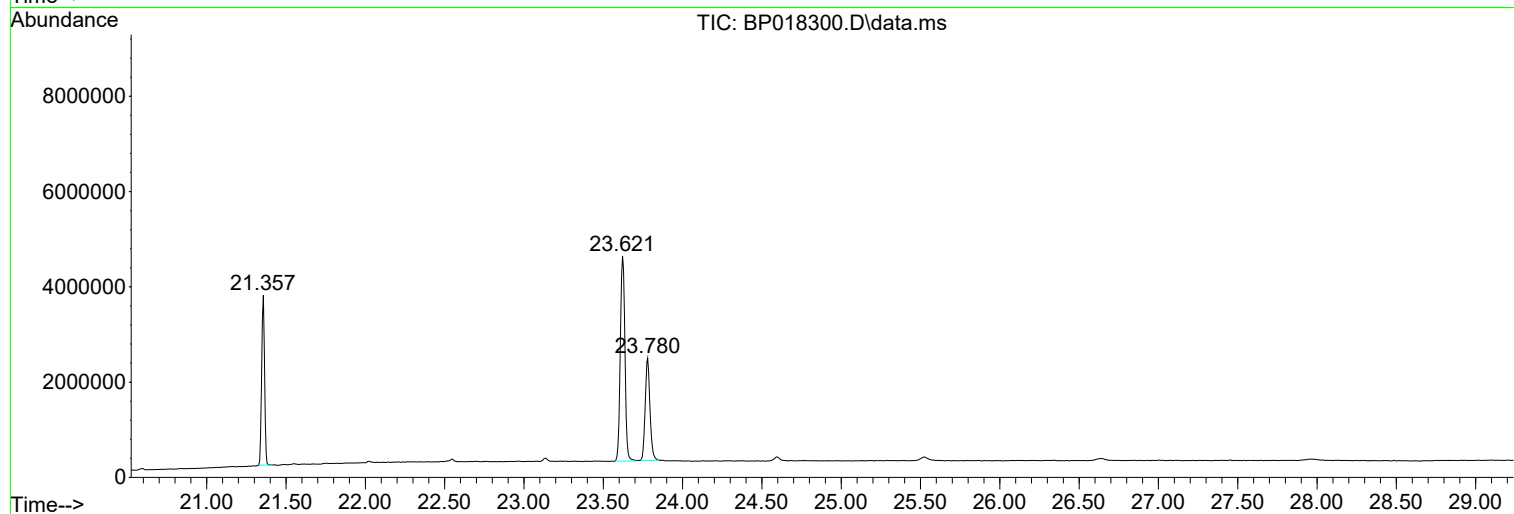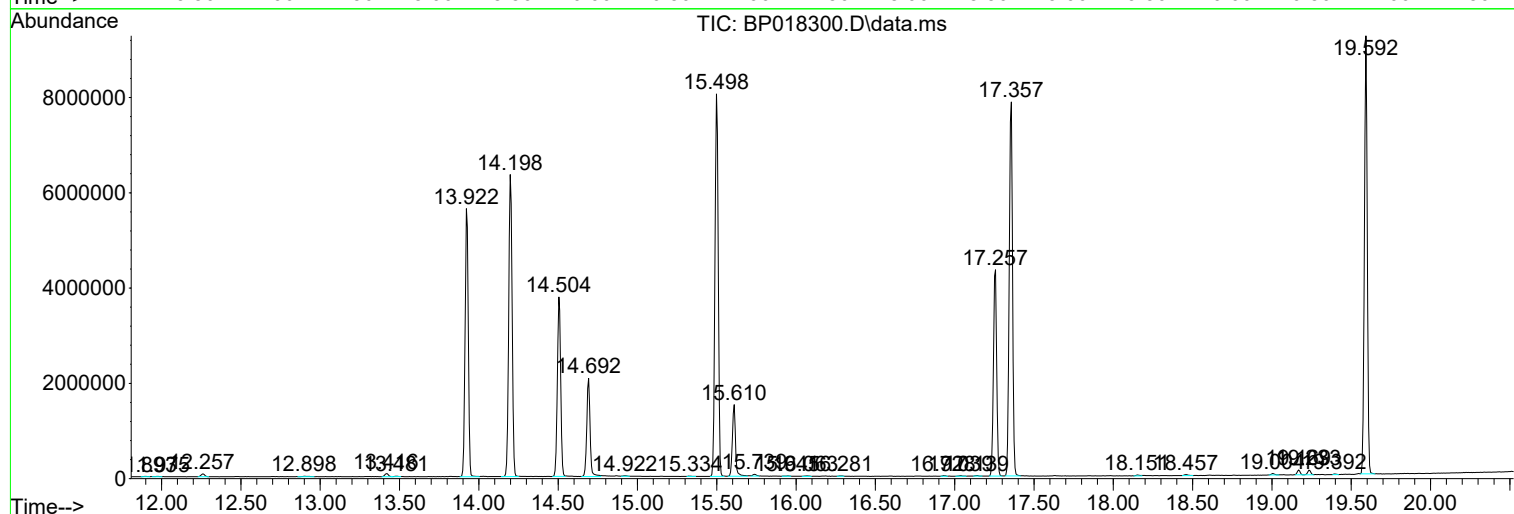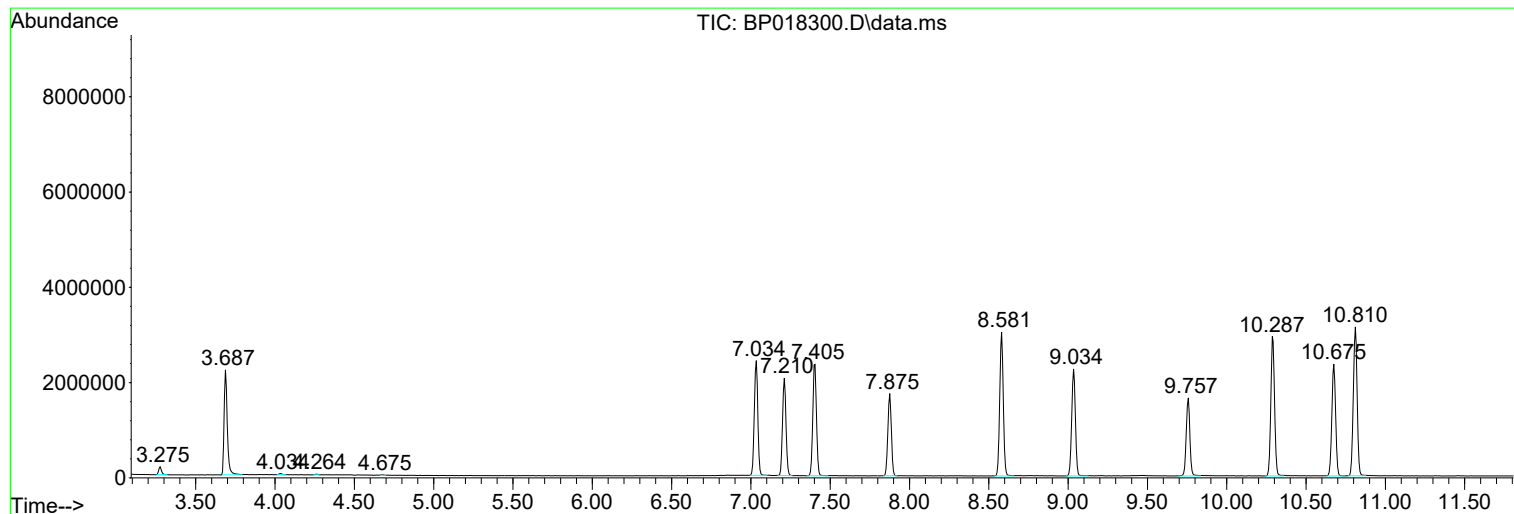

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018300.D
Acq On : 23 Nov 2023 05:57
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018300.D
Acq On : 23 Nov 2023 05:57
Operator : MA/JU
Sample : PB157217BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK217

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc