

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
 Data File : BP018303.D  
 Acq On : 23 Nov 2023 07:39  
 Operator : MA/JU  
 Sample : 05268-05DL 10X  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCKC3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
 Title : SVOA CALIBRATION

Signal : TIC: BP018303.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.276       | 29            | 32          | 36           | rVB      | 18402          | 22464         | 0.25%           | 0.043%        |
| 2         | 3.693       | 99            | 103         | 112          | rBV      | 116889         | 168954        | 1.91%           | 0.326%        |
| 3         | 4.034       | 157           | 161         | 166          | rBV      | 26986          | 35193         | 0.40%           | 0.068%        |
| 4         | 5.875       | 469           | 474         | 478          | rBV      | 19057          | 27784         | 0.31%           | 0.054%        |
| 5         | 6.364       | 552           | 557         | 559          | rBV5     | 6468           | 11582         | 0.13%           | 0.022%        |
| 6         | 6.852       | 636           | 640         | 644          | rBV7     | 5595           | 11000         | 0.12%           | 0.021%        |
| 7         | 7.028       | 664           | 670         | 678          | rVB      | 101503         | 162200        | 1.84%           | 0.313%        |
| 8         | 7.211       | 695           | 701         | 708          | rVB      | 228547         | 356802        | 4.04%           | 0.688%        |
| 9         | 7.399       | 726           | 733         | 743          | rBV      | 207233         | 329190        | 3.73%           | 0.635%        |
| 10        | 7.516       | 750           | 753         | 758          | rBV3     | 9503           | 14830         | 0.17%           | 0.029%        |
| 11        | 7.593       | 761           | 766         | 774          | rVB      | 61104          | 97092         | 1.10%           | 0.187%        |
| 12        | 7.875       | 807           | 814         | 821          | rBV      | 1484829        | 2336409       | 26.47%          | 4.508%        |
| 13        | 7.987       | 829           | 833         | 839          | rBV2     | 12547          | 18531         | 0.21%           | 0.036%        |
| 14        | 8.411       | 897           | 905         | 914          | rVB      | 79768          | 129395        | 1.47%           | 0.250%        |
| 15        | 8.575       | 928           | 933         | 942          | rBV      | 188585         | 299125        | 3.39%           | 0.577%        |
| 16        | 8.722       | 952           | 958         | 962          | rBV      | 30343          | 48069         | 0.54%           | 0.093%        |
| 17        | 8.987       | 998           | 1003        | 1005         | rBV6     | 6332           | 10070         | 0.11%           | 0.019%        |
| 18        | 9.028       | 1005          | 1010        | 1020         | rVB      | 225832         | 402186        | 4.56%           | 0.776%        |
| 19        | 9.228       | 1036          | 1044        | 1053         | rVB3     | 16808          | 34495         | 0.39%           | 0.067%        |
| 20        | 9.358       | 1056          | 1066        | 1073         | rBV3     | 41568          | 91544         | 1.04%           | 0.177%        |
| 21        | 9.416       | 1073          | 1076        | 1079         | rBV5     | 9866           | 13255         | 0.15%           | 0.026%        |
| 22        | 9.752       | 1126          | 1133        | 1142         | rVV      | 117689         | 202759        | 2.30%           | 0.391%        |
| 23        | 10.081      | 1184          | 1189        | 1196         | rVB10    | 10882          | 20931         | 0.24%           | 0.040%        |
| 24        | 10.287      | 1217          | 1224        | 1236         | rBV      | 271529         | 471303        | 5.34%           | 0.909%        |
| 25        | 10.675      | 1282          | 1290        | 1294         | rBV      | 2073209        | 3521889       | 39.90%          | 6.795%        |
| 26        | 10.728      | 1294          | 1299        | 1306         | rVV      | 5418293        | 8826774       | 100.00%         | 17.031%       |
| 27        | 10.810      | 1306          | 1313        | 1315         | rVV      | 282944         | 472792        | 5.36%           | 0.912%        |
| 28        | 10.840      | 1315          | 1318        | 1330         | rVB      | 416035         | 696003        | 7.89%           | 1.343%        |
| 29        | 11.034      | 1347          | 1351        | 1352         | rBV4     | 6362           | 9474          | 0.11%           | 0.018%        |
| 30        | 11.052      | 1352          | 1354        | 1359         | rVV6     | 7775           | 12399         | 0.14%           | 0.024%        |
| 31        | 11.352      | 1402          | 1405        | 1410         | rVB7     | 7122           | 12338         | 0.14%           | 0.024%        |
| 32        | 11.793      | 1475          | 1480        | 1486         | rVB5     | 13433          | 26924         | 0.31%           | 0.052%        |
| 33        | 11.905      | 1495          | 1499        | 1503         | rVV7     | 6971           | 12825         | 0.15%           | 0.025%        |
| 34        | 11.981      | 1507          | 1512        | 1517         | rVB8     | 8153           | 16926         | 0.19%           | 0.033%        |
| 35        | 12.228      | 1548          | 1554        | 1559         | rBV      | 25886          | 46637         | 0.53%           | 0.090%        |
| 36        | 12.334      | 1565          | 1572        | 1579         | rBV      | 600309         | 945699        | 10.71%          | 1.825%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
 Data File : BP018303.D  
 Acq On : 23 Nov 2023 07:39  
 Operator : MA/JU  
 Sample : 05268-05DL 10X  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCKC3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |       |         |         |        |        |
|----|--------|------|------|------|-------|---------|---------|--------|--------|
| 37 | 12.446 | 1586 | 1591 | 1598 | rBV   | 20767   | 38168   | 0.43%  | 0.074% |
| 38 | 12.552 | 1598 | 1609 | 1616 | rVV   | 392884  | 626590  | 7.10%  | 1.209% |
| 39 | 12.663 | 1623 | 1628 | 1630 | rBV6  | 11568   | 15859   | 0.18%  | 0.031% |
| 40 | 12.693 | 1630 | 1633 | 1638 | rVB5  | 15731   | 23331   | 0.26%  | 0.045% |
| 41 | 12.904 | 1662 | 1669 | 1675 | rBV8  | 10285   | 22803   | 0.26%  | 0.044% |
| 42 | 12.999 | 1677 | 1685 | 1689 | rVB10 | 11708   | 29446   | 0.33%  | 0.057% |
| 43 | 13.204 | 1714 | 1720 | 1723 | rBV8  | 8116    | 17267   | 0.20%  | 0.033% |
| 44 | 13.346 | 1738 | 1744 | 1750 | rVB   | 267282  | 392515  | 4.45%  | 0.757% |
| 45 | 13.416 | 1750 | 1756 | 1762 | rBV2  | 43175   | 68378   | 0.77%  | 0.132% |
| 46 | 13.469 | 1762 | 1765 | 1770 | rVV6  | 8762    | 15820   | 0.18%  | 0.031% |
| 47 | 13.540 | 1770 | 1777 | 1786 | rVB   | 20380   | 55143   | 0.62%  | 0.106% |
| 48 | 13.675 | 1789 | 1800 | 1809 | rBV7  | 43583   | 109263  | 1.24%  | 0.211% |
| 49 | 13.757 | 1809 | 1814 | 1818 | rBV8  | 9793    | 15798   | 0.18%  | 0.030% |
| 50 | 13.828 | 1818 | 1826 | 1831 | rBV   | 54956   | 104090  | 1.18%  | 0.201% |
| 51 | 13.881 | 1831 | 1835 | 1837 | rVV2  | 26427   | 40317   | 0.46%  | 0.078% |
| 52 | 13.922 | 1837 | 1842 | 1854 | rVB   | 701399  | 991948  | 11.24% | 1.914% |
| 53 | 14.063 | 1860 | 1866 | 1870 | rBV3  | 19830   | 32063   | 0.36%  | 0.062% |
| 54 | 14.198 | 1882 | 1889 | 1899 | rVB   | 773689  | 1225757 | 13.89% | 2.365% |
| 55 | 14.504 | 1932 | 1941 | 1947 | rVV   | 3370180 | 4900443 | 55.52% | 9.455% |
| 56 | 14.569 | 1947 | 1952 | 1958 | rVV   | 464884  | 677456  | 7.68%  | 1.307% |
| 57 | 14.634 | 1958 | 1963 | 1967 | rVV   | 139512  | 199352  | 2.26%  | 0.385% |
| 58 | 14.687 | 1967 | 1972 | 1977 | rVB   | 43266   | 64868   | 0.73%  | 0.125% |
| 59 | 14.781 | 1984 | 1988 | 1991 | rBV3  | 10813   | 15692   | 0.18%  | 0.030% |
| 60 | 14.840 | 1993 | 1998 | 2003 | rVV8  | 12862   | 25909   | 0.29%  | 0.050% |
| 61 | 14.904 | 2003 | 2009 | 2017 | rVB   | 558087  | 816124  | 9.25%  | 1.575% |
| 62 | 15.040 | 2026 | 2032 | 2037 | rBV   | 65471   | 98001   | 1.11%  | 0.189% |
| 63 | 15.122 | 2042 | 2046 | 2052 | rVB4  | 22143   | 35320   | 0.40%  | 0.068% |
| 64 | 15.328 | 2079 | 2081 | 2085 | rBV5  | 9293    | 9225    | 0.10%  | 0.018% |
| 65 | 15.434 | 2094 | 2099 | 2104 | rBV9  | 6128    | 13446   | 0.15%  | 0.026% |
| 66 | 15.498 | 2104 | 2110 | 2115 | rVV   | 1021909 | 1496437 | 16.95% | 2.887% |
| 67 | 15.551 | 2115 | 2119 | 2124 | rVV   | 351853  | 491995  | 5.57%  | 0.949% |
| 68 | 15.604 | 2124 | 2128 | 2137 | rVV2  | 103591  | 170907  | 1.94%  | 0.330% |
| 69 | 15.681 | 2137 | 2141 | 2148 | rVV4  | 32234   | 51267   | 0.58%  | 0.099% |
| 70 | 15.775 | 2153 | 2157 | 2159 | rVV4  | 7491    | 10024   | 0.11%  | 0.019% |
| 71 | 15.845 | 2164 | 2169 | 2175 | rVB3  | 26361   | 45506   | 0.52%  | 0.088% |
| 72 | 15.993 | 2190 | 2194 | 2201 | rVB3  | 26557   | 44559   | 0.50%  | 0.086% |
| 73 | 16.222 | 2228 | 2233 | 2240 | rVB   | 56387   | 88972   | 1.01%  | 0.172% |
| 74 | 16.434 | 2266 | 2269 | 2273 | rVB3  | 16757   | 21921   | 0.25%  | 0.042% |
| 75 | 16.510 | 2277 | 2282 | 2287 | rBV   | 53628   | 81237   | 0.92%  | 0.157% |
| 76 | 16.769 | 2323 | 2326 | 2329 | rBV5  | 8111    | 11081   | 0.13%  | 0.021% |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
 Data File : BP018303.D  
 Acq On : 23 Nov 2023 07:39  
 Operator : MA/JU  
 Sample : 05268-05DL 10X  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DCKC3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |      |         |         |        |         |
|----|--------|------|------|------|------|---------|---------|--------|---------|
| 77 | 16.898 | 2335 | 2348 | 2356 | rBV  | 168293  | 298538  | 3.38%  | 0.576%  |
| 78 | 17.040 | 2368 | 2372 | 2374 | rBV3 | 11596   | 17376   | 0.20%  | 0.034%  |
| 79 | 17.069 | 2374 | 2377 | 2384 | rVB  | 23542   | 34909   | 0.40%  | 0.067%  |
| 80 | 17.134 | 2384 | 2388 | 2389 | rBV3 | 7387    | 8954    | 0.10%  | 0.017%  |
| 81 | 17.210 | 2398 | 2401 | 2402 | rBV  | 12964   | 12220   | 0.14%  | 0.024%  |
| 82 | 17.251 | 2402 | 2408 | 2413 | rVV  | 3691647 | 5316411 | 60.23% | 10.258% |
| 83 | 17.292 | 2413 | 2415 | 2420 | rVV  | 222165  | 289480  | 3.28%  | 0.559%  |
| 84 | 17.351 | 2420 | 2425 | 2437 | rVB  | 1056778 | 1435578 | 16.26% | 2.770%  |
| 85 | 17.451 | 2437 | 2442 | 2445 | rBV7 | 6661    | 12129   | 0.14%  | 0.023%  |
| 86 | 17.657 | 2468 | 2477 | 2482 | rBV  | 696856  | 950662  | 10.77% | 1.834%  |
| 87 | 17.810 | 2499 | 2503 | 2507 | rBV  | 27403   | 38989   | 0.44%  | 0.075%  |
| 88 | 18.157 | 2558 | 2562 | 2567 | rBV6 | 27286   | 52074   | 0.59%  | 0.100%  |
| 89 | 18.451 | 2610 | 2612 | 2616 | rVB4 | 8932    | 9059    | 0.10%  | 0.017%  |
| 90 | 18.545 | 2625 | 2628 | 2631 | rBV5 | 9077    | 11971   | 0.14%  | 0.023%  |
| 91 | 18.639 | 2641 | 2644 | 2651 | rVB6 | 12581   | 17593   | 0.20%  | 0.034%  |
| 92 | 19.004 | 2703 | 2706 | 2710 | rBV5 | 8875    | 13693   | 0.16%  | 0.026%  |
| 93 | 19.234 | 2742 | 2745 | 2748 | rBV5 | 13804   | 19158   | 0.22%  | 0.037%  |
| 94 | 19.386 | 2769 | 2771 | 2777 | rBV6 | 9706    | 15871   | 0.18%  | 0.031%  |
| 95 | 19.586 | 2800 | 2805 | 2812 | rBV  | 1031284 | 1383480 | 15.67% | 2.669%  |
| 96 | 21.357 | 3100 | 3106 | 3113 | rBV  | 2847772 | 3749113 | 42.47% | 7.234%  |
| 97 | 23.616 | 3485 | 3490 | 3500 | rVB  | 492292  | 940571  | 10.66% | 1.815%  |
| 98 | 23.774 | 3510 | 3517 | 3536 | rVB  | 1952777 | 4089003 | 46.32% | 7.890%  |




Sum of corrected areas: 51826973

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
Data File : BP018303.D  
Acq On : 23 Nov 2023 07:39  
Operator : MA/JU  
Sample : 05268-05DL 10X  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCKC3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

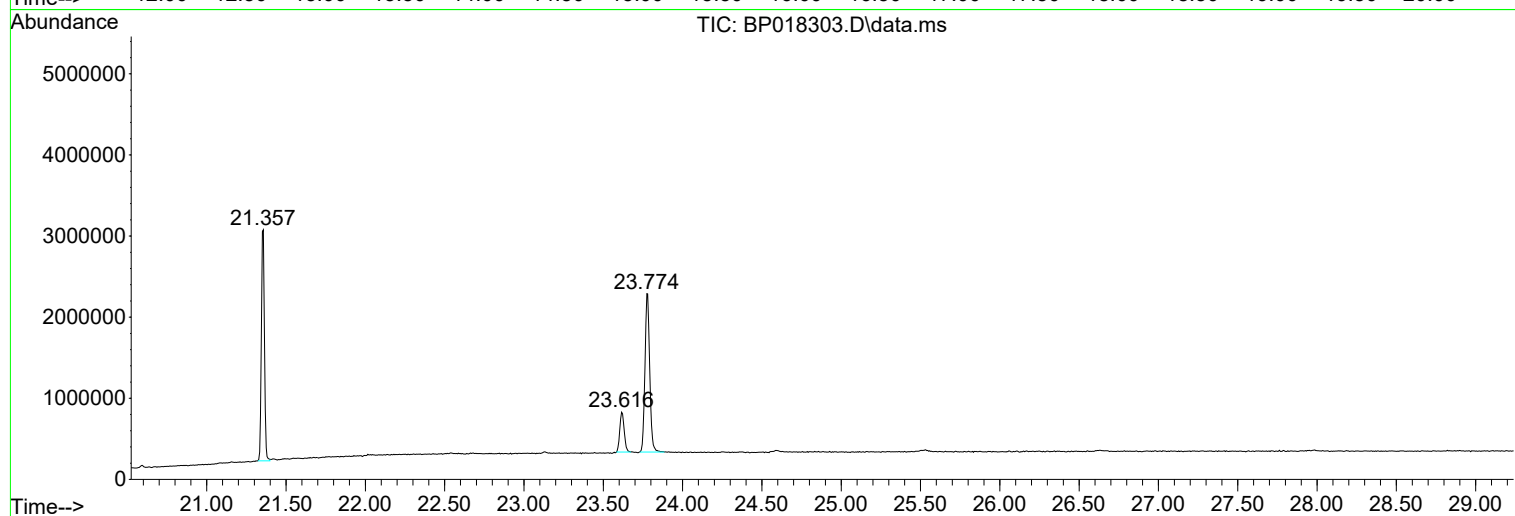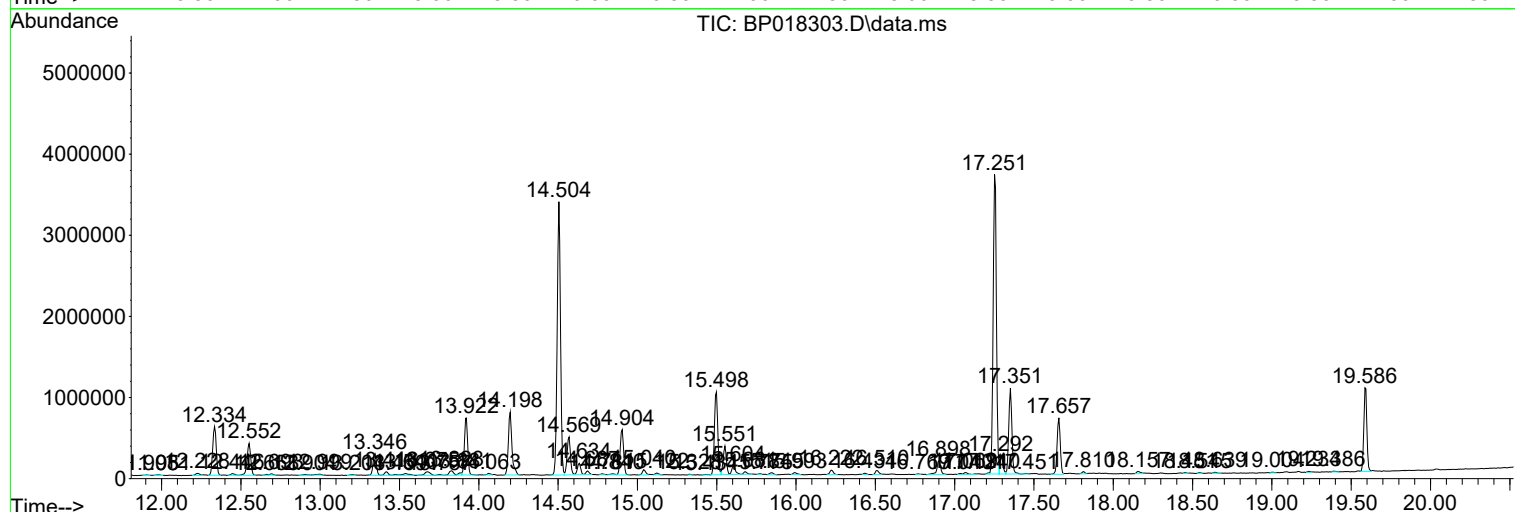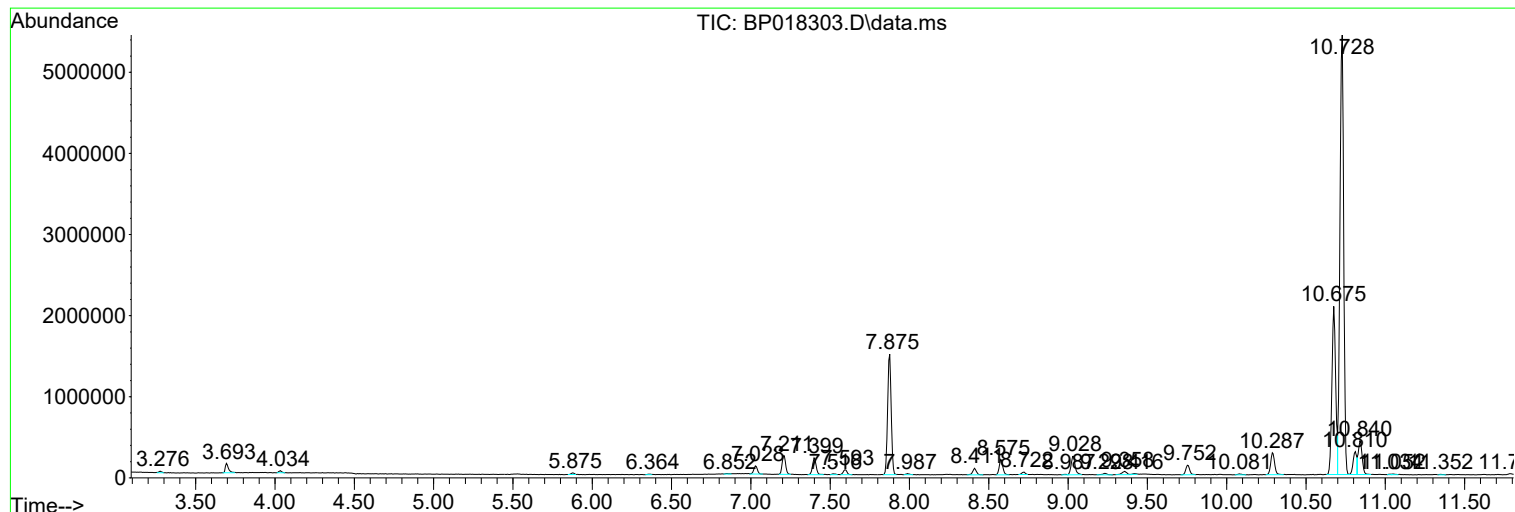

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
Data File : BP018303.D  
Acq On : 23 Nov 2023 07:39  
Operator : MA/JU  
Sample : 05268-05DL 10X  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCKC3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP112223\  
Data File : BP018303.D  
Acq On : 23 Nov 2023 07:39  
Operator : MA/JU  
Sample : 05268-05DL 10X  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DCKC3DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP112223.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |