

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018307.D
 Acq On : 23 Nov 2023 09:54
 Operator : MA/JU
 Sample : PB157319BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK319

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	42	rVB	117353	157324	1.98%	0.171%
2	3.687	98	102	118	rBV	1559561	2172231	27.37%	2.363%
3	4.034	156	161	166	rVB2	24108	35852	0.45%	0.039%
4	7.028	663	670	685	rVB	1622134	2567521	32.36%	2.793%
5	7.210	694	701	708	rVB	1394817	2158458	27.20%	2.348%
6	7.399	726	733	743	rBV	1691736	2619712	33.01%	2.849%
7	7.875	806	814	822	rBV	1434136	2284042	28.78%	2.484%
8	8.581	926	934	945	rBV	2026645	3284922	41.40%	3.573%
9	9.034	1003	1011	1019	rBV	1581871	2520763	31.77%	2.742%
10	9.204	1037	1040	1046	rVB8	5472	8741	0.11%	0.010%
11	9.757	1122	1134	1143	rBV	1054692	1774450	22.36%	1.930%
12	10.287	1216	1224	1234	rBV	2035314	3324290	41.89%	3.616%
13	10.675	1280	1290	1301	rVB	2045409	3384665	42.65%	3.681%
14	10.810	1305	1313	1322	rBV	2181814	3651232	46.01%	3.971%
15	11.969	1505	1510	1516	rBV10	4568	8645	0.11%	0.009%
16	12.257	1552	1559	1565	rBV2	41735	69685	0.88%	0.076%
17	12.904	1662	1669	1672	rBV8	10088	19241	0.24%	0.021%
18	13.416	1751	1756	1761	rBV2	41371	65988	0.83%	0.072%
19	13.475	1763	1766	1773	rVB7	6217	13553	0.17%	0.015%
20	13.816	1820	1824	1828	rBV7	6605	10056	0.13%	0.011%
21	13.922	1835	1842	1852	rBV	4066094	5340947	67.31%	5.809%
22	14.198	1881	1889	1896	rBV	4540201	6576438	82.88%	7.153%
23	14.504	1934	1941	1952	rBV	3284558	4731212	59.62%	5.146%
24	14.687	1965	1972	1989	rBV	1271169	1831625	23.08%	1.992%
25	14.928	2009	2013	2016	rVB6	9899	15262	0.19%	0.017%
26	15.322	2074	2080	2085	rBV9	8506	16465	0.21%	0.018%
27	15.498	2103	2110	2119	rBV	5651172	7935252	100.00%	8.631%
28	15.604	2122	2128	2145	rVV	842743	1217569	15.34%	1.324%
29	15.739	2145	2151	2162	rVB3	27195	58991	0.74%	0.064%
30	15.945	2180	2186	2192	rBV10	5758	11884	0.15%	0.013%
31	16.069	2203	2207	2212	rVB8	5986	10708	0.13%	0.012%
32	16.286	2239	2244	2251	rVB10	8299	15503	0.20%	0.017%
33	16.933	2351	2354	2359	rVB7	9158	13391	0.17%	0.015%
34	17.039	2368	2372	2375	rBV6	8547	13124	0.17%	0.014%
35	17.133	2385	2388	2395	rBV8	6378	11091	0.14%	0.012%
36	17.251	2402	2408	2418	rBV	3373558	5007862	63.11%	5.447%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018307.D
 Acq On : 23 Nov 2023 09:54
 Operator : MA/JU
 Sample : PB157319BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK319

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.351	2418	2425	2438	rVV	5236746	7597078	95.74%	8.263%
38	17.628	2467	2472	2474	rBV5	5975	9106	0.11%	0.010%
39	17.845	2506	2509	2513	rBV5	6026	9641	0.12%	0.010%
40	18.151	2559	2561	2567	rBV7	10429	18854	0.24%	0.021%
41	19.169	2730	2734	2740	rVB	59210	77386	0.98%	0.084%
42	19.233	2741	2745	2750	rBV	52313	73217	0.92%	0.080%
43	19.392	2770	2772	2774	rBV3	10576	9876	0.12%	0.011%
44	19.545	2796	2798	2800	rBV3	15658	12578	0.16%	0.014%
45	19.592	2800	2806	2813	rBV	5655781	7191316	90.62%	7.822%
46	21.357	3101	3106	3111	rBV	2835278	3592275	45.27%	3.907%
47	23.621	3483	3491	3507	rBV2	3155330	6323076	79.68%	6.877%
48	23.780	3511	3518	3531	rVB	2019041	4086760	51.50%	4.445%




Sum of corrected areas: 91939858

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018307.D
Acq On : 23 Nov 2023 09:54
Operator : MA/JU
Sample : PB157319BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

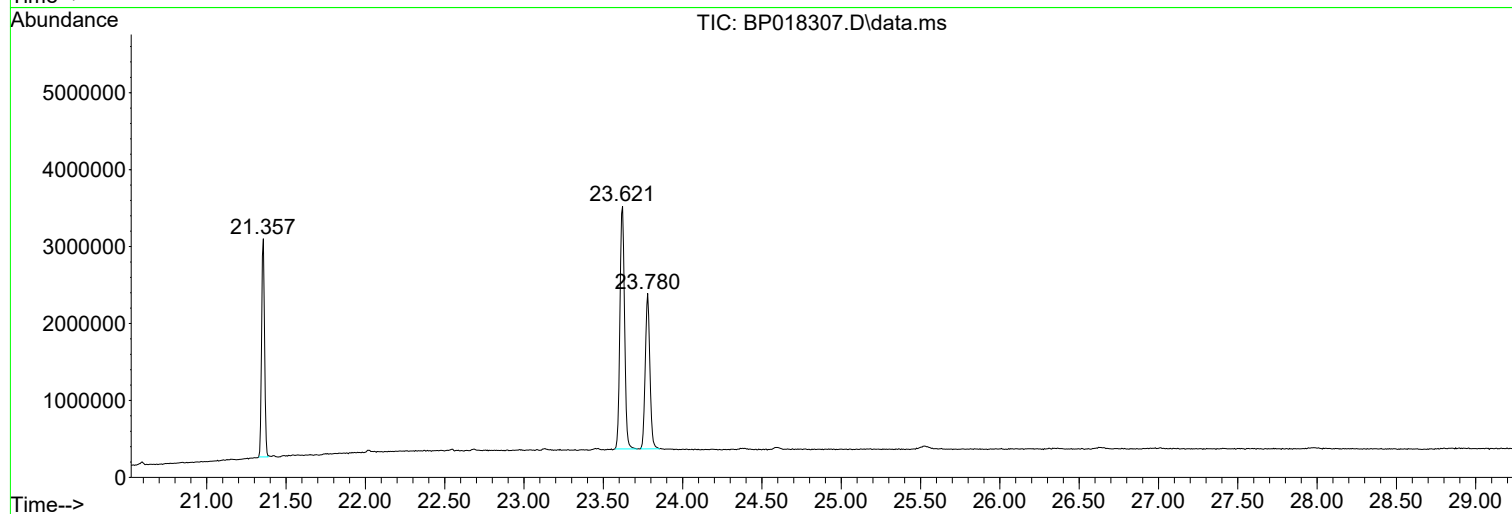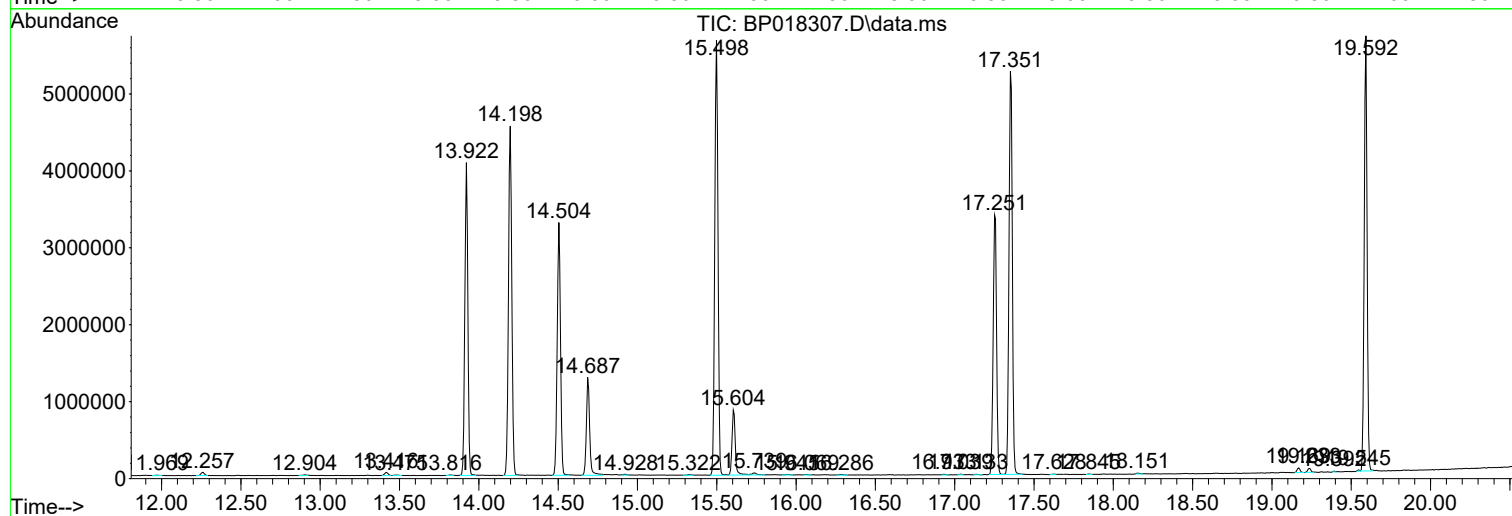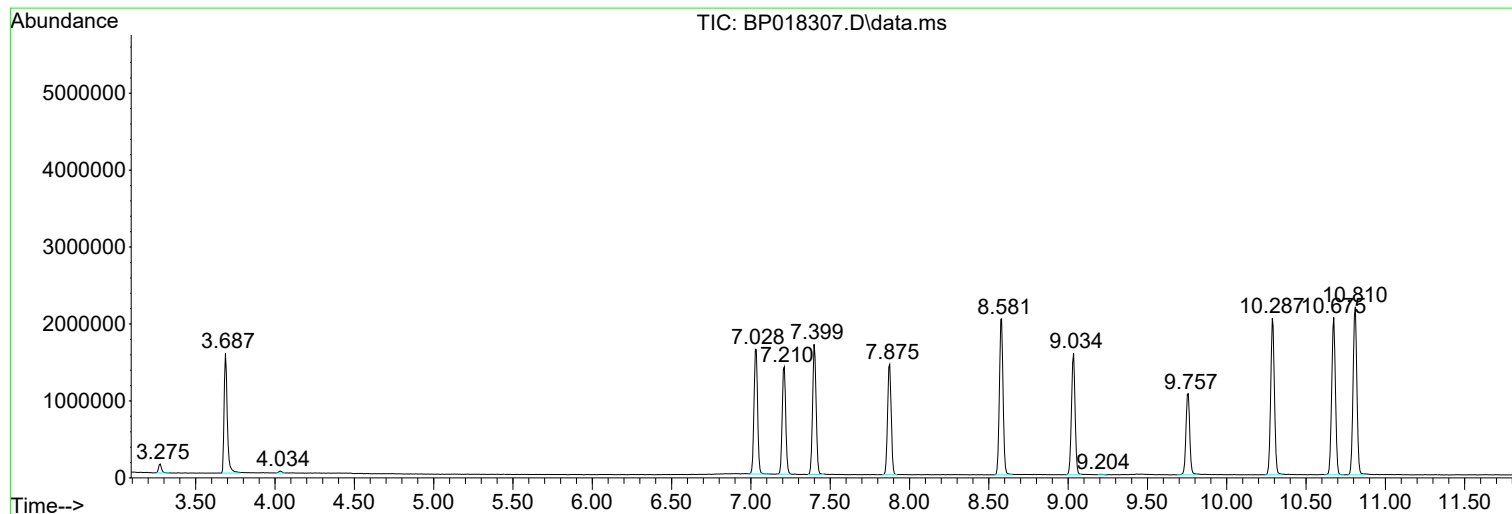

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018307.D
Acq On : 23 Nov 2023 09:54
Operator : MA/JU
Sample : PB157319BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018307.D
Acq On : 23 Nov 2023 09:54
Operator : MA/JU
Sample : PB157319BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK319

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------