

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018308.D
 Acq On : 23 Nov 2023 10:28
 Operator : MA/JU
 Sample : 05390-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	40	rVB	110677	137351	1.19%	0.127%
2	3.687	98	102	112	rBV	780190	1099993	9.50%	1.021%
3	3.940	141	145	149	rVB	20987	30454	0.26%	0.028%
4	4.034	156	161	167	rBV	26672	43384	0.37%	0.040%
5	7.028	663	670	683	rVB	580835	910909	7.86%	0.845%
6	7.211	693	701	710	rVB	1723050	2668787	23.04%	2.477%
7	7.399	727	733	742	rBV	1588836	2451157	21.16%	2.275%
8	7.875	805	814	822	rBV	1325930	2084132	17.99%	1.934%
9	8.575	926	933	945	rBV	1400969	2203709	19.02%	2.045%
10	9.034	1003	1011	1025	rBV	2006788	3241413	27.98%	3.008%
11	9.205	1034	1040	1048	rVB	7378	13900	0.12%	0.013%
12	9.481	1080	1087	1093	rVB	80130	135121	1.17%	0.125%
13	9.758	1125	1134	1145	rBV	1325889	2193332	18.93%	2.035%
14	10.287	1217	1224	1235	rBV	2374108	3867082	33.38%	3.588%
15	10.675	1282	1290	1298	rVB	1870104	3118345	26.92%	2.894%
16	10.810	1304	1313	1324	rBV	2588790	4286415	37.00%	3.978%
17	11.975	1504	1511	1523	rVB2	55118	90222	0.78%	0.084%
18	12.257	1554	1559	1569	rVB	50871	85411	0.74%	0.079%
19	12.899	1660	1668	1673	rBV7	8363	19938	0.17%	0.019%
20	13.416	1750	1756	1762	rBV3	21705	36436	0.31%	0.034%
21	13.481	1762	1767	1777	rVB7	10035	23683	0.20%	0.022%
22	13.834	1818	1827	1831	rBV10	13818	26805	0.23%	0.025%
23	13.922	1835	1842	1854	rBV	5491937	7617838	65.76%	7.069%
24	14.199	1880	1889	1898	rBV	6243097	9095287	78.52%	8.440%
25	14.504	1934	1941	1952	rBV	3154677	4472474	38.61%	4.150%
26	14.581	1952	1954	1960	rVB7	9033	12438	0.11%	0.012%
27	14.687	1966	1972	1985	rBV	424335	636211	5.49%	0.590%
28	14.922	2008	2012	2018	rVB7	19436	32407	0.28%	0.030%
29	15.328	2076	2081	2085	rBV8	8523	13400	0.12%	0.012%
30	15.498	2103	2110	2119	rBV	8127418	11344516	97.94%	10.527%
31	15.604	2122	2128	2144	rVV	1229205	1748378	15.09%	1.622%
32	15.740	2146	2151	2158	rVB	38999	66205	0.57%	0.061%
33	16.281	2239	2243	2250	rBV10	10006	15867	0.14%	0.015%
34	16.928	2350	2353	2359	rVB4	12553	19296	0.17%	0.018%
35	17.140	2384	2389	2394	rBV9	7095	15374	0.13%	0.014%
36	17.257	2402	2409	2415	rBV	3495201	4973957	42.94%	4.616%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018308.D
Acq On : 23 Nov 2023 10:28
Operator : MA/JU
Sample : 05390-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	17.357	2419	2426	2438	rVV	8045252	11533814	99.57%	10.703%
38	17.622	2468	2471	2476	rBV3	9892	16656	0.14%	0.015%
39	18.151	2557	2561	2566	rBV5	37386	55507	0.48%	0.052%
40	19.169	2729	2734	2739	rBV2	102849	133165	1.15%	0.124%
41	19.234	2741	2745	2749	rBV	86686	109935	0.95%	0.102%
42	19.392	2769	2772	2778	rBV6	25554	37237	0.32%	0.035%
43	19.592	2800	2806	2820	rBV	8805059	11583599	100.00%	10.749%
44	21.357	3101	3106	3113	rBV	2817781	3510200	30.30%	3.257%
45	23.622	3483	3491	3504	rBV2	4234132	8468327	73.11%	7.858%
46	23.780	3511	3518	3531	rVB	1691612	3483261	30.07%	3.232%




Sum of corrected areas: 107763328

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018308.D
Acq On : 23 Nov 2023 10:28
Operator : MA/JU
Sample : 05390-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

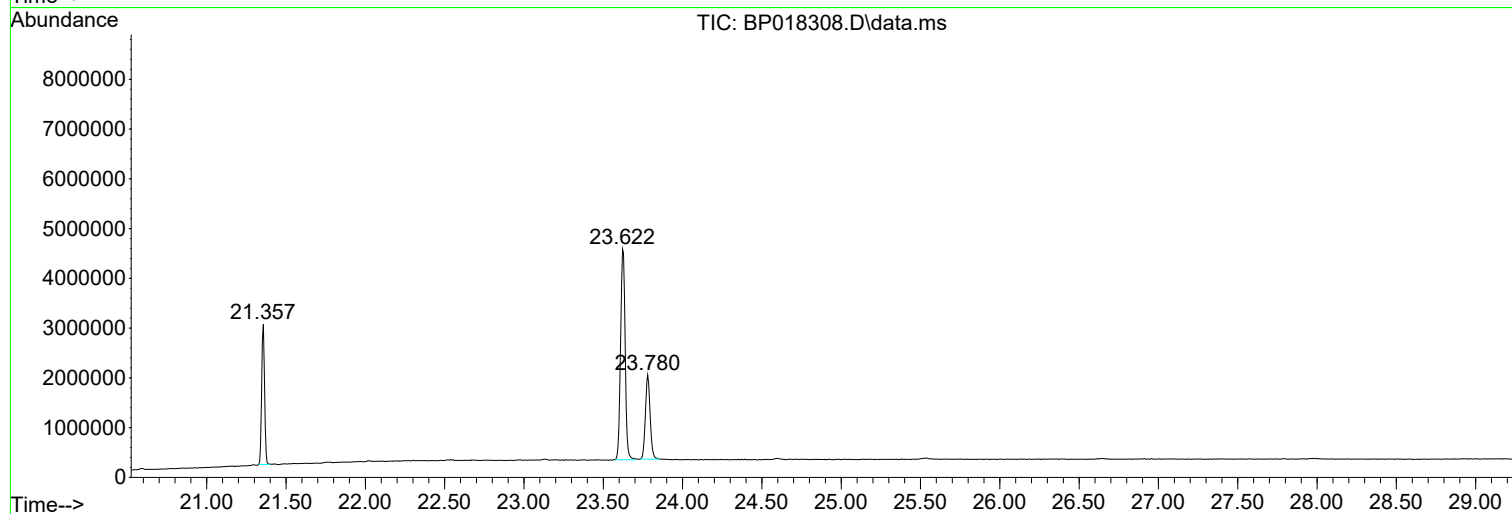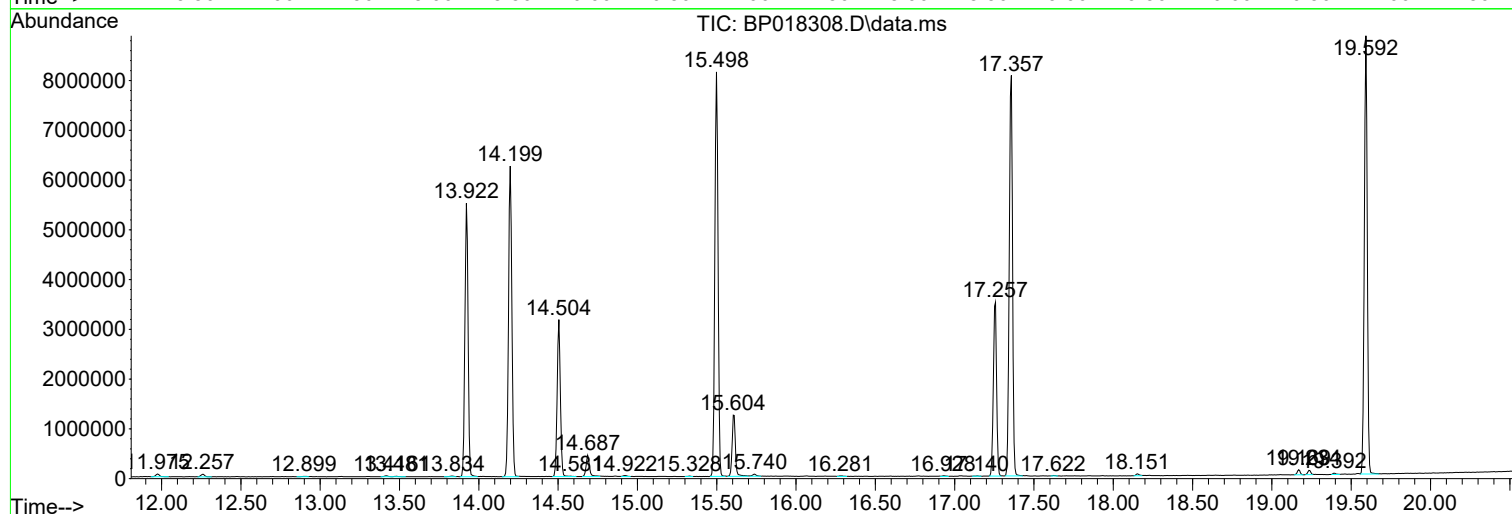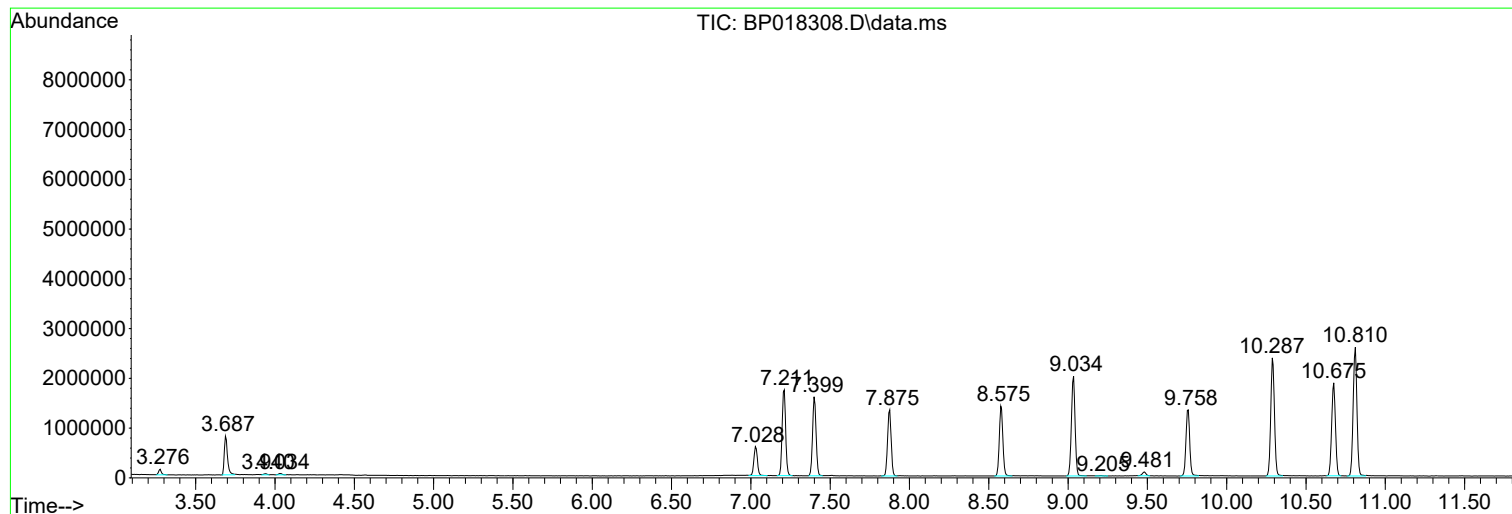

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018308.D
Acq On : 23 Nov 2023 10:28
Operator : MA/JU
Sample : 05390-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018308.D
Acq On : 23 Nov 2023 10:28
Operator : MA/JU
Sample : 05390-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc