

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018309.D
 Acq On : 23 Nov 2023 11:02
 Operator : MA/JU
 Sample : 05390-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	37	rBV	89282	111106	1.16%	0.124%
2	3.693	99	103	117	rBV	322842	481292	5.01%	0.537%
3	3.940	141	145	149	rVB	23868	30830	0.32%	0.034%
4	4.034	157	161	167	rVB	27052	38013	0.40%	0.042%
5	7.028	664	670	682	rVB	391166	613869	6.39%	0.685%
6	7.211	692	701	711	rVB	1420597	2229795	23.20%	2.490%
7	7.399	722	733	744	rBV	1340184	2070010	21.53%	2.311%
8	7.875	806	814	823	rBV	1254377	1975343	20.55%	2.206%
9	8.575	926	933	946	rBV	1118504	1725867	17.95%	1.927%
10	9.034	1002	1011	1022	rBV	1606620	2626834	27.33%	2.933%
11	9.205	1036	1040	1045	rBV8	8012	13850	0.14%	0.015%
12	9.481	1082	1087	1096	rVB	37164	64838	0.67%	0.072%
13	9.752	1122	1133	1147	rBV	1029603	1716600	17.86%	1.917%
14	10.287	1215	1224	1239	rBV	1883500	3098450	32.23%	3.460%
15	10.675	1282	1290	1297	rBV	1744006	2920801	30.38%	3.261%
16	10.810	1305	1313	1322	rBV	1837204	3131888	32.58%	3.497%
17	11.975	1505	1511	1517	rVB3	45041	78033	0.81%	0.087%
18	12.257	1554	1559	1567	rVV2	41184	65658	0.68%	0.073%
19	12.552	1603	1609	1612	rBV8	4859	10512	0.11%	0.012%
20	12.693	1625	1633	1638	rBV7	13880	29958	0.31%	0.033%
21	12.899	1661	1668	1672	rBV7	10024	21600	0.22%	0.024%
22	13.140	1703	1709	1712	rVB8	6267	10301	0.11%	0.012%
23	13.299	1731	1736	1739	rBV6	10918	18588	0.19%	0.021%
24	13.416	1752	1756	1762	rVB2	31041	47782	0.50%	0.053%
25	13.481	1762	1767	1771	rBV6	6869	11754	0.12%	0.013%
26	13.922	1834	1842	1854	rBV	4616892	6125515	63.72%	6.840%
27	14.198	1882	1889	1900	rBV2	4830943	7075246	73.60%	7.900%
28	14.504	1933	1941	1948	rBV	2914711	4181070	43.49%	4.669%
29	14.687	1965	1972	1985	rBV	269710	416199	4.33%	0.465%
30	14.816	1991	1994	1999	rVB6	7256	10236	0.11%	0.011%
31	14.922	2005	2012	2018	rVB7	18085	37619	0.39%	0.042%
32	15.334	2075	2082	2087	rVB8	11361	22202	0.23%	0.025%
33	15.498	2103	2110	2117	rBV	6328245	9053044	94.18%	10.109%
34	15.545	2117	2118	2123	rVB5	14190	17124	0.18%	0.019%
35	15.604	2123	2128	2139	rBV	1024085	1454981	15.14%	1.625%
36	15.740	2146	2151	2154	rVB2	26619	33175	0.35%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018309.D
 Acq On : 23 Nov 2023 11:02
 Operator : MA/JU
 Sample : 05390-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.587	2293	2295	2301	rVB6	7337	12222	0.13%	0.014%
38	16.934	2350	2354	2362	rBV10	11411	18534	0.19%	0.021%
39	17.040	2368	2372	2379	rVB3	7381	13408	0.14%	0.015%
40	17.134	2384	2388	2393	rBV8	6570	11343	0.12%	0.013%
41	17.251	2402	2408	2418	rBV	3256314	4602382	47.88%	5.139%
42	17.351	2419	2425	2438	rVB	6401397	9612845	100.00%	10.734%
43	17.622	2468	2471	2476	rBV3	9023	15203	0.16%	0.017%
44	18.151	2557	2561	2569	rBV5	31568	53643	0.56%	0.060%
45	18.763	2660	2665	2670	rBV8	7463	15494	0.16%	0.017%
46	19.169	2729	2734	2741	rBV2	75943	102265	1.06%	0.114%
47	19.234	2741	2745	2750	rBV	72298	105250	1.09%	0.118%
48	19.392	2769	2772	2776	rBV4	20886	24175	0.25%	0.027%
49	19.592	2800	2806	2814	rBV	7619097	9545182	99.30%	10.658%
50	21.351	3101	3105	3113	rBV	2501337	3190760	33.19%	3.563%
51	23.622	3483	3491	3506	rBV2	3724365	7309101	76.03%	8.162%
52	23.780	3511	3518	3531	rVB	1598165	3353614	34.89%	3.745%




Sum of corrected areas: 89555404

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018309.D
Acq On : 23 Nov 2023 11:02
Operator : MA/JU
Sample : 05390-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

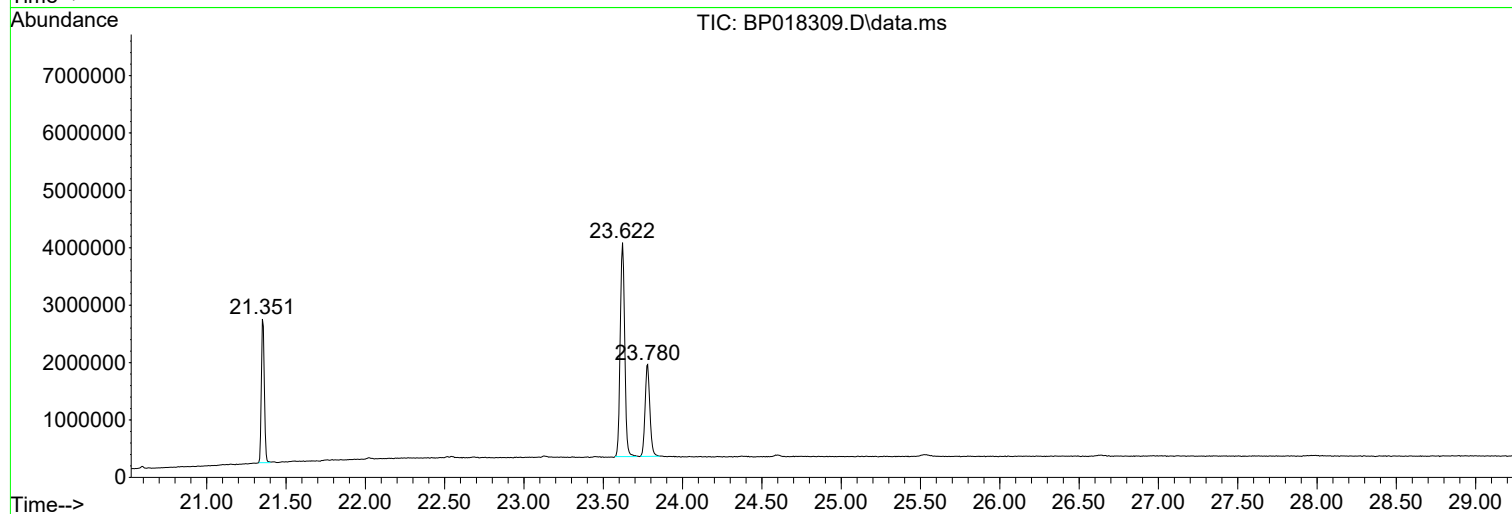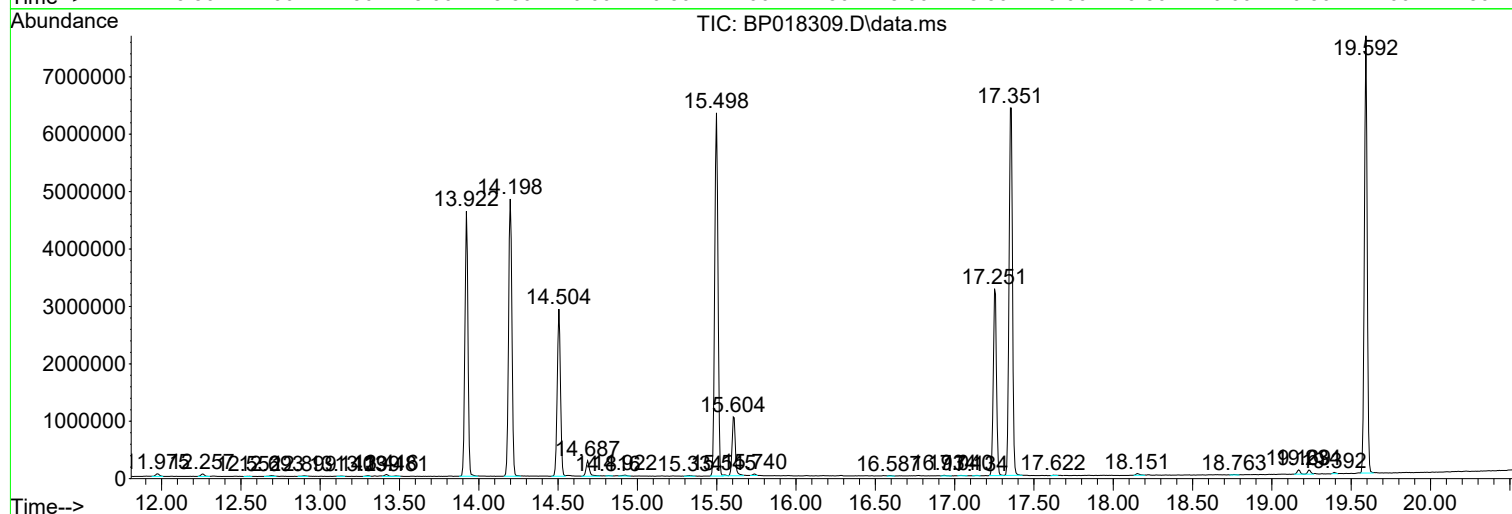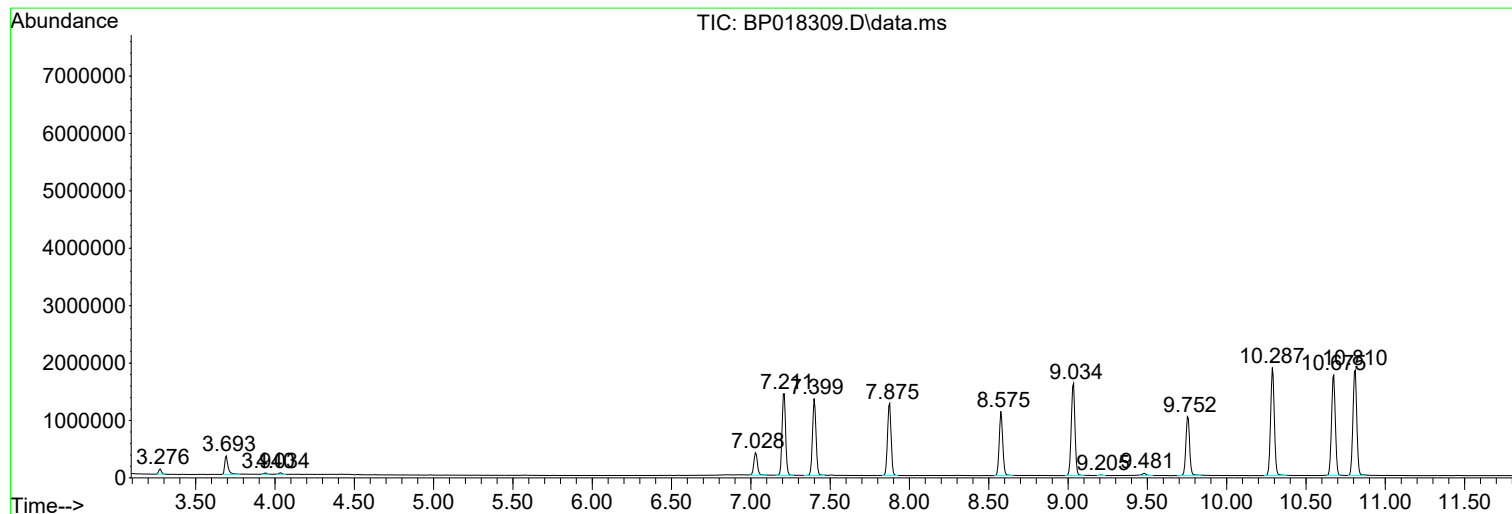

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018309.D
Acq On : 23 Nov 2023 11:02
Operator : MA/JU
Sample : 05390-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018309.D
Acq On : 23 Nov 2023 11:02
Operator : MA/JU
Sample : 05390-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc