

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018310.D
 Acq On : 23 Nov 2023 11:36
 Operator : MA/JU
 Sample : 05390-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rVB	93987	107374	1.00%	0.124%
2	3.693	99	103	113	rBV	425515	607024	5.68%	0.700%
3	3.940	141	145	151	rVB3	21767	37072	0.35%	0.043%
4	4.034	157	161	166	rVB2	21161	30762	0.29%	0.035%
5	7.028	663	670	680	rVB	409019	653676	6.11%	0.754%
6	7.210	693	701	713	rVB	1550526	2459509	23.00%	2.836%
7	7.399	726	733	742	rBV	1481508	2319922	21.69%	2.675%
8	7.505	748	751	758	rVB6	8736	14529	0.14%	0.017%
9	7.875	805	814	822	rBV	1328565	2115400	19.78%	2.439%
10	8.575	926	933	943	rBV	1151215	1804785	16.88%	2.081%
11	9.034	1003	1011	1020	rBV	1711825	2759344	25.80%	3.181%
12	9.481	1081	1087	1092	rVB4	13463	25312	0.24%	0.029%
13	9.752	1124	1133	1147	rBV	1045575	1777640	16.62%	2.050%
14	10.287	1216	1224	1236	rBV	1920645	3175038	29.69%	3.661%
15	10.675	1282	1290	1297	rBV	1726471	2852782	26.67%	3.289%
16	10.810	1304	1313	1323	rBV	1451701	2456954	22.97%	2.833%
17	11.481	1421	1427	1438	rVB	7771	16836	0.16%	0.019%
18	12.257	1553	1559	1567	rBV2	42823	80076	0.75%	0.092%
19	12.328	1567	1571	1576	rVB6	7136	12806	0.12%	0.015%
20	12.693	1626	1633	1639	rBV7	11606	25572	0.24%	0.029%
21	12.898	1663	1668	1676	rBV8	8119	17904	0.17%	0.021%
22	13.298	1731	1736	1741	rBV10	9274	15698	0.15%	0.018%
23	13.416	1751	1756	1760	rVB2	29620	41895	0.39%	0.048%
24	13.828	1822	1826	1829	rBV6	5888	11088	0.10%	0.013%
25	13.922	1835	1842	1853	rBV	3435318	4656309	43.54%	5.369%
26	14.198	1881	1889	1903	rBV	4240559	6152994	57.53%	7.094%
27	14.504	1934	1941	1949	rBV	2384705	3415998	31.94%	3.939%
28	14.563	1949	1951	1958	rVB6	11342	20729	0.19%	0.024%
29	14.687	1964	1972	1979	rBV	219147	336906	3.15%	0.388%
30	14.922	2006	2012	2017	rVB7	12540	27552	0.26%	0.032%
31	15.328	2075	2081	2084	rBV7	9108	13282	0.12%	0.015%
32	15.498	2103	2110	2117	rBV	5147011	7284429	68.11%	8.399%
33	15.604	2122	2128	2140	rVV	772435	1097303	10.26%	1.265%
34	15.739	2146	2151	2155	rVB3	21215	36826	0.34%	0.042%
35	16.933	2350	2354	2360	rVB7	8209	12316	0.12%	0.014%
36	17.139	2385	2389	2392	rBV6	7496	12339	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018310.D
 Acq On : 23 Nov 2023 11:36
 Operator : MA/JU
 Sample : 05390-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0TJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	17.251	2402	2408	2415	rBV	2486877	3556540	33.25%	4.101%
38	17.351	2419	2425	2436	rVV2	5494387	7791600	72.85%	8.983%
39	17.445	2438	2441	2446	rVB7	16494	25887	0.24%	0.030%
40	18.151	2558	2561	2566	rBV4	32488	46923	0.44%	0.054%
41	19.169	2730	2734	2740	rBV2	70180	92389	0.86%	0.107%
42	19.233	2740	2745	2750	rBV	62720	97979	0.92%	0.113%
43	19.392	2769	2772	2777	rBV5	23489	32740	0.31%	0.038%
44	19.539	2794	2797	2800	rBV4	13232	21657	0.20%	0.025%
45	19.592	2800	2806	2815	rVV	6990530	9132301	85.39%	10.529%
46	21.357	3101	3106	3115	rBV	3260521	4055434	37.92%	4.676%
47	23.627	3484	3492	3504	rBV2	5401886	10694924	100.00%	12.331%
48	23.780	3511	3518	3530	rVB	2299451	4698848	43.94%	5.418%




Sum of corrected areas: 86733203

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018310.D
Acq On : 23 Nov 2023 11:36
Operator : MA/JU
Sample : 05390-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

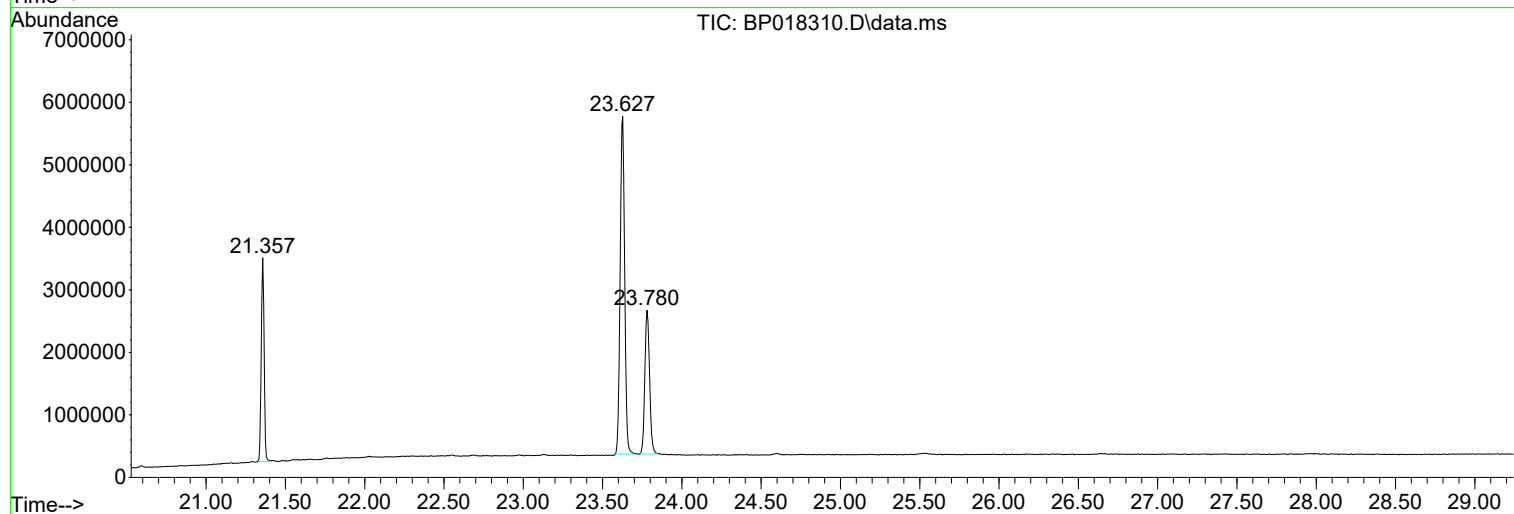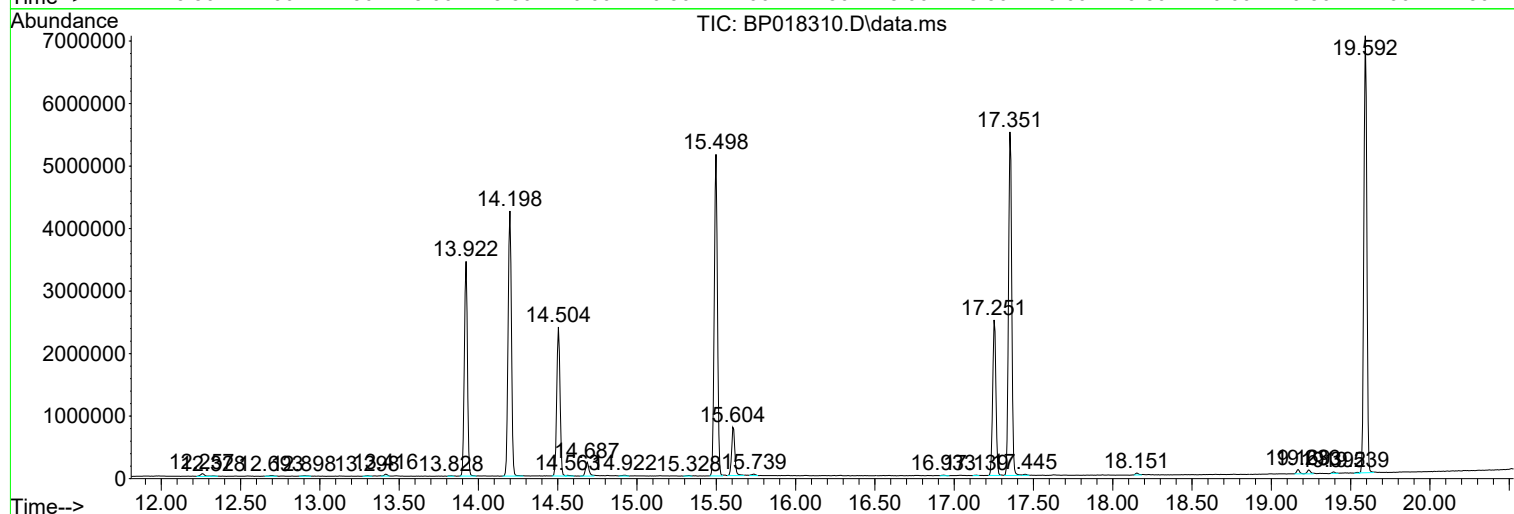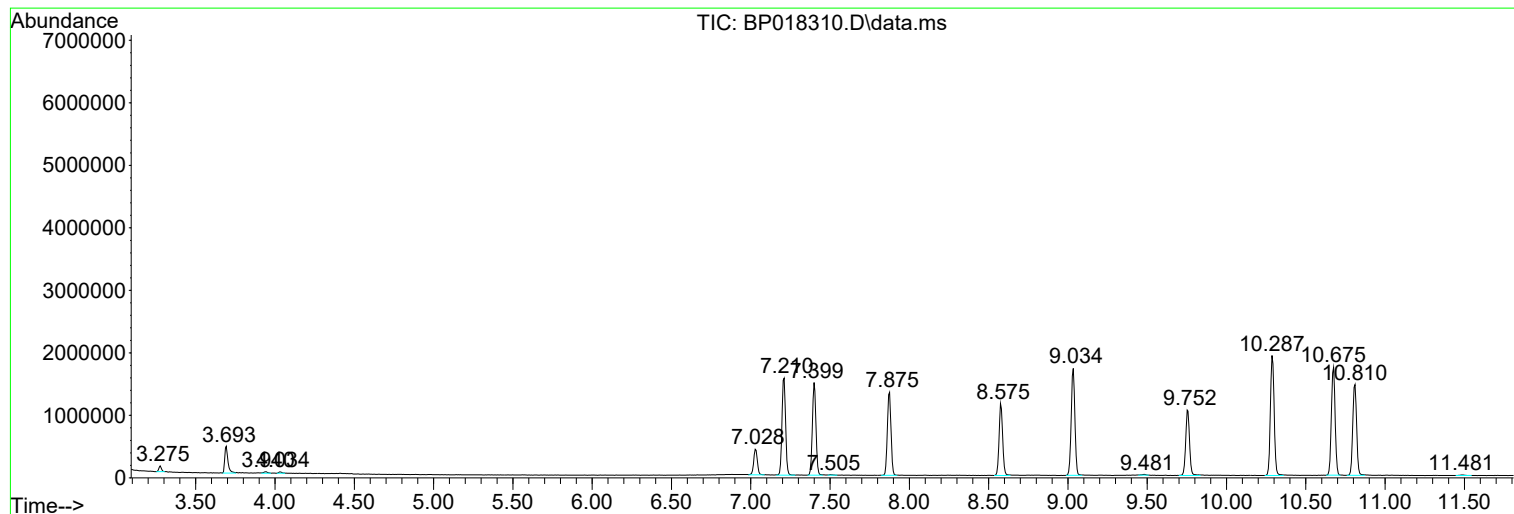

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018310.D
Acq On : 23 Nov 2023 11:36
Operator : MA/JU
Sample : 05390-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018310.D
Acq On : 23 Nov 2023 11:36
Operator : MA/JU
Sample : 05390-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0TJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------