

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018311.D
 Acq On : 23 Nov 2023 12:10
 Operator : MA/JU
 Sample : 05411-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	42	rVB	89595	124473	1.06%	0.130%
2	3.687	98	102	114	rBV	410661	615500	5.23%	0.642%
3	3.940	141	145	152	rVB	22542	37274	0.32%	0.039%
4	4.034	157	161	169	rVV3	22110	32400	0.28%	0.034%
5	4.111	172	174	187	rVB3	8490	16873	0.14%	0.018%
6	7.028	663	670	681	rVB	329837	511302	4.34%	0.533%
7	7.205	692	700	708	rBV	1476297	2292800	19.48%	2.391%
8	7.399	727	733	743	rBV	1277521	1955991	16.62%	2.040%
9	7.505	747	751	758	rVB10	7072	12694	0.11%	0.013%
10	7.875	806	814	822	rVB	1231762	1965364	16.70%	2.050%
11	8.575	924	933	943	rBV	1012652	1560184	13.26%	1.627%
12	9.034	1002	1011	1023	rBV	1638376	2697029	22.92%	2.813%
13	9.475	1083	1086	1093	rVB6	17901	31293	0.27%	0.033%
14	9.752	1124	1133	1149	rBV	1009530	1673352	14.22%	1.745%
15	10.287	1217	1224	1234	rBV	1848333	3007119	25.55%	3.136%
16	10.675	1282	1290	1297	rVB	1737755	2955359	25.11%	3.082%
17	10.804	1305	1312	1322	rBV	1777625	2996917	25.46%	3.126%
18	11.481	1423	1427	1434	rVB8	12228	25427	0.22%	0.027%
19	11.975	1507	1511	1515	rVB5	7329	11986	0.10%	0.013%
20	12.257	1554	1559	1566	rVB3	42070	70604	0.60%	0.074%
21	12.904	1662	1669	1676	rBV10	8665	19012	0.16%	0.020%
22	13.416	1750	1756	1762	rBV3	37242	58467	0.50%	0.061%
23	13.922	1835	1842	1854	rBV	4647868	6263718	53.22%	6.533%
24	14.198	1880	1889	1898	rBV	4855923	7206027	61.23%	7.516%
25	14.504	1932	1941	1953	rBV	2983753	4331116	36.80%	4.517%
26	14.687	1966	1972	1984	rBV	197869	321053	2.73%	0.335%
27	14.922	2007	2012	2017	rVB9	16911	26254	0.22%	0.027%
28	15.498	2102	2110	2122	rBV	6788445	9791519	83.20%	10.212%
29	15.604	2122	2128	2145	rVV	1101189	1553198	13.20%	1.620%
30	15.734	2145	2150	2156	rVB3	32601	56926	0.48%	0.059%
31	16.928	2350	2353	2360	rVB8	11394	16311	0.14%	0.017%
32	17.039	2368	2372	2376	rBV2	8396	12797	0.11%	0.013%
33	17.251	2401	2408	2415	rBV	3441475	4975270	42.27%	5.189%
34	17.351	2419	2425	2437	rVV2	7811795	11145769	94.70%	11.625%
35	17.622	2466	2471	2479	rVB6	11168	25854	0.22%	0.027%
36	18.151	2557	2561	2567	rBV5	39389	61729	0.52%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018311.D
Acq On : 23 Nov 2023 12:10
Operator : MA/JU
Sample : 05411-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.169	2729	2734	2740	rBV2	95987	134783	1.15%	0.141%
38	19.233	2741	2745	2752	rVV	87000	121969	1.04%	0.127%
39	19.392	2768	2772	2776	rBV4	32768	45507	0.39%	0.047%
40	19.592	2800	2806	2814	rBV	8994336	11769354	100.00%	12.275%
41	21.357	3101	3106	3114	rBV	3050546	3792541	32.22%	3.955%
42	23.621	3484	3491	3507	rVB2	4039603	8136017	69.13%	8.486%
43	23.780	3511	3518	3531	rVB	1651512	3421600	29.07%	3.569%




Sum of corrected areas: 95880732

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018311.D
Acq On : 23 Nov 2023 12:10
Operator : MA/JU
Sample : 05411-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

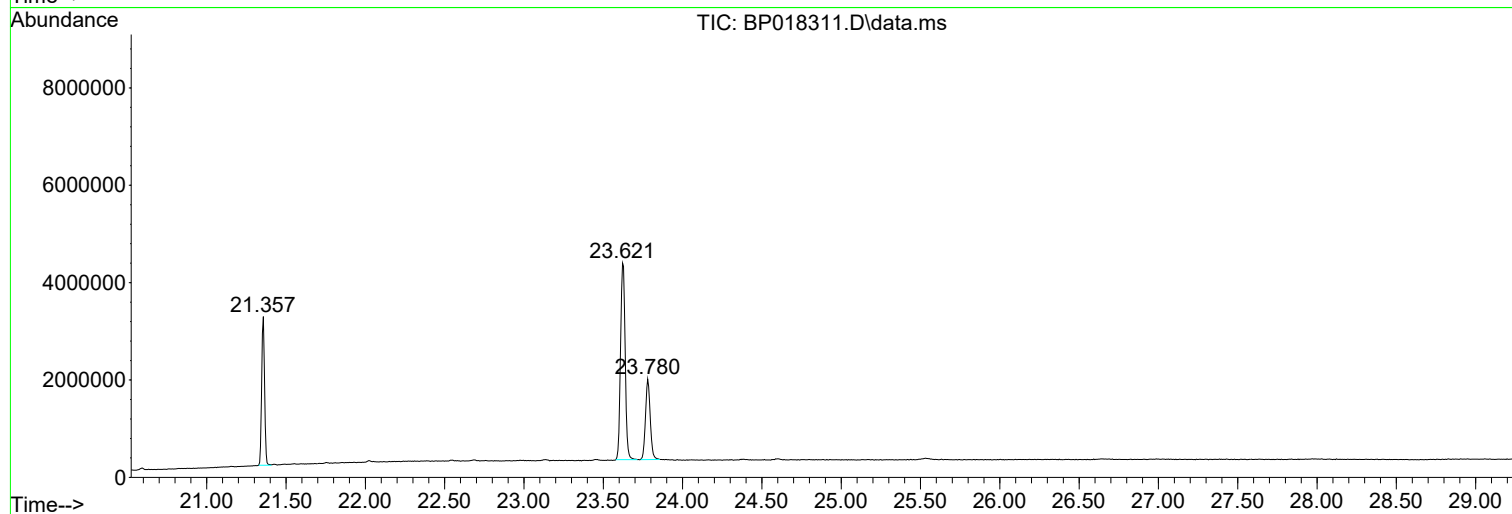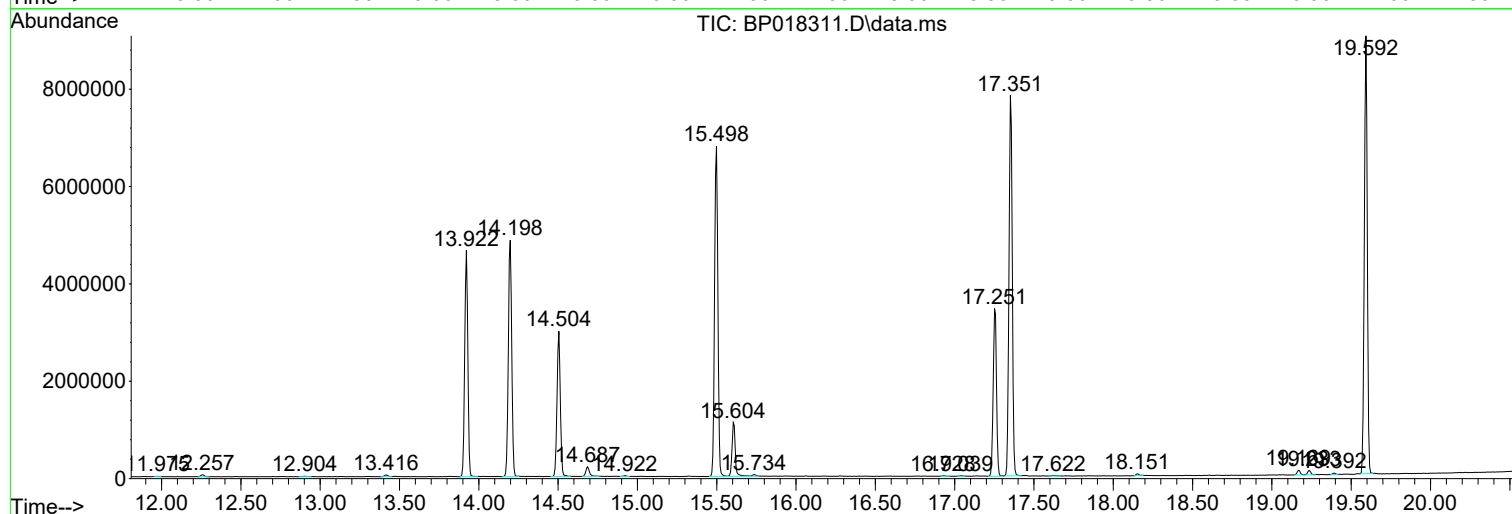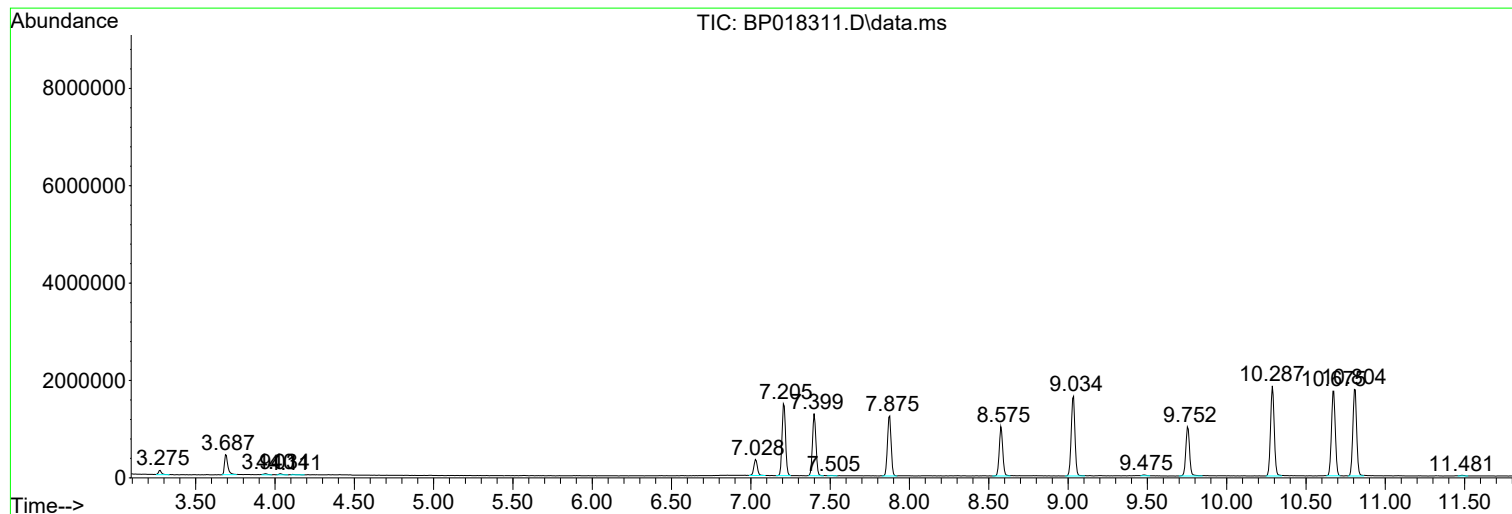

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018311.D
Acq On : 23 Nov 2023 12:10
Operator : MA/JU
Sample : 05411-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018311.D
Acq On : 23 Nov 2023 12:10
Operator : MA/JU
Sample : 05411-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
