

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018313.D
 Acq On : 23 Nov 2023 13:17
 Operator : MA/JU
 Sample : 05411-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	21	27	42	rVB2	1296253	2069978	22.38%	2.296%
2	3.687	98	102	113	rBV	523802	739349	8.00%	0.820%
3	3.940	140	145	151	rBV	23083	36265	0.39%	0.040%
4	4.028	157	160	168	rVB	21317	32036	0.35%	0.036%
5	5.146	345	350	355	rBV	20951	35813	0.39%	0.040%
6	6.275	535	542	547	rBV3	16655	27037	0.29%	0.030%
7	7.028	663	670	681	rVB	318167	504466	5.46%	0.560%
8	7.205	694	700	714	rVB	1545862	2374636	25.68%	2.634%
9	7.399	726	733	745	rBV	1288277	1963848	21.24%	2.179%
10	7.505	747	751	757	rVB6	9393	15510	0.17%	0.017%
11	7.875	806	814	823	rBV	1384098	2198933	23.78%	2.439%
12	8.575	927	933	944	rBV	908213	1407178	15.22%	1.561%
13	9.034	1002	1011	1024	rBV	1667796	2763780	29.89%	3.066%
14	9.481	1078	1087	1095	rVB3	17927	41406	0.45%	0.046%
15	9.752	1125	1133	1150	rBV	1041857	1697293	18.35%	1.883%
16	10.287	1215	1224	1234	rBV	1834298	2985331	32.28%	3.312%
17	10.675	1282	1290	1300	rVB	1931795	3242122	35.06%	3.597%
18	10.810	1304	1313	1330	rBV	1478570	2521298	27.26%	2.797%
19	11.410	1411	1415	1420	rBV5	6103	12961	0.14%	0.014%
20	11.487	1420	1428	1436	rVV	74803	133896	1.45%	0.149%
21	12.257	1553	1559	1565	rBV2	45195	66443	0.72%	0.074%
22	12.622	1613	1621	1626	rBV2	5233	10412	0.11%	0.012%
23	12.893	1659	1667	1668	rBV8	8668	11632	0.13%	0.013%
24	13.416	1750	1756	1763	rBV3	22522	40023	0.43%	0.044%
25	13.481	1763	1767	1774	rVB5	11104	19747	0.21%	0.022%
26	13.922	1835	1842	1853	rBV	4362231	5918597	64.00%	6.566%
27	14.198	1880	1889	1898	rBV	4855062	7048134	76.22%	7.819%
28	14.504	1932	1941	1954	rBV	3066347	4434196	47.95%	4.919%
29	14.687	1965	1972	1978	rBV	197457	303833	3.29%	0.337%
30	14.863	1997	2002	2007	rVB7	7428	13977	0.15%	0.016%
31	14.916	2007	2011	2017	rBV9	13211	23488	0.25%	0.026%
32	15.328	2074	2081	2087	rBV9	9848	20657	0.22%	0.023%
33	15.498	2102	2110	2122	rBV	6055277	9247391	100.00%	10.258%
34	15.604	2122	2128	2138	rBV	1001138	1365790	14.77%	1.515%
35	15.734	2146	2150	2156	rVB	28456	41079	0.44%	0.046%
36	16.281	2240	2243	2248	rVB7	8567	14655	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018313.D
 Acq On : 23 Nov 2023 13:17
 Operator : MA/JU
 Sample : 05411-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

37	16.934	2348	2354	2357	rBV5	9962	15598	0.17%	0.017%
38	17.034	2368	2371	2376	rVB3	7346	10152	0.11%	0.011%
39	17.134	2385	2388	2392	rVB6	7987	10564	0.11%	0.012%
40	17.251	2402	2408	2415	rBV	3259763	4548812	49.19%	5.046%
41	17.351	2419	2425	2439	rVB	6219993	8746155	94.58%	9.702%
42	17.557	2456	2460	2463	rBV3	6819	10091	0.11%	0.011%
43	18.151	2557	2561	2570	rBV2	52299	84863	0.92%	0.094%
44	18.457	2609	2613	2619	rBV5	15435	25626	0.28%	0.028%
45	18.604	2635	2638	2643	rBV5	16948	22361	0.24%	0.025%
46	19.169	2729	2734	2739	rBV	74822	99021	1.07%	0.110%
47	19.233	2740	2745	2750	rVV	66795	98035	1.06%	0.109%
48	19.392	2768	2772	2776	rBV4	47970	63905	0.69%	0.071%
49	19.592	2800	2806	2813	rBV	6631489	8592791	92.92%	9.532%
50	20.592	2973	2976	2980	rBV2	30348	31365	0.34%	0.035%
51	21.357	3101	3106	3114	rBV	2692532	3271572	35.38%	3.629%
52	23.621	3484	3491	3503	rBV2	3924189	7456970	80.64%	8.272%
53	23.780	3511	3518	3533	rVB	1826357	3672738	39.72%	4.074%




Sum of corrected areas: 90143809

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018313.D
Acq On : 23 Nov 2023 13:17
Operator : MA/JU
Sample : 05411-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

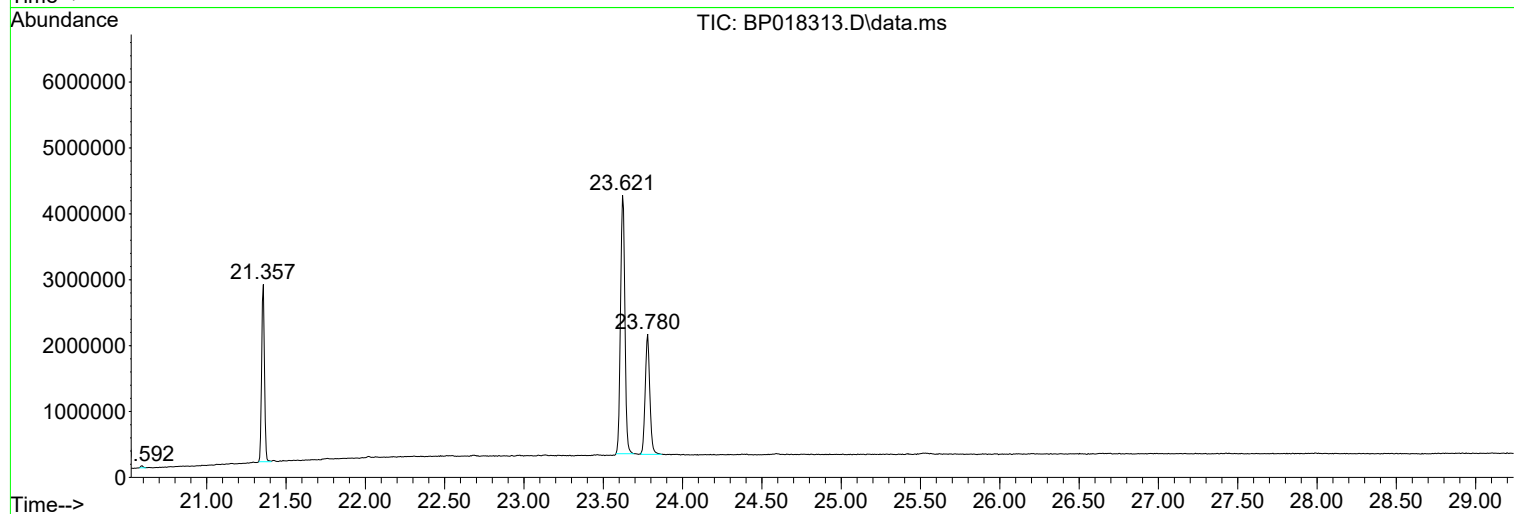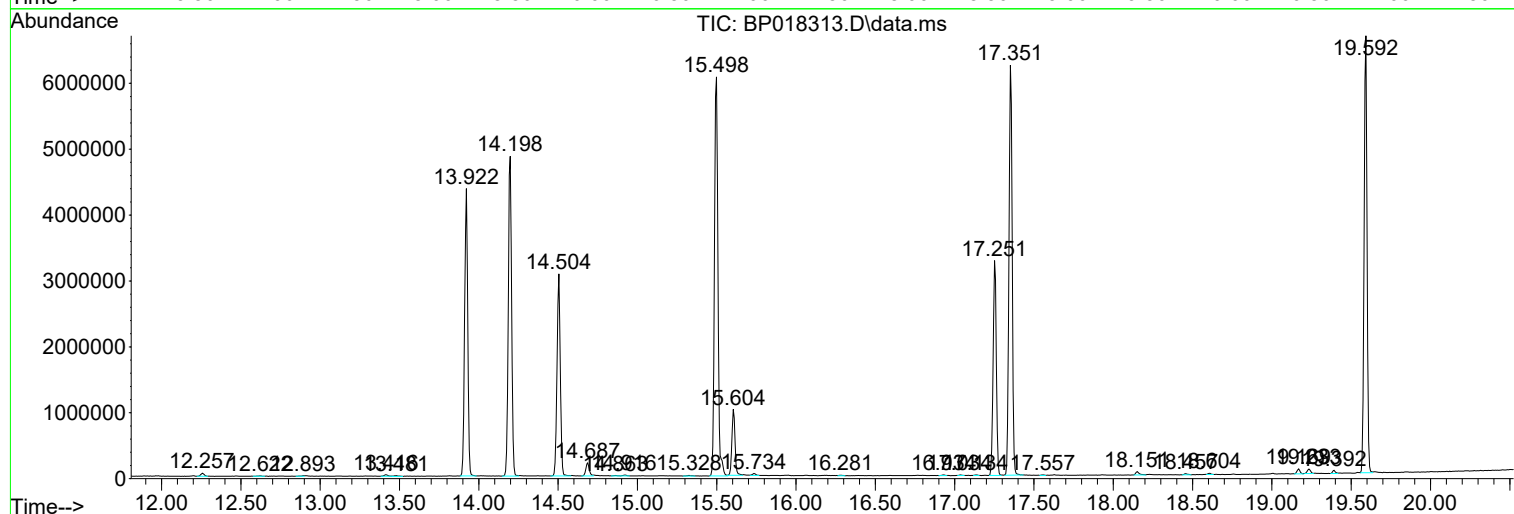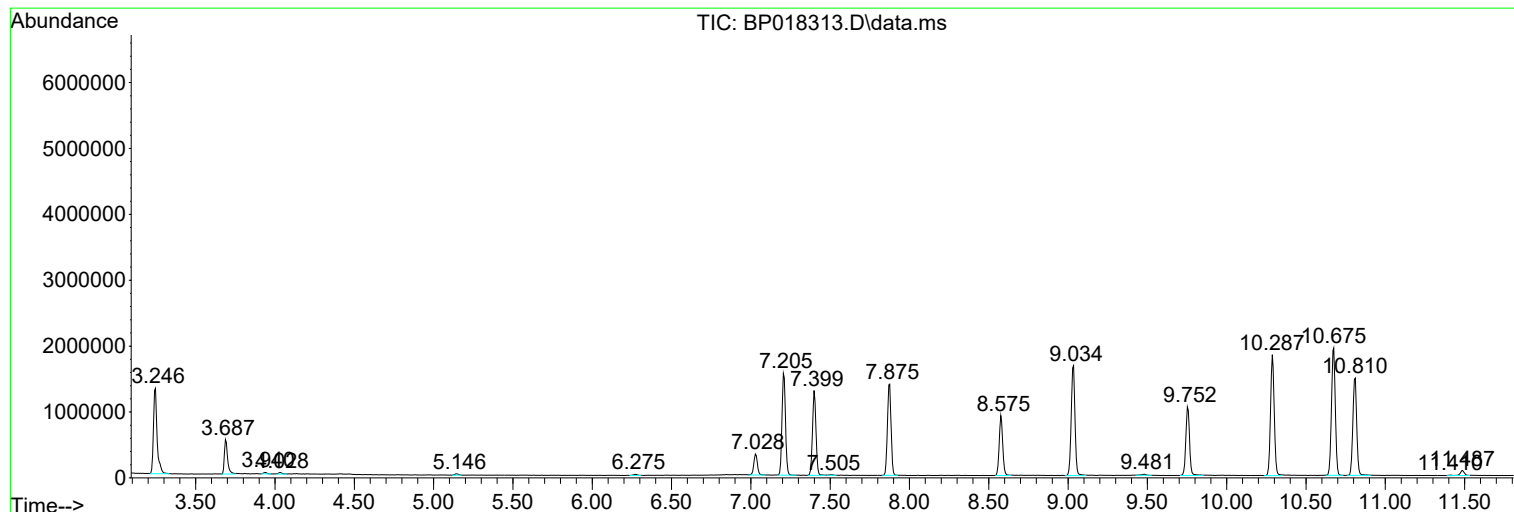

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018313.D
Acq On : 23 Nov 2023 13:17
Operator : MA/JU
Sample : 05411-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018313.D
Acq On : 23 Nov 2023 13:17
Operator : MA/JU
Sample : 05411-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc