

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018316.D
 Acq On : 23 Nov 2023 14:59
 Operator : MA/JU
 Sample : PB157189BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK189

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	42	rVB	157766	210961	2.17%	0.189%
2	3.687	97	102	117	rBV	2011232	2788674	28.67%	2.495%
3	4.034	157	161	169	rVB	29057	42402	0.44%	0.038%
4	7.034	664	671	678	rBV	2105310	3320382	34.13%	2.970%
5	7.211	693	701	712	rVB	1816782	2822130	29.01%	2.525%
6	7.399	725	733	745	rBV	2237018	3439250	35.35%	3.077%
7	7.875	807	814	821	rBV	1577369	2503424	25.73%	2.239%
8	8.575	926	933	945	rBV	2648657	4292160	44.12%	3.840%
9	9.034	1002	1011	1027	rBV	2000106	3313114	34.06%	2.964%
10	9.469	1080	1085	1091	rVB9	6039	12646	0.13%	0.011%
11	9.752	1123	1133	1147	rBV	1462815	2393341	24.60%	2.141%
12	10.287	1216	1224	1234	rBV	2647644	4361016	44.83%	3.901%
13	10.669	1281	1289	1298	rVB	2145803	3665318	37.68%	3.279%
14	10.810	1303	1313	1321	rBV	2777697	4673180	48.04%	4.180%
15	11.899	1491	1498	1500	rBV7	6030	13227	0.14%	0.012%
16	12.257	1553	1559	1565	rBV	54605	88682	0.91%	0.079%
17	13.416	1750	1756	1761	rBV	33433	52108	0.54%	0.047%
18	13.828	1819	1826	1829	rBV7	6326	13027	0.13%	0.012%
19	13.922	1835	1842	1854	rBV	4837912	6532510	67.15%	5.844%
20	14.198	1881	1889	1899	rBV	5604294	8271026	85.02%	7.399%
21	14.504	1934	1941	1948	rBV	3419439	4995545	51.35%	4.469%
22	14.687	1964	1972	1992	rBV	1558507	2309250	23.74%	2.066%
23	14.857	1998	2001	2006	rVB7	6332	11189	0.12%	0.010%
24	14.922	2008	2012	2015	rVB6	9233	13215	0.14%	0.012%
25	15.328	2074	2081	2083	rVB6	7005	10241	0.11%	0.009%
26	15.498	2103	2110	2121	rBV	6823133	9728080	100.00%	8.702%
27	15.604	2122	2128	2139	rBV	1077741	1490929	15.33%	1.334%
28	15.740	2146	2151	2156	rVB	33383	50659	0.52%	0.045%
29	16.281	2239	2243	2247	rBV7	10507	15257	0.16%	0.014%
30	16.934	2349	2354	2360	rBV9	9596	17806	0.18%	0.016%
31	17.034	2367	2371	2376	rBV4	9239	14520	0.15%	0.013%
32	17.251	2401	2408	2418	rBV	3515738	5083901	52.26%	4.548%
33	17.351	2419	2425	2438	rVV2	6356495	9100753	93.55%	8.141%
34	18.151	2558	2561	2563	rBV4	9198	12082	0.12%	0.011%
35	19.169	2730	2734	2739	rBV	75374	94743	0.97%	0.085%
36	19.233	2741	2745	2750	rVB	59929	82902	0.85%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018316.D
Acq On : 23 Nov 2023 14:59
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.592	2800	2806	2820	rBV	6654945	8579933	88.20%	7.675%
38	21.357	3100	3106	3114	rBV	3131255	3955701	40.66%	3.539%
39	23.621	3484	3491	3506	rVB2	4204262	8655347	88.97%	7.743%
40	23.780	3511	3518	3534	rVB	2296522	4756342	48.89%	4.255%




Sum of corrected areas: 111786973

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018316.D
Acq On : 23 Nov 2023 14:59
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

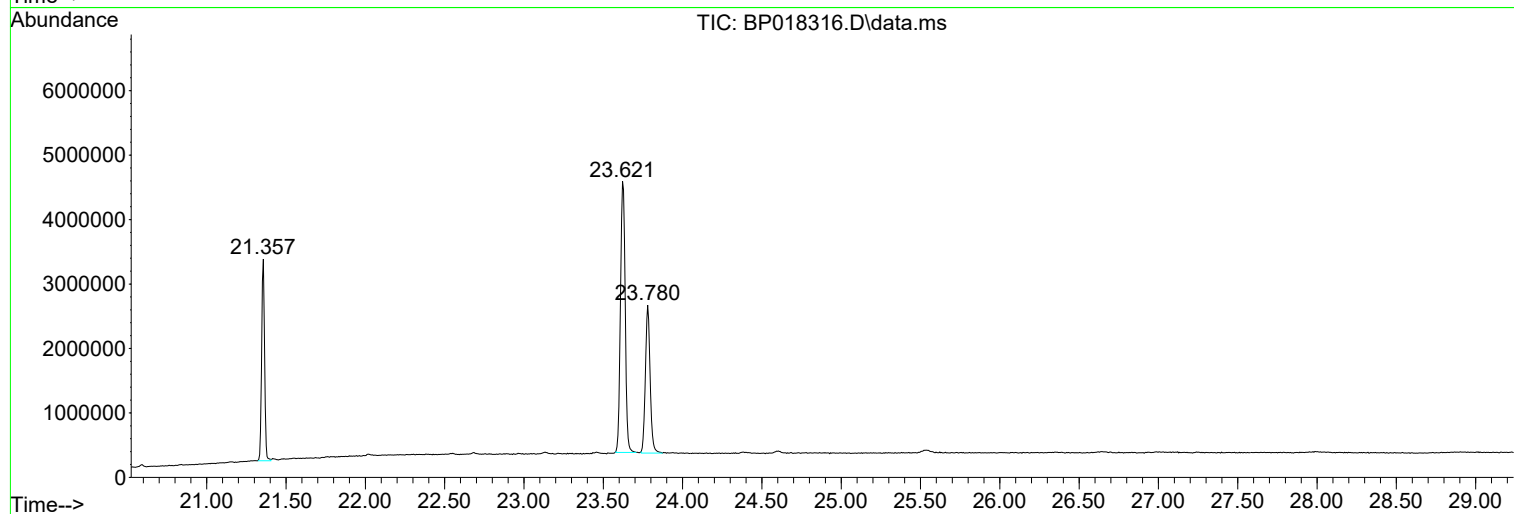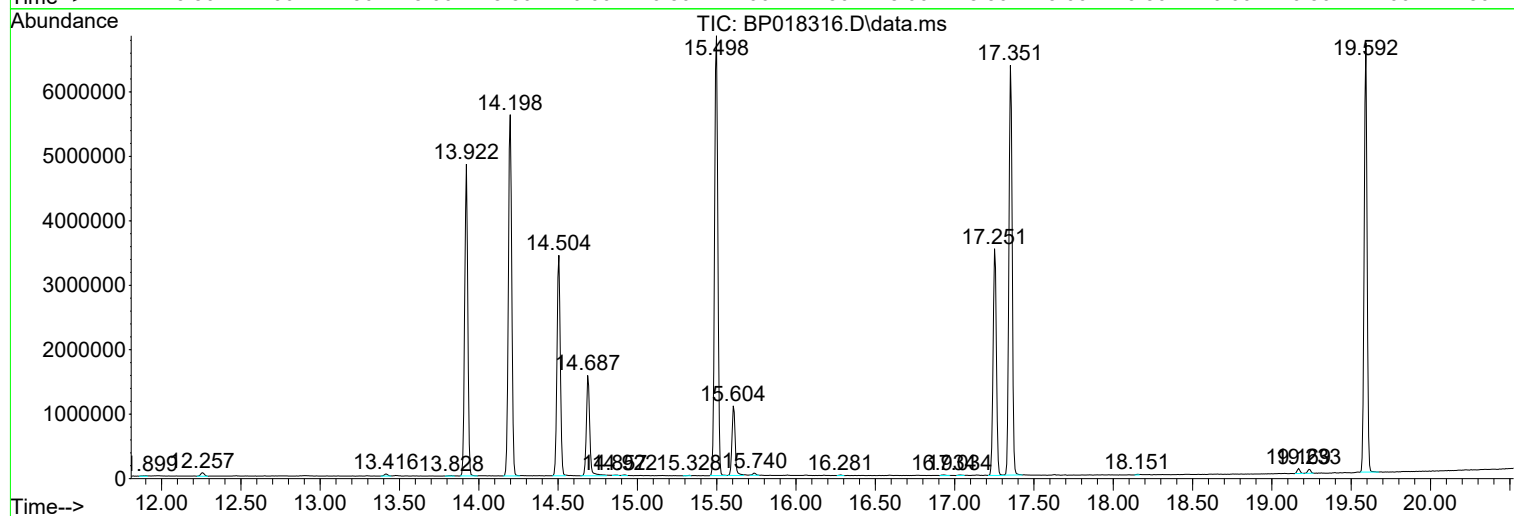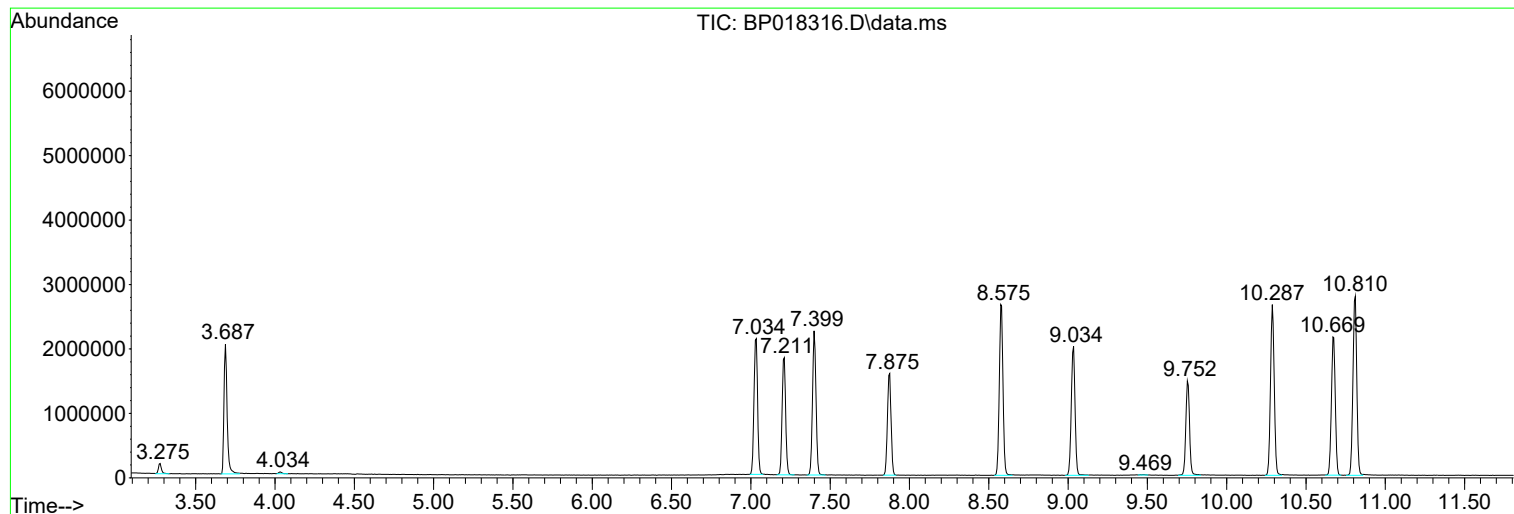

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018316.D
Acq On : 23 Nov 2023 14:59
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018316.D
Acq On : 23 Nov 2023 14:59
Operator : MA/JU
Sample : PB157189BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK189

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------