

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
 Data File : BP018317.D
 Acq On : 23 Nov 2023 15:33
 Operator : MA/JU
 Sample : PB157173BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	38	rBV	160642	204180	1.68%	0.156%
2	3.687	97	102	119	rBV	2185981	3106197	25.50%	2.370%
3	4.034	156	161	166	rBV2	26933	38025	0.31%	0.029%
4	5.564	417	421	427	rBV8	7600	12572	0.10%	0.010%
5	6.793	624	630	634	rBV8	5746	12699	0.10%	0.010%
6	7.034	663	671	683	rVB	2325204	3714673	30.49%	2.834%
7	7.205	694	700	710	rVB	1998000	3132551	25.71%	2.390%
8	7.399	725	733	743	rBV	2438600	3772267	30.96%	2.878%
9	7.869	806	813	821	rBV	1591145	2539259	20.84%	1.937%
10	8.575	925	933	942	rBV	2985310	4824634	39.60%	3.681%
11	9.034	1002	1011	1019	rBV	2265770	3682826	30.23%	2.810%
12	9.205	1035	1040	1047	rBV	8202	14960	0.12%	0.011%
13	9.752	1122	1133	1146	rBV	1623800	2690603	22.08%	2.053%
14	10.287	1214	1224	1236	rBV	3016425	4927868	40.45%	3.760%
15	10.669	1282	1289	1298	rVB	2216722	3822839	31.38%	2.917%
16	10.810	1305	1313	1328	rBV	3184455	5363854	44.03%	4.092%
17	12.257	1553	1559	1566	rBV	63437	96367	0.79%	0.074%
18	13.416	1748	1756	1761	rBV	51742	83779	0.69%	0.064%
19	13.475	1763	1766	1773	rVB6	12830	18673	0.15%	0.014%
20	13.922	1835	1842	1852	rBV	5840765	7934236	65.12%	6.054%
21	14.198	1881	1889	1899	rBV	6676103	9741605	79.96%	7.433%
22	14.504	1932	1941	1948	rBV	3781611	5499404	45.14%	4.196%
23	14.693	1965	1973	1986	rBV	2024169	3000008	24.62%	2.289%
24	14.922	2007	2012	2018	rVB8	13642	24756	0.20%	0.019%
25	15.498	2103	2110	2118	rBV	8102616	11807870	96.92%	9.009%
26	15.604	2122	2128	2141	rBV	1434133	2067248	16.97%	1.577%
27	15.734	2146	2150	2156	rVB	40485	67574	0.55%	0.052%
28	16.181	2218	2226	2231	rBV	9682	19275	0.16%	0.015%
29	16.928	2349	2353	2359	rVB9	13690	23123	0.19%	0.018%
30	17.040	2366	2372	2377	rBV3	11791	23848	0.20%	0.018%
31	17.134	2383	2388	2392	rBV8	9411	16381	0.13%	0.012%
32	17.251	2401	2408	2418	rBV	4422155	6236549	51.19%	4.758%
33	17.351	2418	2425	2438	rVV	8433388	11920459	97.84%	9.095%
34	17.628	2468	2472	2476	rVB2	9787	12887	0.11%	0.010%
35	18.151	2557	2561	2566	rBV7	28681	49594	0.41%	0.038%
36	19.169	2729	2734	2739	rBV	106290	142032	1.17%	0.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018317.D
Acq On : 23 Nov 2023 15:33
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Title : SVOA CALIBRATION

37	19.234	2741	2745	2751	rVV	95812	126982	1.04%	0.097%
38	19.392	2769	2772	2776	rBV5	26058	37440	0.31%	0.029%
39	19.592	2800	2806	2816	rBV	9481826	12183122	100.00%	9.295%
40	20.592	2973	2976	2980	rVB	72301	80469	0.66%	0.061%
41	21.357	3101	3106	3114	rBV	3726397	4611524	37.85%	3.518%
42	23.622	3483	3491	3509	rBV2	4457597	8949836	73.46%	6.828%
43	23.780	3511	3518	3529	rVB	2123451	4432558	36.38%	3.382%




Sum of corrected areas: 131067606

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018317.D
Acq On : 23 Nov 2023 15:33
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

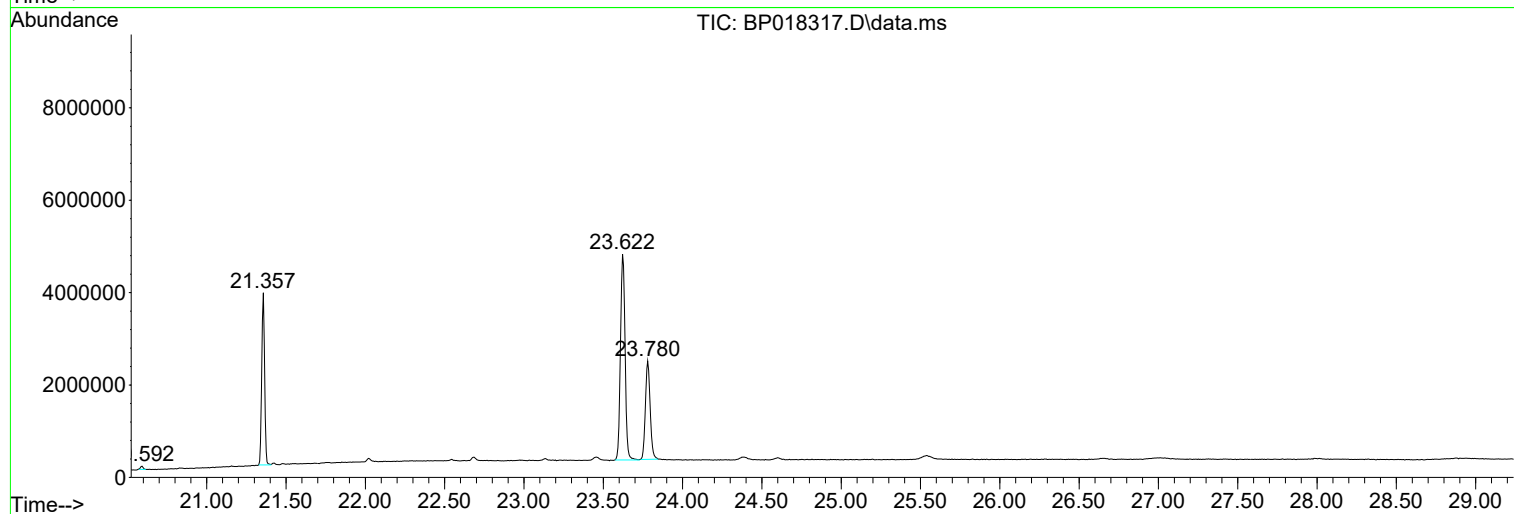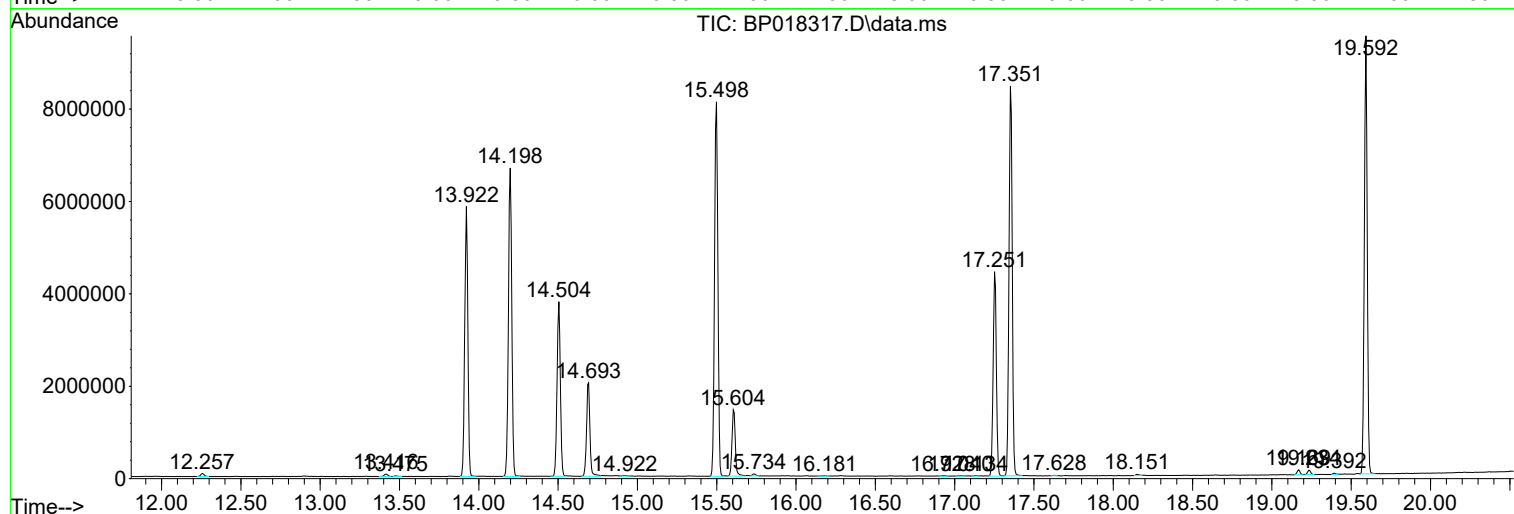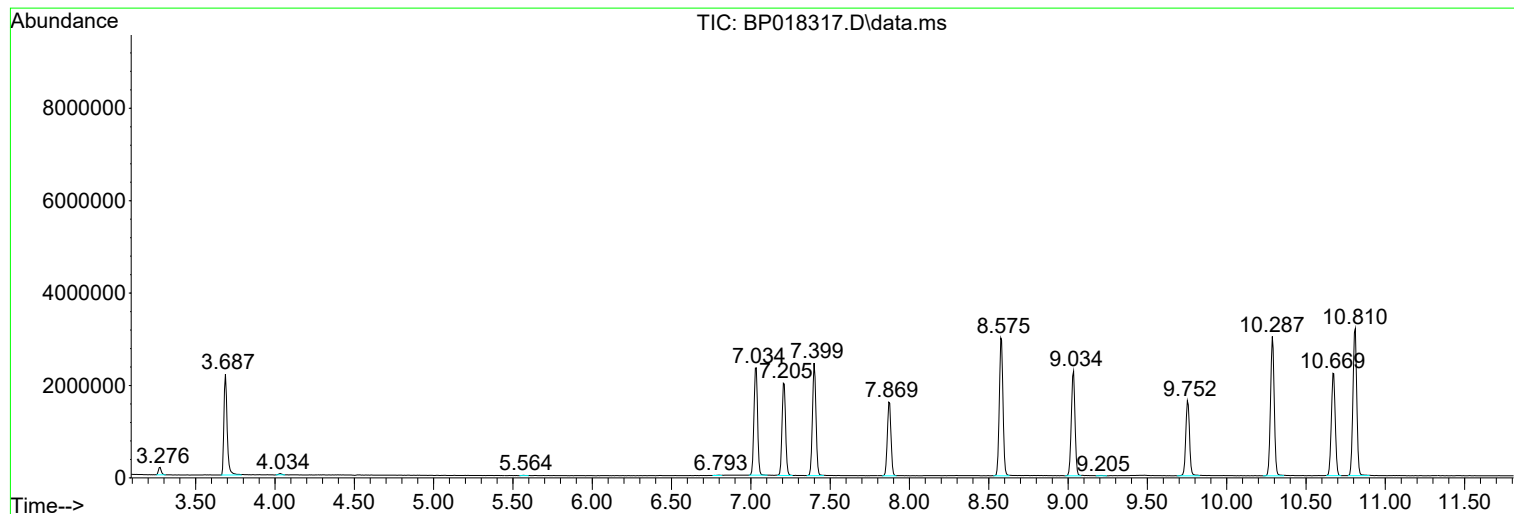

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018317.D
Acq On : 23 Nov 2023 15:33
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112223\
Data File : BP018317.D
Acq On : 23 Nov 2023 15:33
Operator : MA/JU
Sample : PB157173BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------