
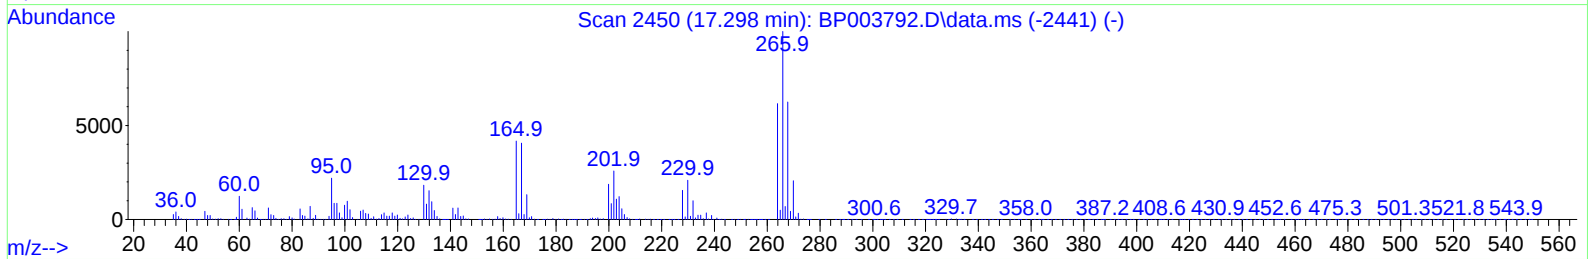
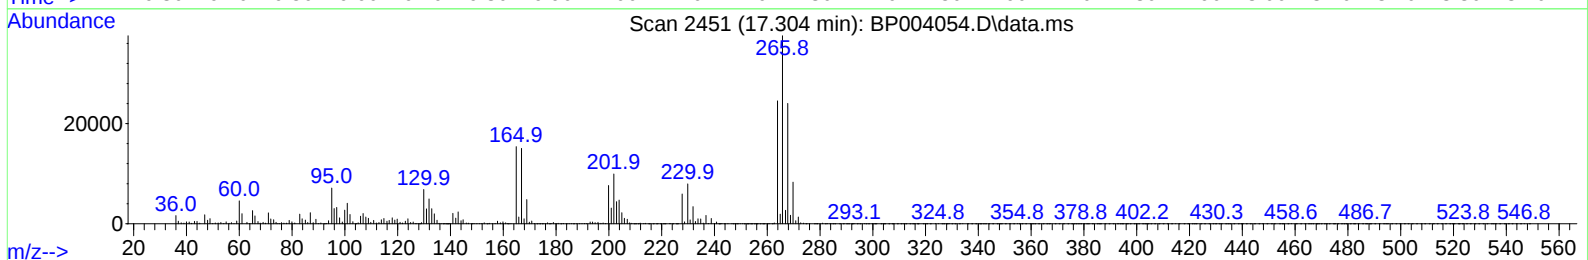


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004054.D
Acq On : 23 Nov 2020 13:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 06:27:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

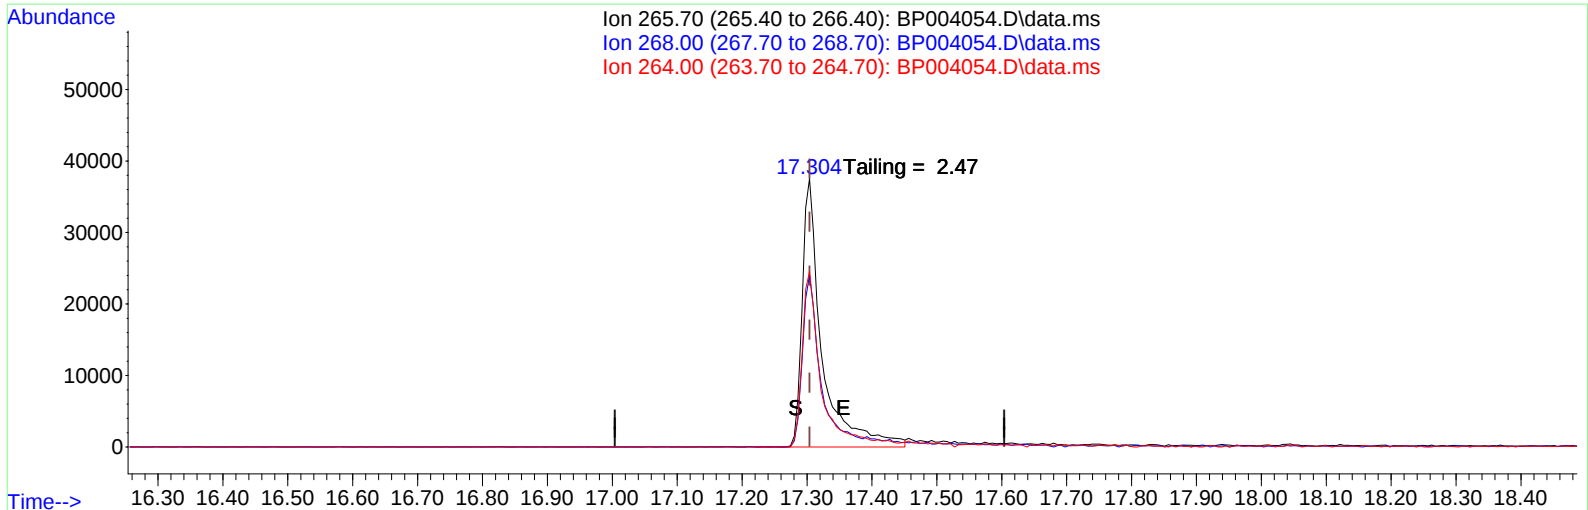

TIC: BP004054.D\data.ms

(70) Pentachlorophenol (C)




17.304min (-0.000) 224247.57 ng

response 81632

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.02
264.00	63.30	65.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004054.D
Acq On : 23 Nov 2020 13:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 06:27:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

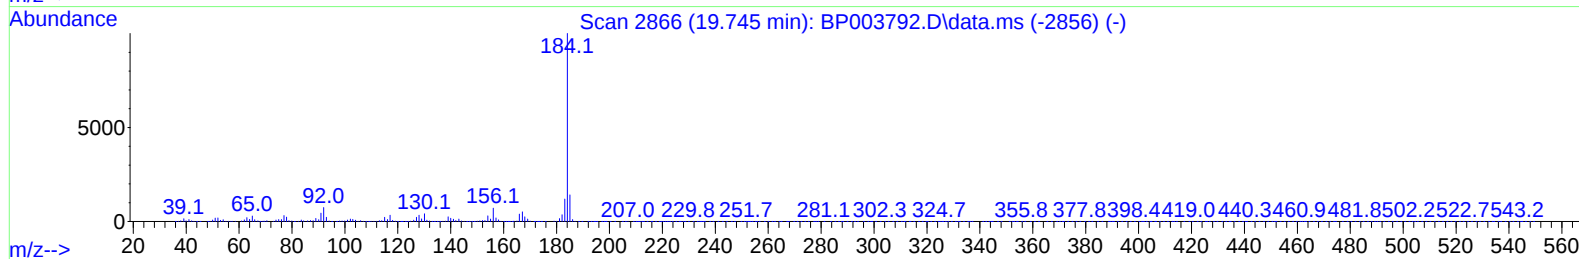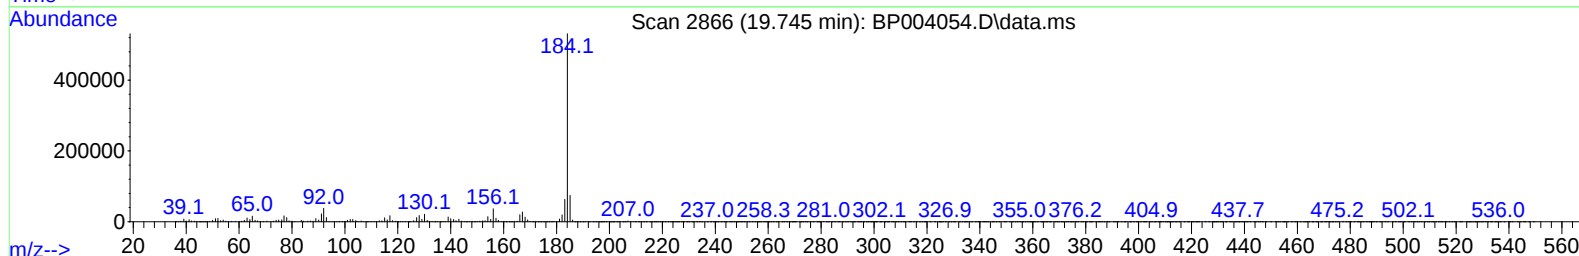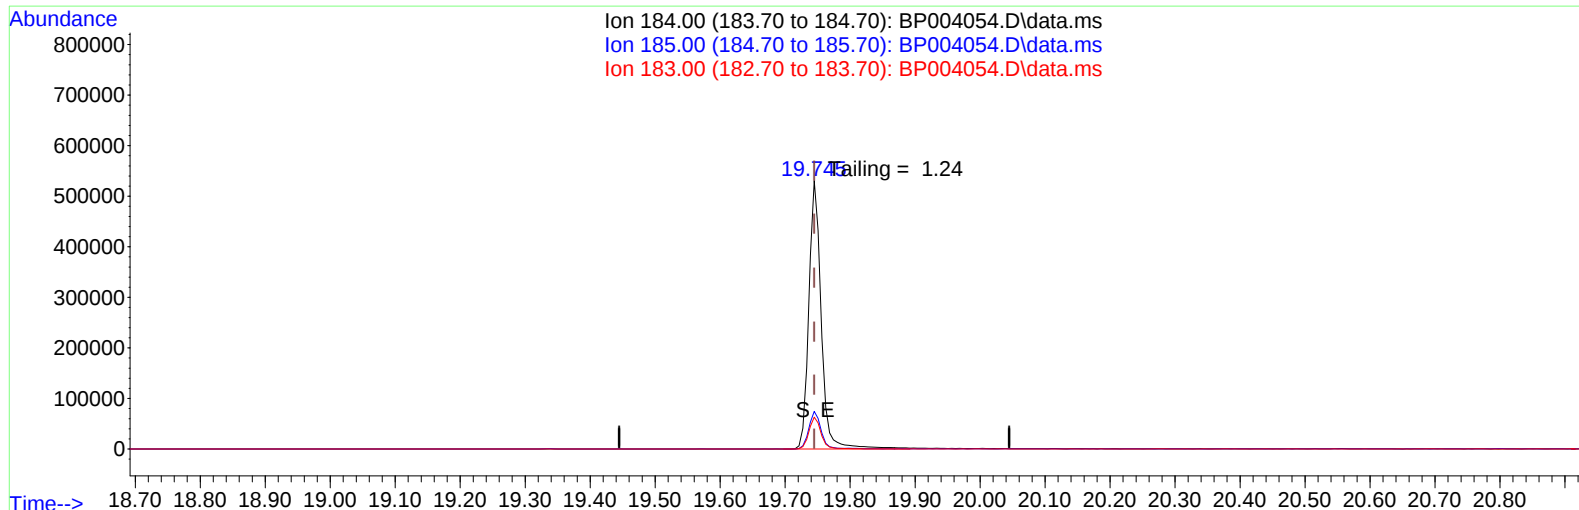

TIC: BP004054.D\data.ms

(77) Benzidine

19.745min (-0.000) 221106.17 ng

response 709289

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.02
183.00	12.00	11.90
0.00	0.00	0.00