

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004064.D
 Acq On : 23 Nov 2020 20:12
 Operator : CG/JU
 Sample : L4857-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 304EM-STOCKPILE

Manual Integrations
 APPROVED

mohammad
 11/25/2020 12:49:53 PM

Quant Time: Nov 24 06:23:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 16:42:41 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.263	152	115482	20.00	ng	0.00
21) Naphthalene-d8	11.098	136	447287	20.00	ng	# 0.00
39) Acenaphthene-d10	14.886	164	281565	20.00	ng	0.00
64) Phenanthrene-d10	17.622	188	566323	20.00	ng	0.00
76) Chrysene-d12	21.657	240	517122	20.00	ng	0.00
86) Perylene-d12	24.127	264	544532	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.805	112	585830	84.67	ng	0.00
7) Phenol-d6	7.451	99	747211	75.23	ng	0.00
23) Nitrobenzene-d5	9.428	82	480845	52.65	ng	0.00
42) 2,4,6-Tribromophenol	16.375	330	253108	71.87	ng	0.00
45) 2-Fluorobiphenyl	13.510	172	1001281	49.72	ng	0.00
79) Terphenyl-d14	20.121	244	1179742	44.08	ng	0.00
Target Compounds						Qvalue
10) Phenol	7.481	94	39431	4.11	ng	78
49) Acenaphthylene	14.610	152	78329	2.97	ng	99
50) Dimethylphthalate	14.310	163	80953	3.68	ng	# 98
71) Phenanthrene	17.663	178	137242	4.32	ng	98
75) Fluoranthene	19.598	202	421316	11.49	ng	98
78) Pyrene	19.945	202	404148	11.52	ng	98
81) Benzo(a)anthracene	21.639	228	208201	6.11	ng	97
83) Chrysene	21.692	228	231521	7.07	ng	97
87) Indeno(1,2,3-cd)pyrene	26.680	276	167843	4.27	ng	# 94
88) Benzo(b)fluoranthene	23.380	252	331965m	9.32	ng	
89) Benzo(k)fluoranthene	23.421	252	100813m	2.87	ng	
90) Benzo(a)pyrene	24.021	252	217253	6.59	ng	98
92) Benzo(g,h,i)perylene	27.474	276	178441	5.63	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004064.D
Acq On : 23 Nov 2020 20:12
Operator : CG/JU
Sample : L4857-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

Manual Integrations
APPROVED

mohammad
11/25/2020 12:49:53 PM

Quant Time: Nov 24 06:23:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 16:42:41 2020
Response via : Initial Calibration

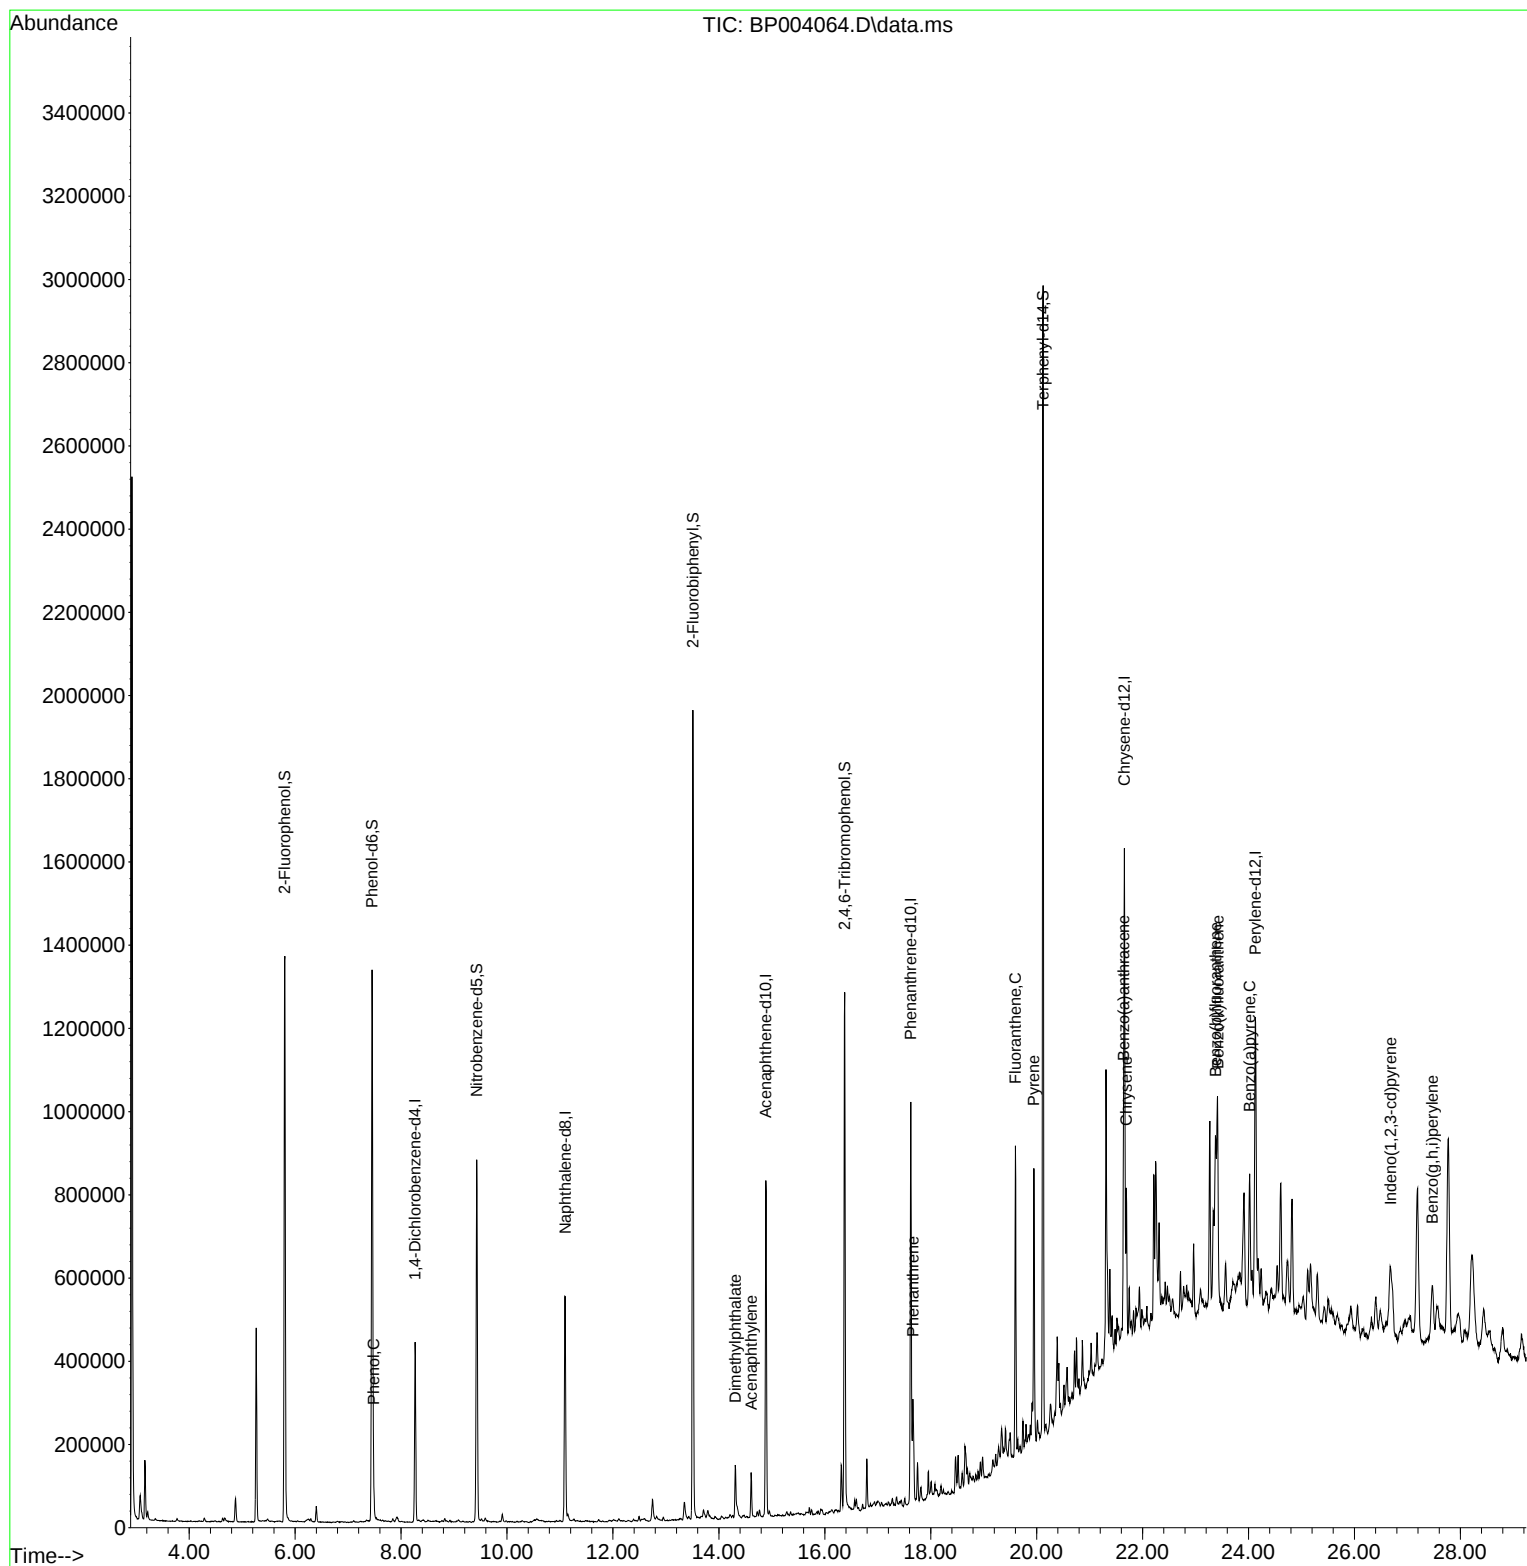







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.263 min Scan# 914
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:152 Resp: 115482
Ion Ratio Lower Upper
152 100
150 151.4 123.8 185.6
115 60.3 43.8 65.6

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Manual Integrations
APPROVED

mohammad
11/25/2020 12:49:53 PM

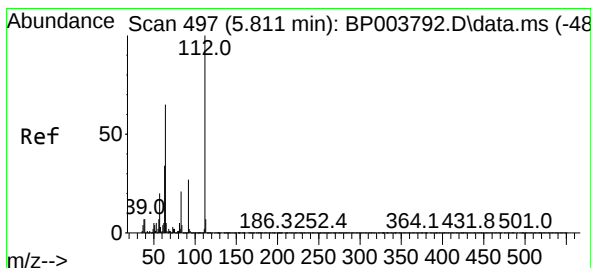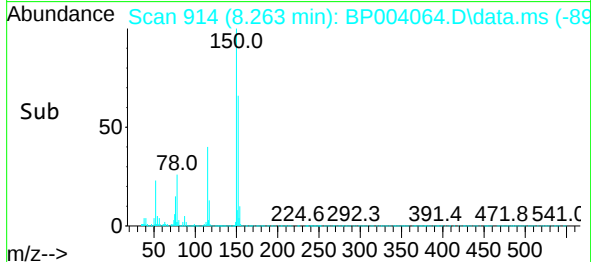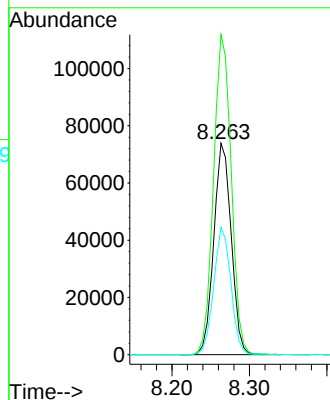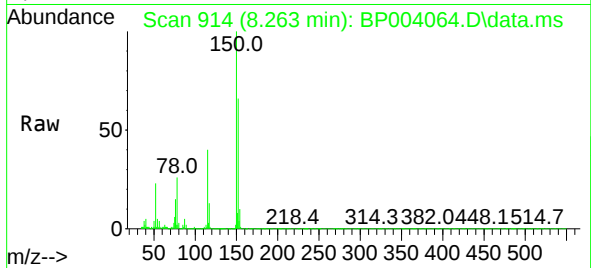

#5
2-Fluorophenol
Concen: 84.67 ng
RT: 5.805 min Scan# 496
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion:112 Resp: 585830
Ion Ratio Lower Upper
112 100
64 63.8 32.8 49.2#
63 33.2 17.0 25.4#

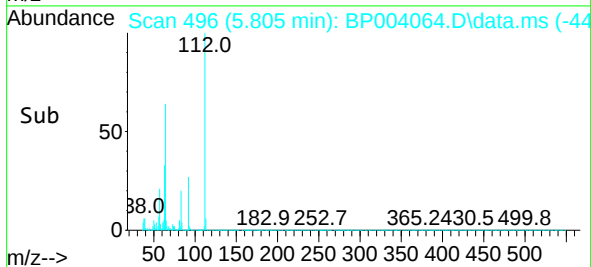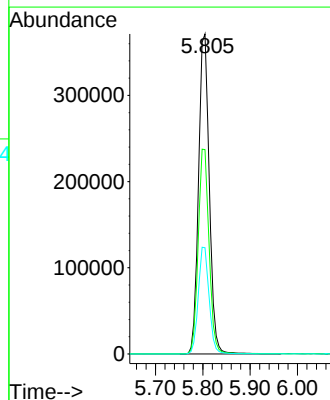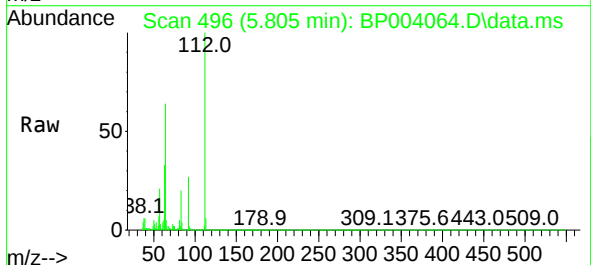



#7
Phenol-d6
Concen: 75.23 ng
RT: 7.451 min Scan# 776
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE



Tgt Ion: 99 Resp: 747211
Ion Ratio Lower Upper
99 100
42 19.3 8.6 13.0#
71 35.9 23.4 35.2#




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

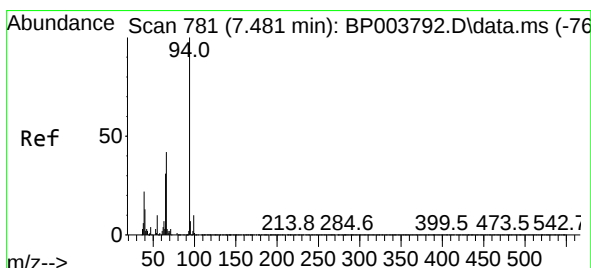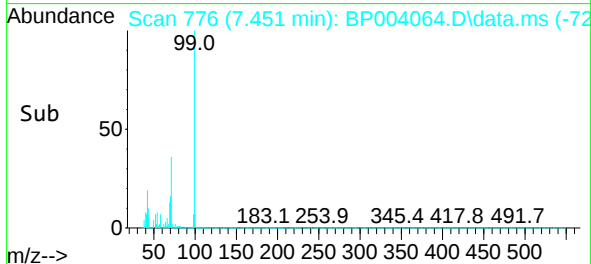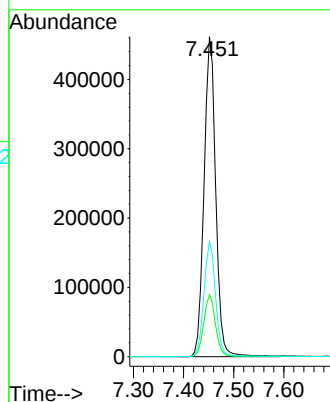

#10
Phenol
Concen: 4.11 ng
RT: 7.481 min Scan# 781
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion: 94 Resp: 39431
Ion Ratio Lower Upper
94 100
65 32.8 2.3 42.3
66 42.7 10.9 50.9

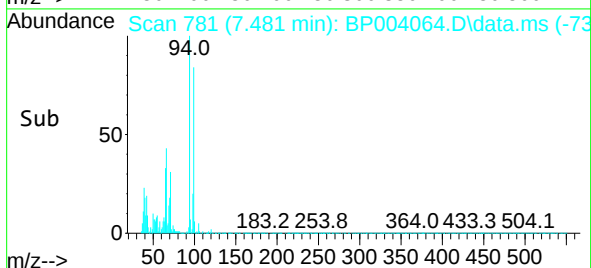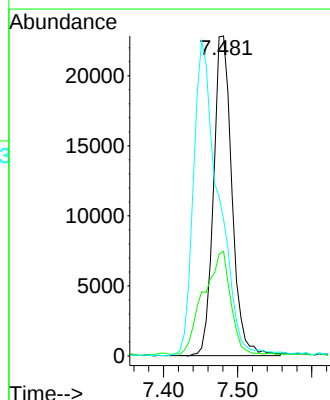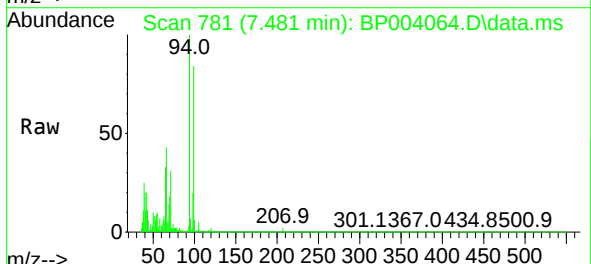



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.098 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

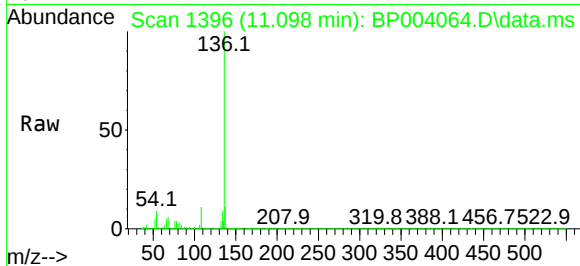

Tgt Ion:136 Resp: 447287
Ion Ratio Lower Upper
136 100
137 10.6 8.6 13.0
54 9.0 3.6 5.4#
68 6.1 3.3 4.9#




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

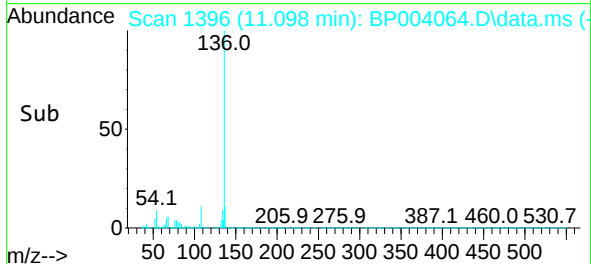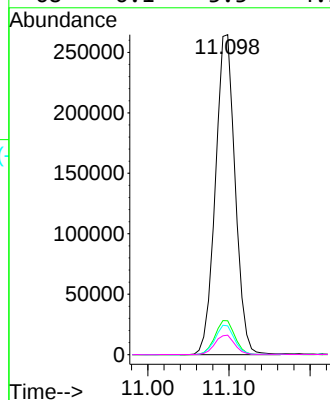

#23
Nitrobenzene-d5
Concen: 52.65 ng
RT: 9.428 min Scan# 1112
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion: 82 Resp: 480845
Ion Ratio Lower Upper
82 100
128 41.3 45.6 68.4#
54 54.2 30.1 45.1#

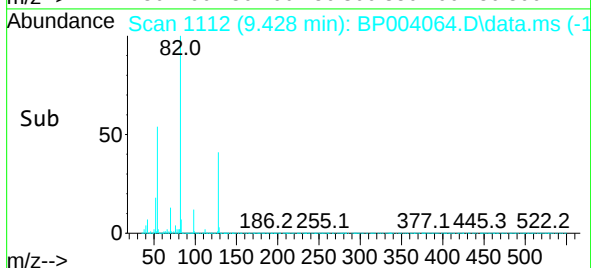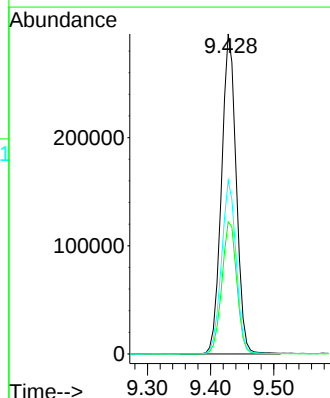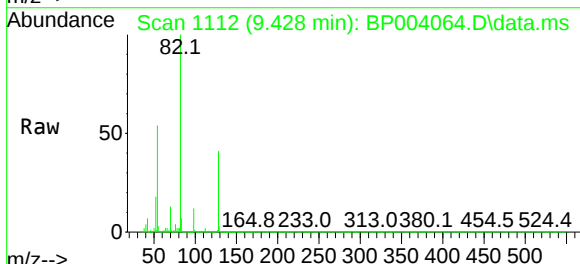



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.886 min Scan# 2040
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

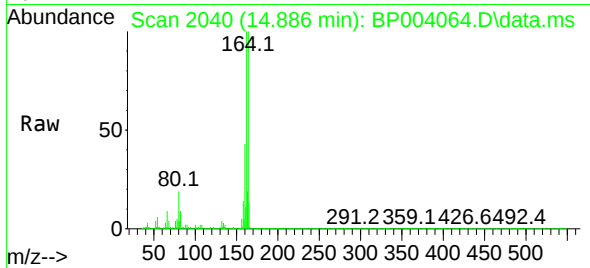


Tgt Ion:164 Resp: 281565
Ion Ratio Lower Upper
164 100
162 99.7 79.4 119.2
160 43.0 36.1 54.1

Manual Integrations
APPROVED



mohammad
11/25/2020 12:49:53 PM

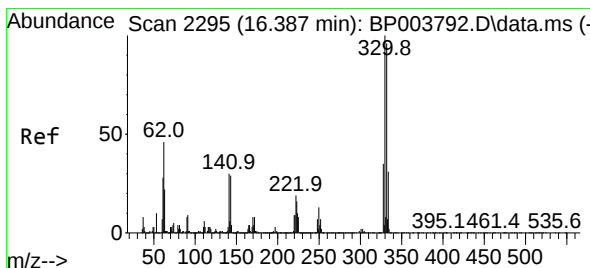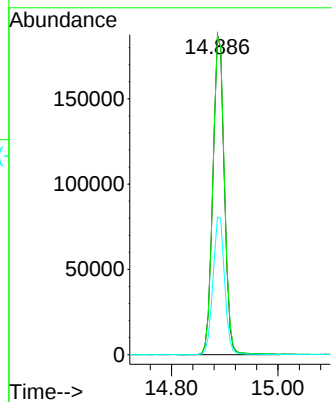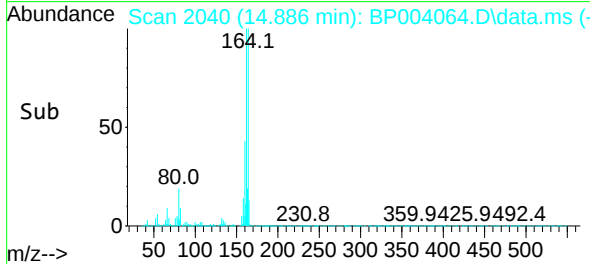


#42
2,4,6-Tribromophenol
Concen: 71.87 ng
RT: 16.375 min Scan# 2293
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

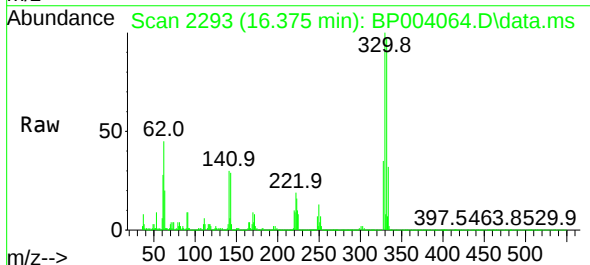


Tgt Ion:330 Resp: 253108
Ion Ratio Lower Upper
330 100
332 96.7 77.1 115.7
141 31.1 23.4 35.2

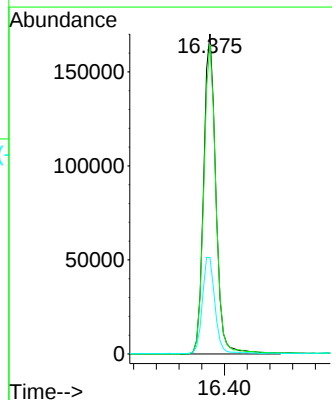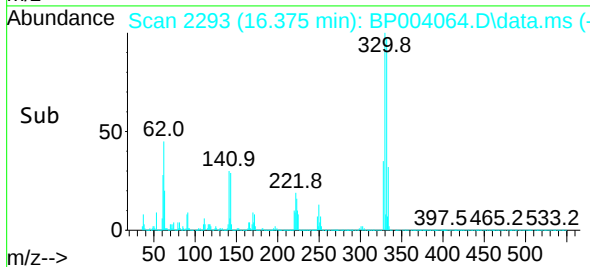

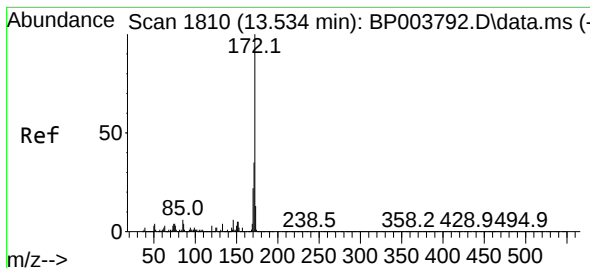

#45
2-Fluorobiphenyl
Concen: 49.72 ng
RT: 13.510 min Scan# 1806
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

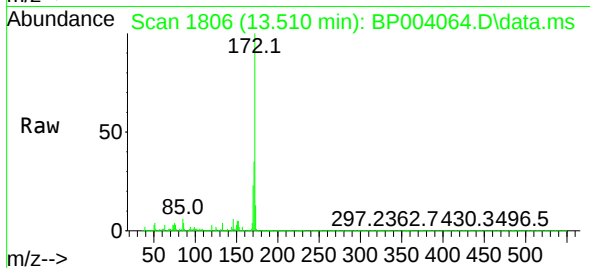

Tgt Ion:172 Resp: 1001281
Ion Ratio Lower Upper
172 100
171 35.3 28.5 42.7
170 22.9 19.2 28.8




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

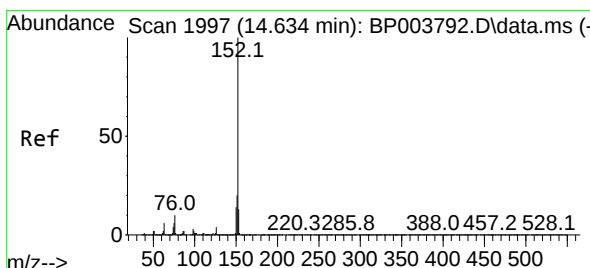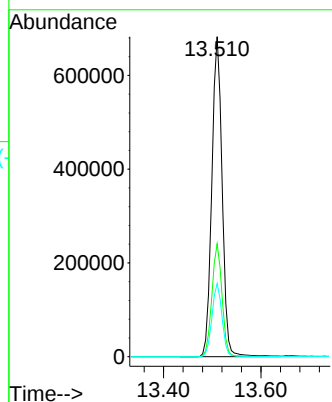

#49
Acenaphthylene
Concen: 2.97 ng
RT: 14.610 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:152 Resp: 78329
Ion Ratio Lower Upper
152 100
151 20.2 15.9 23.9
153 13.8 10.5 15.7

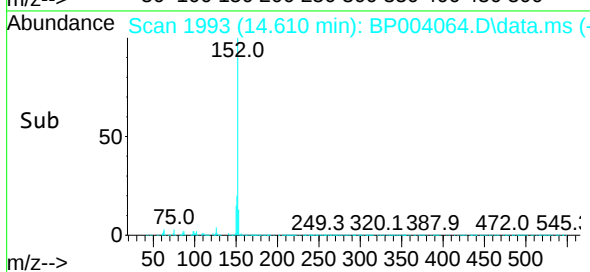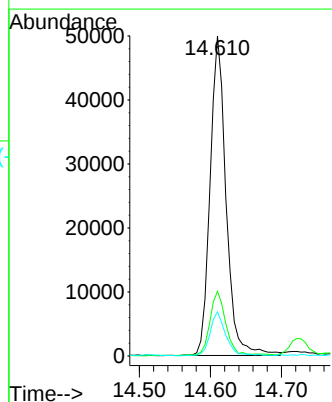







#50
Dimethylphthalate
Concen: 3.68 ng
RT: 14.310 min Scan# 1942
Delta R.T. -0.012 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:163 Resp: 80953
Ion Ratio Lower Upper
163 100
194 5.2 3.3 4.9#
164 9.8 8.2 12.2

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

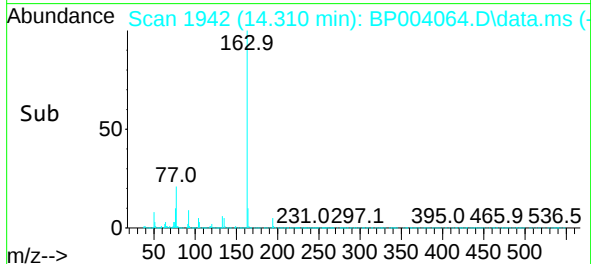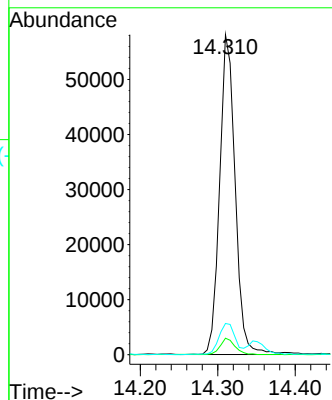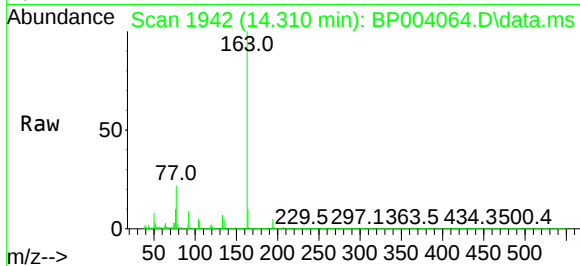

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.622 min Scan# 2505
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion:188 Resp: 566323
Ion Ratio Lower Upper
188 100
94 8.1 6.2 9.2
80 9.0 6.2 9.2

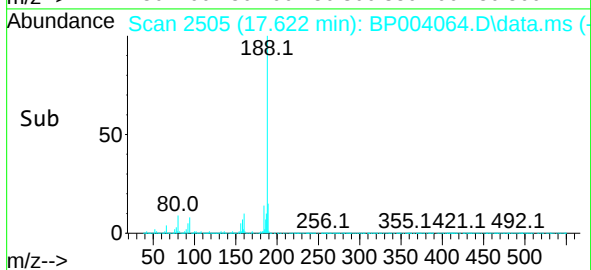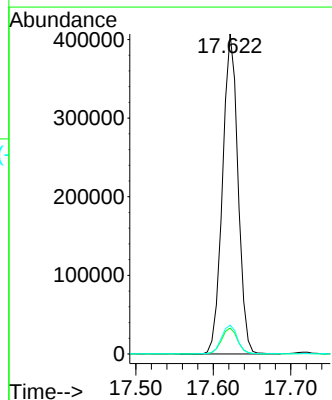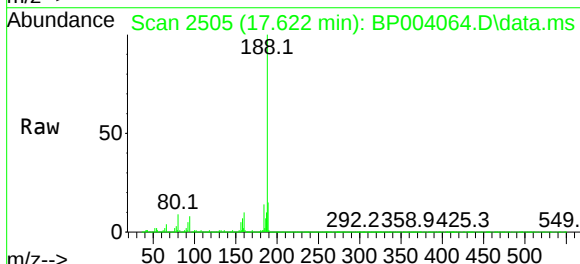



#71
Phenanthrene
Concen: 4.32 ng
RT: 17.663 min Scan# 2512
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE



Tgt Ion:178 Resp: 137242
Ion Ratio Lower Upper
178 100
176 17.9 15.3 22.9
179 16.4 12.5 18.7




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

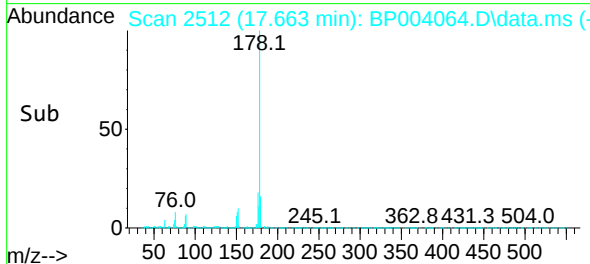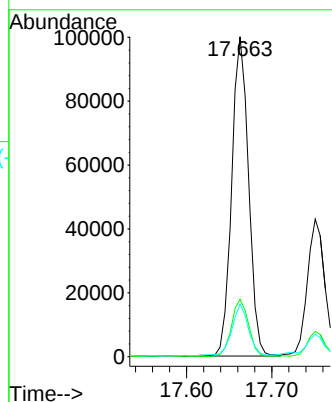

#75
Fluoranthene
Concen: 11.49 ng
RT: 19.598 min Scan# 2841
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:202 Resp: 421316
Ion Ratio Lower Upper
202 100
101 10.2 0.0 29.4
203 18.6 0.0 37.8

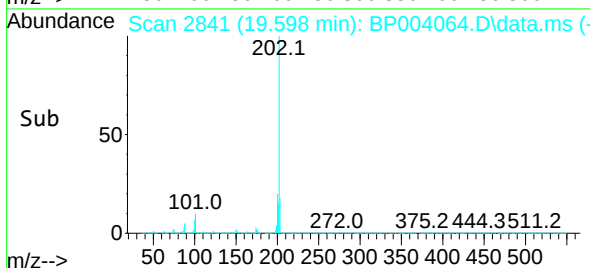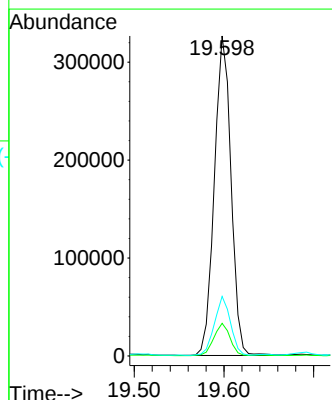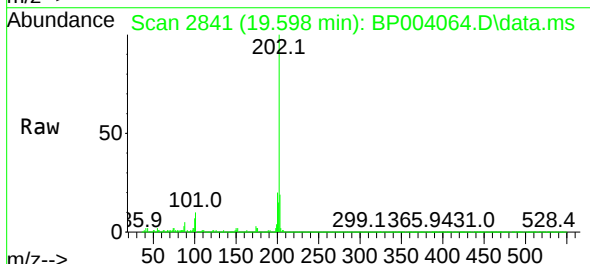







#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.657 min Scan# 3191
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:240 Resp: 517122
Ion Ratio Lower Upper
240 100
120 8.8 7.8 11.6
236 24.4 20.8 31.2

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

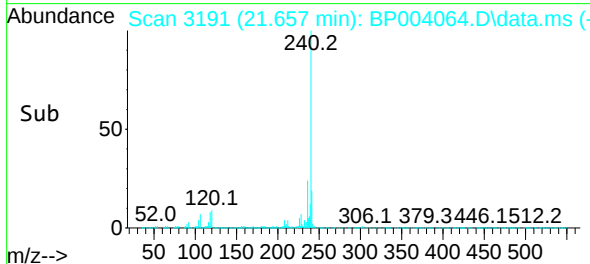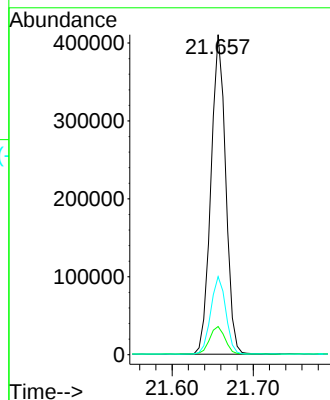

#78
Pyrene
Concen: 11.52 ng
RT: 19.945 min Scan# 2900
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:202 Resp: 404148
Ion Ratio Lower Upper
202 100
200 20.0 17.1 25.7
203 17.9 14.2 21.2

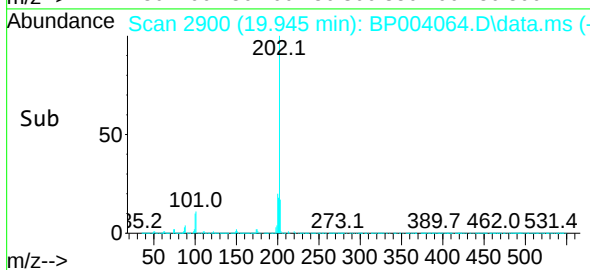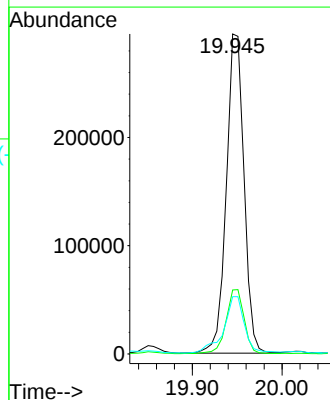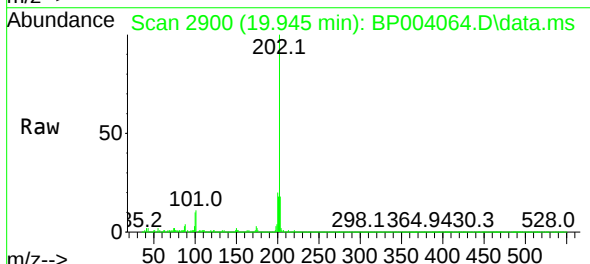







#79
Terphenyl-d14
Concen: 44.08 ng
RT: 20.121 min Scan# 2930
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Tgt Ion:244 Resp: 1179742
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 8.7 7.8 11.8

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

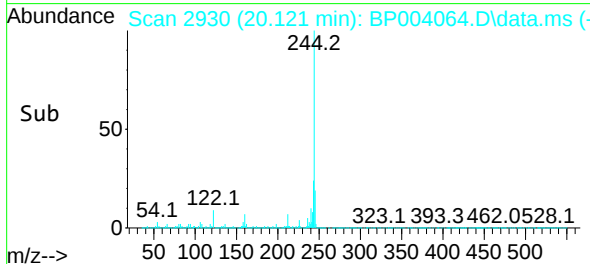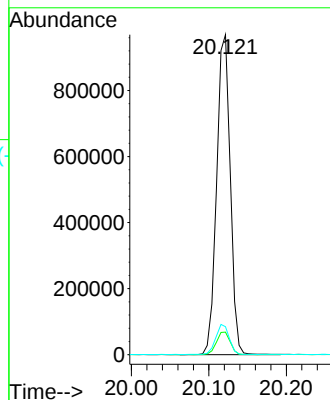

#81
Benzo(a)anthracene
Concen: 6.11 ng
RT: 21.639 min Scan# 3188
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion:228 Resp: 208201
Ion Ratio Lower Upper
228 100
226 26.5 22.1 33.1
229 21.6 15.9 23.9

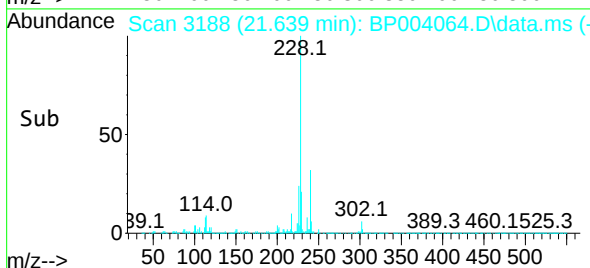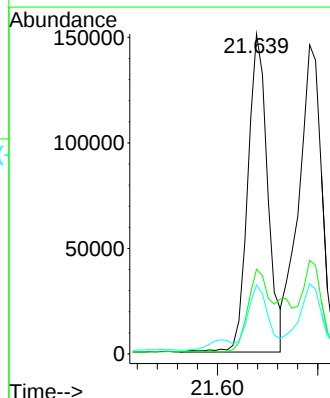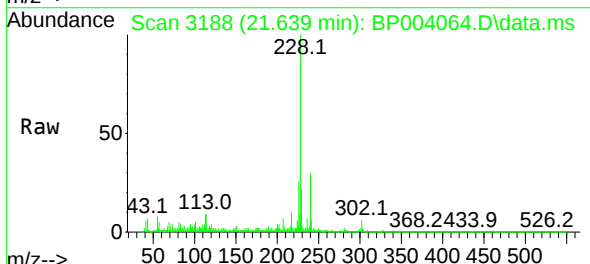



#83
Chrysene
Concen: 7.07 ng
RT: 21.692 min Scan# 3197
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Tgt Ion:228 Resp: 231521
Ion Ratio Lower Upper
228 100
226 30.3 24.4 36.6
229 22.7 15.8 23.6

Manual Integrations
APPROVED



mohammad
11/25/2020 12:49:53 PM

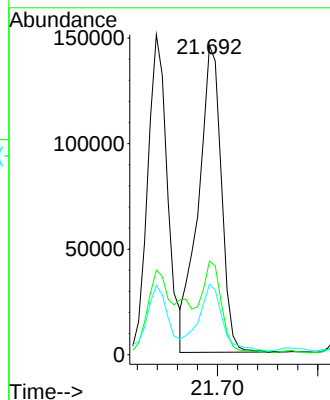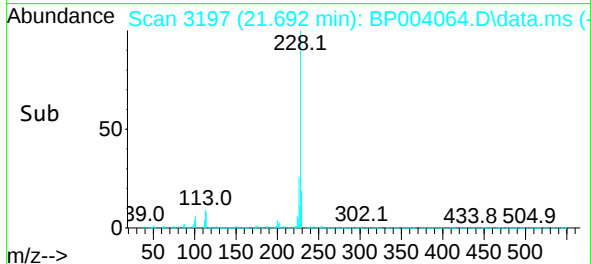


#86
Perylene-d12
Concen: 20.00 ng
RT: 24.127 min Scan# 3611
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

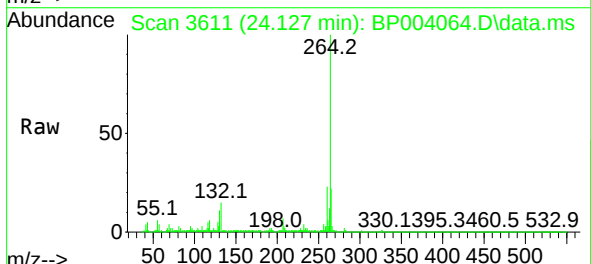


Tgt Ion:264 Resp: 544532
Ion Ratio Lower Upper
264 100
260 22.8 18.8 28.2
265 21.8 17.4 26.2

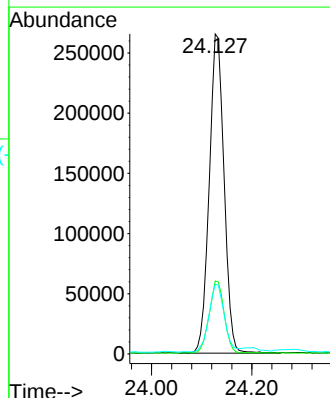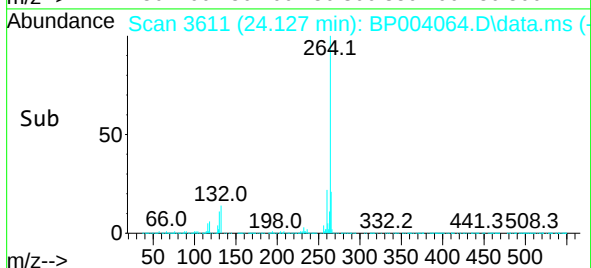



#87
Indeno(1,2,3-cd)pyrene
Concen: 4.27 ng
RT: 26.680 min Scan# 4045
Delta R.T. -0.012 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE




Tgt Ion: 276 Resp: 167843
Ion Ratio Lower Upper
276 100
138 18.1 18.7 28.1#
277 24.7 20.4 30.6

Manual Integrations
APPROVED



mohammad
11/25/2020 12:49:53 PM

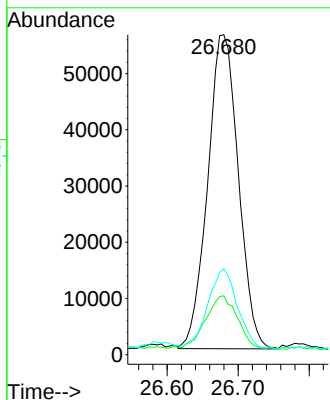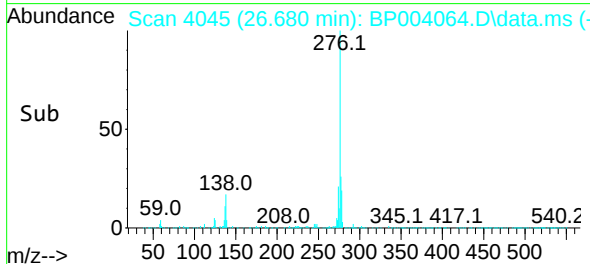


#88
Benzo(b)fluoranthene
Concen: 9.32 ng m
RT: 23.380 min Scan# 3484
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

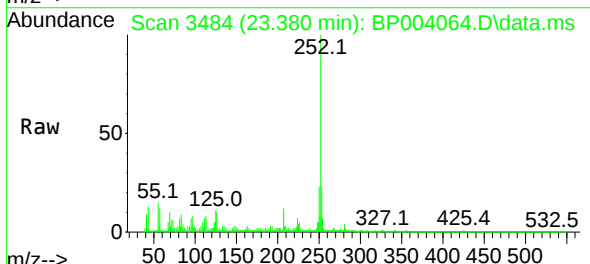


Tgt Ion: 252 Resp: 331965
Ion Ratio Lower Upper
252 100
253 22.9 17.6 26.4
125 11.4 7.3 10.9#

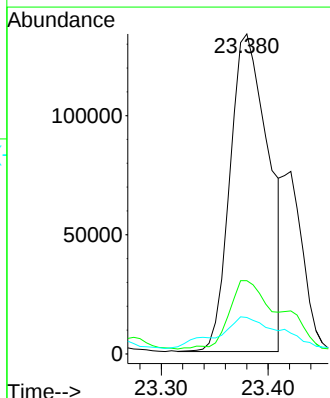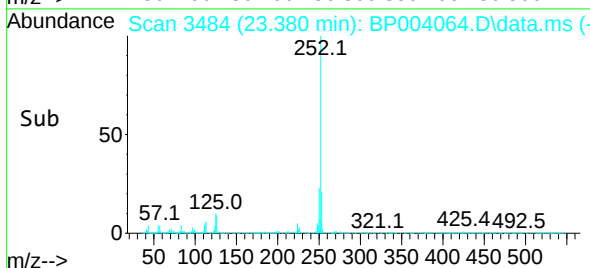



#89
Benzo(k)fluoranthene
Concen: 2.87 ng m
RT: 23.421 min Scan# 3491
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12




Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE



Tgt Ion:252 Resp: 100813
Ion Ratio Lower Upper
252 100
253 23.5 17.8 26.8
125 11.4 7.4 11.2#




Manual Integrations
APPROVED


mohammad
11/25/2020 12:49:53 PM

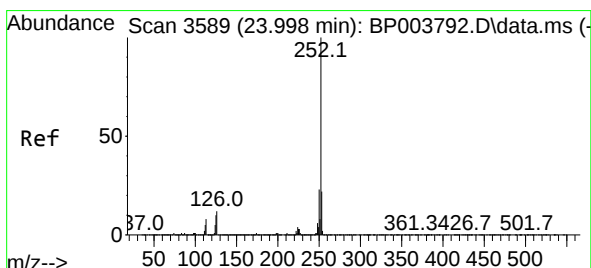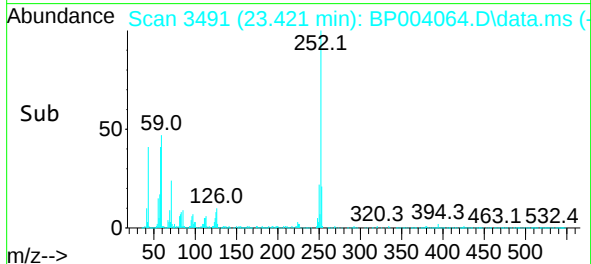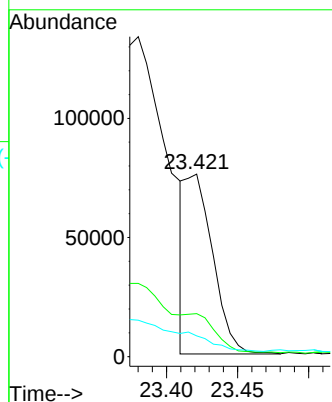

#90
Benzo(a)pyrene
Concen: 6.59 ng
RT: 24.021 min Scan# 3593
Delta R.T. 0.000 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12


Tgt Ion:252 Resp: 217253
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.0
125 10.0 8.2 12.4

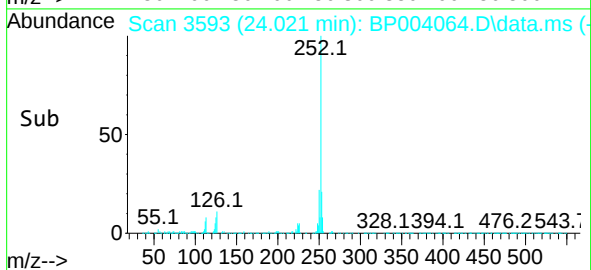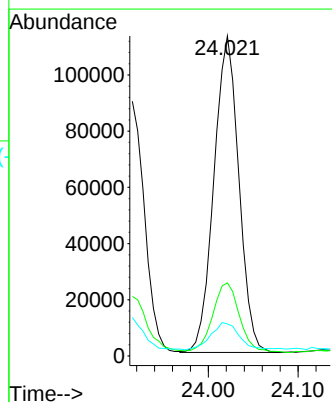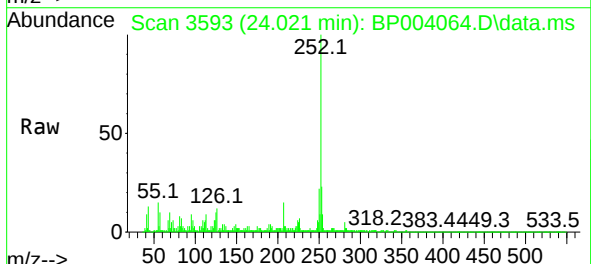

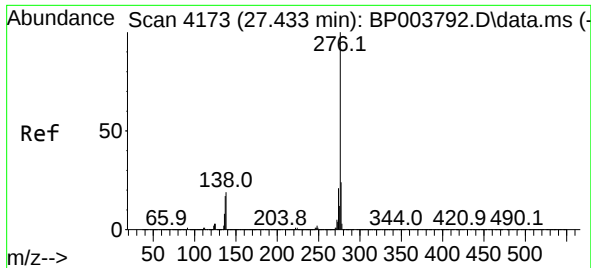

#92
Benzo(g,h,i)perylene
Concen: 5.63 ng
RT: 27.474 min Scan# 4180
Delta R.T. -0.006 min
Lab File: BP004064.D
Acq: 23 Nov 2020 20:12

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE



Tgt Ion:276 Resp: 178441
Ion Ratio Lower Upper
276 100
277 26.3 19.0 28.6
138 20.6 16.6 24.8

Manual Integrations
APPROVED

mohammad
11/25/2020 12:49:53 PM

