

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004062.D
 Acq On : 23 Nov 2020 19:04
 Operator : CG/JU
 Sample : L4857-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 340EM-STOCKPILE-EAST

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.917	3	5	24	rVB	7323196	7964427	100.00%	11.768%
2	3.075	26	32	42	rVB	90261	168562	2.12%	0.249%
3	3.164	42	47	52	rBV	238190	284446	3.57%	0.420%
4	5.264	398	404	411	rBV	559742	805627	10.12%	1.190%
5	5.799	487	495	512	rBV	1908955	2926673	36.75%	4.324%
6	7.452	769	776	790	rVB	1808943	3031113	38.06%	4.479%
7	8.263	907	914	922	rVB	480426	742082	9.32%	1.096%
8	9.428	1095	1112	1122	rBV	1146753	1950188	24.49%	2.882%
9	11.093	1385	1395	1400	rBV	583464	1053756	13.23%	1.557%
10	11.146	1400	1404	1414	rVB	124357	215361	2.70%	0.318%
11	12.110	1561	1568	1572	rBV	50988	80339	1.01%	0.119%
12	12.487	1627	1632	1637	rBV	62519	87941	1.10%	0.130%
13	12.728	1663	1673	1684	rVB	120588	218569	2.74%	0.323%
14	12.951	1704	1711	1718	rVB	73855	120798	1.52%	0.178%
15	13.510	1798	1806	1819	rBV	2443085	3596618	45.16%	5.314%
16	13.710	1835	1840	1848	rBV2	94707	164772	2.07%	0.243%
17	14.210	1920	1925	1930	rBV	65285	105904	1.33%	0.156%
18	14.310	1938	1942	1948	rBV	107882	184430	2.32%	0.273%
19	14.610	1988	1993	1999	rVB	81021	112407	1.41%	0.166%
20	14.763	2016	2019	2024	rVB	81474	98512	1.24%	0.146%
21	14.887	2035	2040	2046	rVB	828896	1186252	14.89%	1.753%
22	14.951	2046	2051	2057	rVB	113679	172615	2.17%	0.255%
23	15.281	2100	2107	2113	rBV	119202	184333	2.31%	0.272%
24	15.710	2176	2180	2183	rVB	95333	121975	1.53%	0.180%
25	15.928	2211	2217	2223	rBV2	142848	247337	3.11%	0.365%
26	16.375	2287	2293	2305	rBV	1807979	2713773	34.07%	4.010%
27	16.563	2321	2325	2327	rBV	100217	117865	1.48%	0.174%
28	16.592	2327	2330	2340	rVB2	116460	175724	2.21%	0.260%
29	17.157	2418	2426	2430	rBV6	37604	96667	1.21%	0.143%
30	17.269	2441	2445	2454	rBV2	79849	140564	1.76%	0.208%
31	17.351	2454	2459	2465	rVV	116743	155212	1.95%	0.229%
32	17.439	2471	2474	2482	rVB	95571	140105	1.76%	0.207%
33	17.622	2499	2505	2508	rBV	1019687	1436586	18.04%	2.123%
34	17.663	2508	2512	2518	rVV	1574112	2165493	27.19%	3.200%
35	17.751	2522	2527	2532	rVV	387330	536021	6.73%	0.792%
36	17.804	2532	2536	2542	rVB4	51328	92523	1.16%	0.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004062.D
 Acq On : 23 Nov 2020 19:04
 Operator : CG/JU
 Sample : L4857-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 340EM-STOCKPILE-EAST

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.004	2564	2570	2575	rBV2	166954	268445	3.37%	0.397%
38	18.075	2579	2582	2586	rVB	80691	90506	1.14%	0.134%
39	18.469	2645	2649	2653	rBV	184879	254112	3.19%	0.375%
40	18.516	2653	2657	2662	rVB	286239	386134	4.85%	0.571%
41	18.592	2666	2670	2675	rVB	74254	98637	1.24%	0.146%
42	18.663	2675	2682	2685	rBV2	264378	501643	6.30%	0.741%
43	18.692	2685	2687	2691	rVB	123414	126627	1.59%	0.187%
44	18.733	2691	2694	2698	rBV2	87090	110842	1.39%	0.164%
45	18.933	2724	2728	2732	rBV	181200	252598	3.17%	0.373%
46	18.980	2732	2736	2746	rVB2	132490	237891	2.99%	0.352%
47	19.175	2762	2769	2773	rBV3	82744	143718	1.80%	0.212%
48	19.339	2792	2797	2803	rBV3	197743	368060	4.62%	0.544%
49	19.480	2817	2821	2822	rBV2	107307	131769	1.65%	0.195%
50	19.598	2835	2841	2846	rBV	2521301	3245953	40.76%	4.796%
51	19.645	2846	2849	2852	rBV	75031	80815	1.01%	0.119%
52	19.686	2852	2856	2860	rVB3	68886	100931	1.27%	0.149%
53	19.739	2861	2865	2868	rBV2	50890	82703	1.04%	0.122%
54	19.916	2891	2895	2897	rBV2	349543	521648	6.55%	0.771%
55	19.951	2897	2901	2907	rVV	2042044	2754839	34.59%	4.071%
56	20.016	2908	2912	2917	rVB2	135711	191414	2.40%	0.283%
57	20.122	2924	2930	2935	rBV	3682864	4559176	57.24%	6.737%
58	20.174	2936	2939	2945	rVB	105965	158759	1.99%	0.235%
59	20.257	2946	2953	2959	rBV3	123677	305491	3.84%	0.451%
60	20.386	2971	2975	2977	rBV3	149303	193860	2.43%	0.286%
61	20.422	2977	2981	2989	rVB	305692	448375	5.63%	0.663%
62	20.516	2993	2997	3001	rBV	214146	272792	3.43%	0.403%
63	20.574	3001	3007	3010	rVB2	161464	228358	2.87%	0.337%
64	20.710	3027	3030	3033	rBV	115139	151531	1.90%	0.224%
65	20.751	3033	3037	3043	rVB2	394434	483118	6.07%	0.714%
66	20.863	3053	3056	3059	rVB2	126282	137712	1.73%	0.203%
67	21.139	3099	3103	3109	rVB	218955	301676	3.79%	0.446%
68	21.310	3125	3132	3135	rBV4	628907	1010532	12.69%	1.493%
69	21.386	3141	3145	3148	rBV2	227556	291389	3.66%	0.431%
70	21.427	3148	3152	3158	rVB2	178671	278063	3.49%	0.411%
71	21.516	3163	3167	3169	rBV	123615	153189	1.92%	0.226%
72	21.645	3183	3189	3194	rBV2	1509825	3311801	41.58%	4.893%
73	21.692	3194	3197	3203	rVV	990042	1398221	17.56%	2.066%
74	21.745	3204	3206	3209	rVB	111578	108868	1.37%	0.161%
75	21.827	3216	3220	3224	rBV	240256	332064	4.17%	0.491%
76	21.874	3226	3228	3233	rVV2	57201	100024	1.26%	0.148%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004062.D
 Acq On : 23 Nov 2020 19:04
 Operator : CG/JU
 Sample : L4857-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 340EM-STOCKPILE-EAST

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	21.986	3243	3247	3253	rBV2	157866	261997	3.29%	0.387%
78	22.216	3283	3286	3288	rBV	105965	139398	1.75%	0.206%
79	22.304	3297	3301	3306	rVB	141730	215600	2.71%	0.319%
80	22.468	3325	3329	3333	rBV3	99506	157587	1.98%	0.233%
81	22.568	3342	3346	3352	rVB3	91842	158777	1.99%	0.235%
82	23.268	3461	3465	3473	rVB2	130979	207511	2.61%	0.307%
83	23.380	3477	3484	3489	rBV	804862	2025037	25.43%	2.992%
84	23.568	3511	3516	3522	rBV	157596	272914	3.43%	0.403%
85	23.910	3568	3574	3583	rVB	516277	1152157	14.47%	1.702%
86	24.015	3586	3592	3602	rVV	736349	1481589	18.60%	2.189%
87	24.127	3604	3611	3617	rVV2	732540	1554502	19.52%	2.297%
88	24.180	3617	3620	3627	rVB2	222863	417001	5.24%	0.616%
89	26.674	4036	4044	4056	rVB3	358215	1118821	14.05%	1.653%
90	27.462	4171	4178	4190	rVB	248785	745101	9.36%	1.101%




Sum of corrected areas: 67677846

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004062.D
Acq On : 23 Nov 2020 19:04
Operator : CG/JU
Sample : L4857-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-EAST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

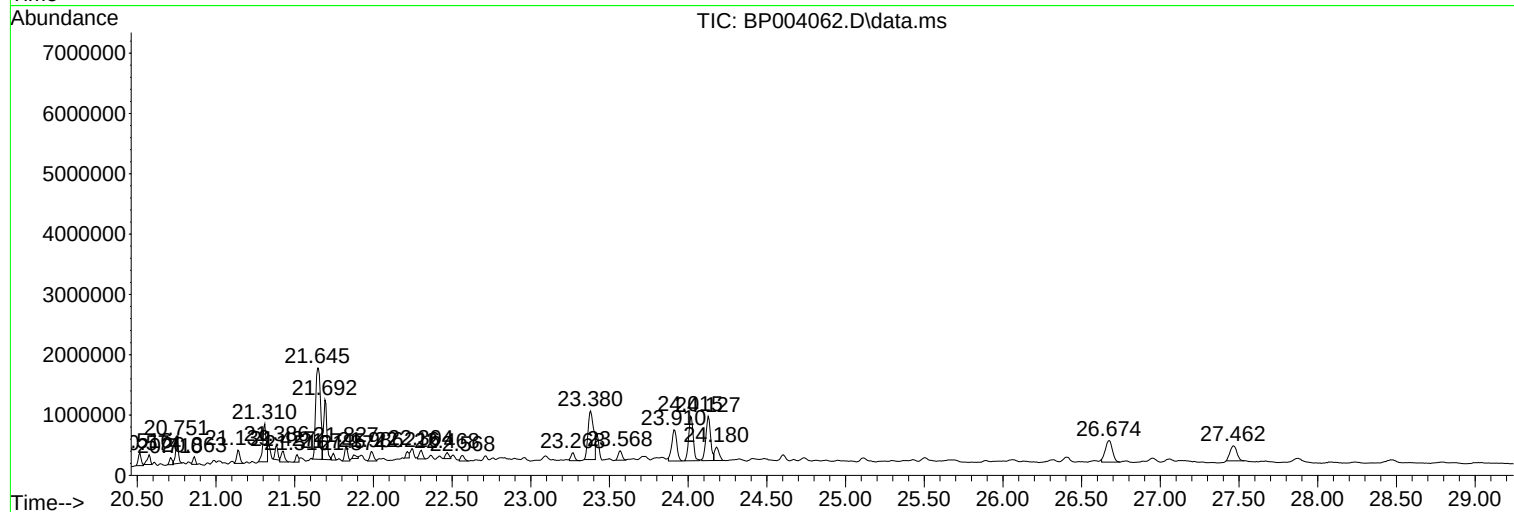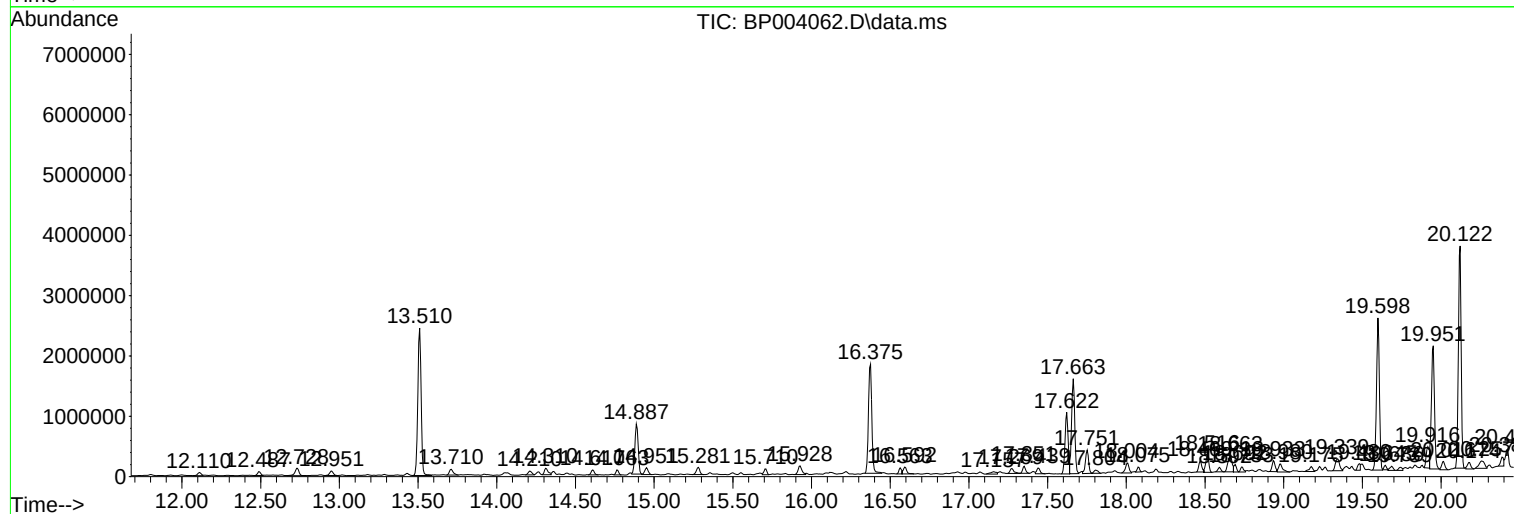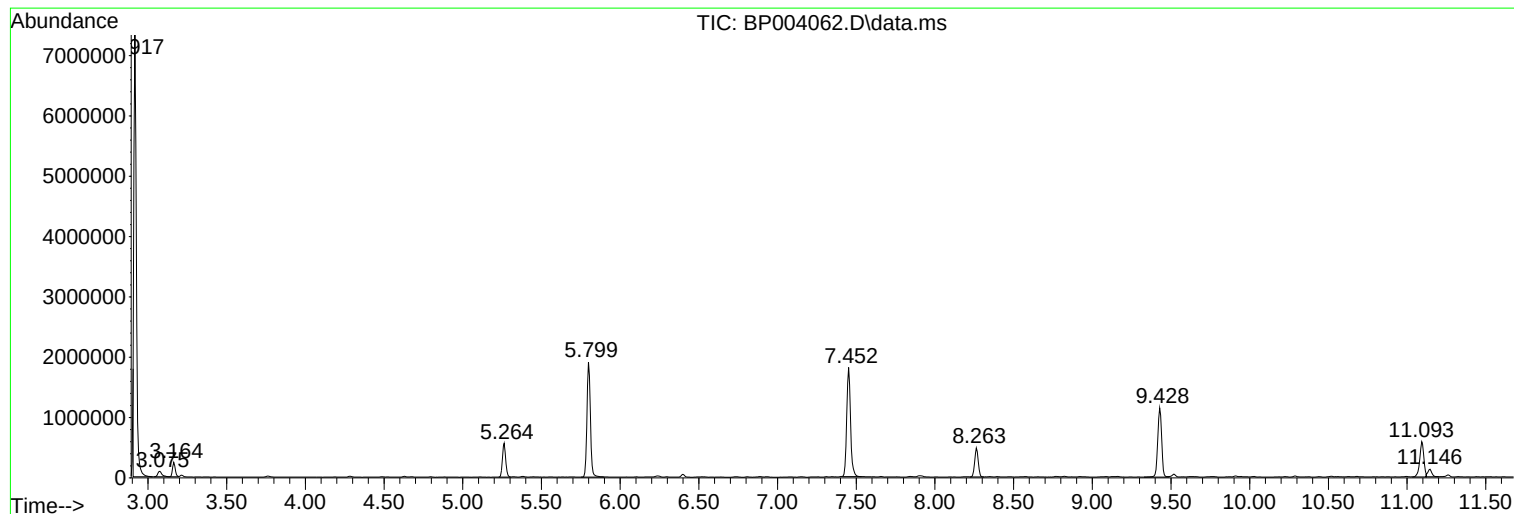

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004062.D
Acq On : 23 Nov 2020 19:04
Operator : CG/JU
Sample : L4857-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-EAST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004062.D
Acq On : 23 Nov 2020 19:04
Operator : CG/JU
Sample : L4857-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-EAST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
