

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004063.D
 Acq On : 23 Nov 2020 19:38
 Operator : CG/JU
 Sample : L4857-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 340EM-STOCKPILE-WEST

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.916	3	5	23	rVB	5666369	6281041	100.00%	14.457%
2	3.075	25	32	42	rVB	83127	164671	2.62%	0.379%
3	3.163	42	47	53	rBV	128381	161167	2.57%	0.371%
4	5.263	398	404	413	rBV	540727	776450	12.36%	1.787%
5	5.799	488	495	515	rBV	1750959	2676004	42.60%	6.159%
6	6.398	591	597	605	rVB	47575	71485	1.14%	0.165%
7	7.451	768	776	790	rBV	1728609	2890401	46.02%	6.653%
8	8.263	907	914	922	rBV	461538	732934	11.67%	1.687%
9	9.428	1103	1112	1122	rBV	1082211	1794669	28.57%	4.131%
10	11.092	1386	1395	1401	rBV	564224	994863	15.84%	2.290%
11	13.510	1799	1806	1821	rBV	2494506	3622476	57.67%	8.338%
12	14.310	1937	1942	1949	rBV	121095	184403	2.94%	0.424%
13	14.610	1988	1993	2000	rBV	44542	63469	1.01%	0.146%
14	14.886	2029	2040	2047	rBV	835921	1289651	20.53%	2.968%
15	16.374	2283	2293	2313	rBV	1715208	2653218	42.24%	6.107%
16	17.621	2499	2505	2509	rBV	1036825	1484722	23.64%	3.417%
17	17.663	2509	2512	2519	rVV	409234	544247	8.66%	1.253%
18	17.751	2523	2527	2532	rVB	82785	113376	1.81%	0.261%
19	18.468	2645	2649	2653	rBV	70156	99684	1.59%	0.229%
20	18.515	2653	2657	2664	rVB	93906	133283	2.12%	0.307%
21	18.663	2676	2682	2685	rBV2	87601	172984	2.75%	0.398%
22	18.933	2724	2728	2732	rBV	61914	85608	1.36%	0.197%
23	18.980	2732	2736	2745	rVB3	66410	105002	1.67%	0.242%
24	19.345	2793	2798	2802	rBV2	60728	103434	1.65%	0.238%
25	19.598	2835	2841	2846	rBV	1129828	1391612	22.16%	3.203%
26	19.915	2891	2895	2897	rBV2	135864	216946	3.45%	0.499%
27	19.945	2897	2900	2907	rVB	882244	1182870	18.83%	2.723%
28	20.010	2908	2911	2920	rVB2	47178	68357	1.09%	0.157%
29	20.121	2924	2930	2935	rBV	3836727	4600855	73.25%	10.590%
30	20.257	2949	2953	2959	rBV5	50223	106631	1.70%	0.245%
31	20.392	2972	2976	2977	rBV2	66771	80844	1.29%	0.186%
32	20.415	2978	2980	2985	rVB	120754	145372	2.31%	0.335%
33	20.515	2993	2997	3001	rBV	78749	99939	1.59%	0.230%
34	20.574	3004	3007	3011	rVB	63090	86338	1.37%	0.199%
35	20.751	3034	3037	3041	rVB2	153957	184523	2.94%	0.425%
36	21.139	3100	3103	3109	rVB	104720	140061	2.23%	0.322%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004063.D
 Acq On : 23 Nov 2020 19:38
 Operator : CG/JU
 Sample : L4857-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 340EM-STOCKPILE-WEST

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.309	3128	3132	3135	rBV2	252465	349571	5.57%	0.805%
38	21.386	3141	3145	3148	rVV2	105739	141938	2.26%	0.327%
39	21.427	3149	3152	3158	rVB2	111968	154940	2.47%	0.357%
40	21.656	3184	3191	3195	rBV2	1201579	2260202	35.98%	5.202%
41	21.692	3195	3197	3202	rVB	467884	539271	8.59%	1.241%
42	21.827	3217	3220	3224	rBV	74688	90128	1.43%	0.207%
43	22.209	3283	3285	3288	rBV	76199	88067	1.40%	0.203%
44	23.268	3461	3465	3471	rVB2	182770	272082	4.33%	0.626%
45	23.374	3478	3483	3496	rVB	454554	1418011	22.58%	3.264%
46	23.909	3571	3574	3584	rVB	298256	581582	9.26%	1.339%
47	24.015	3587	3592	3600	rVB	344986	651906	10.38%	1.501%
48	24.127	3605	3611	3617	rBV	693317	1394512	22.20%	3.210%




Sum of corrected areas: 43445800

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004063.D
Acq On : 23 Nov 2020 19:38
Operator : CG/JU
Sample : L4857-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-WEST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

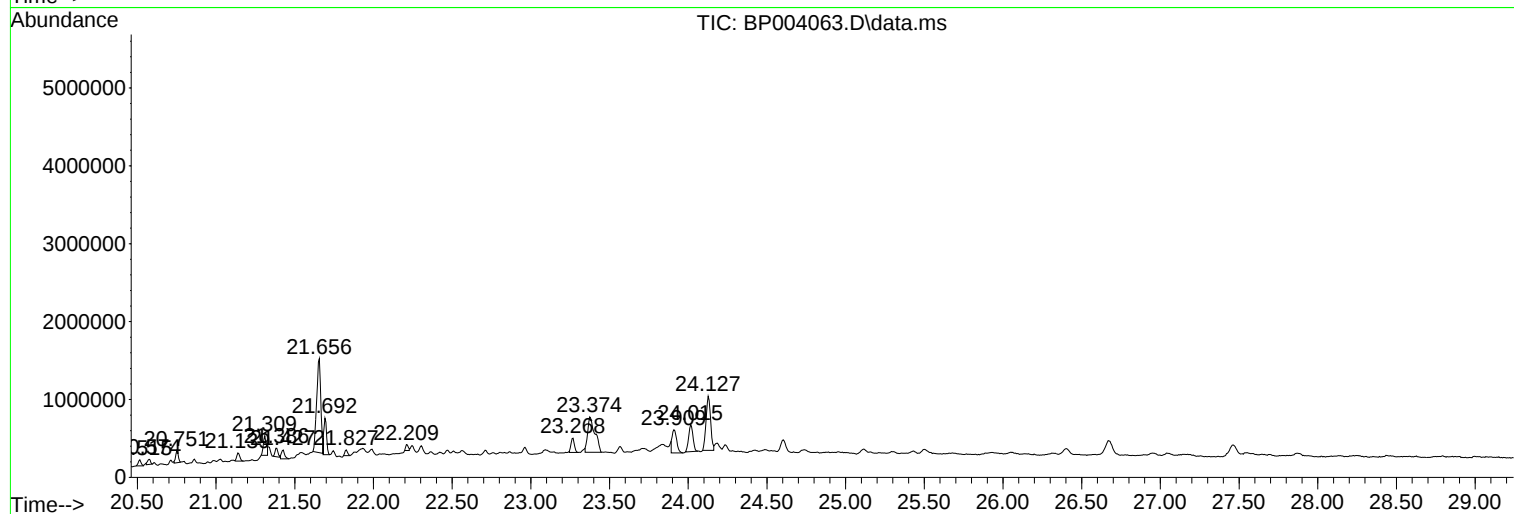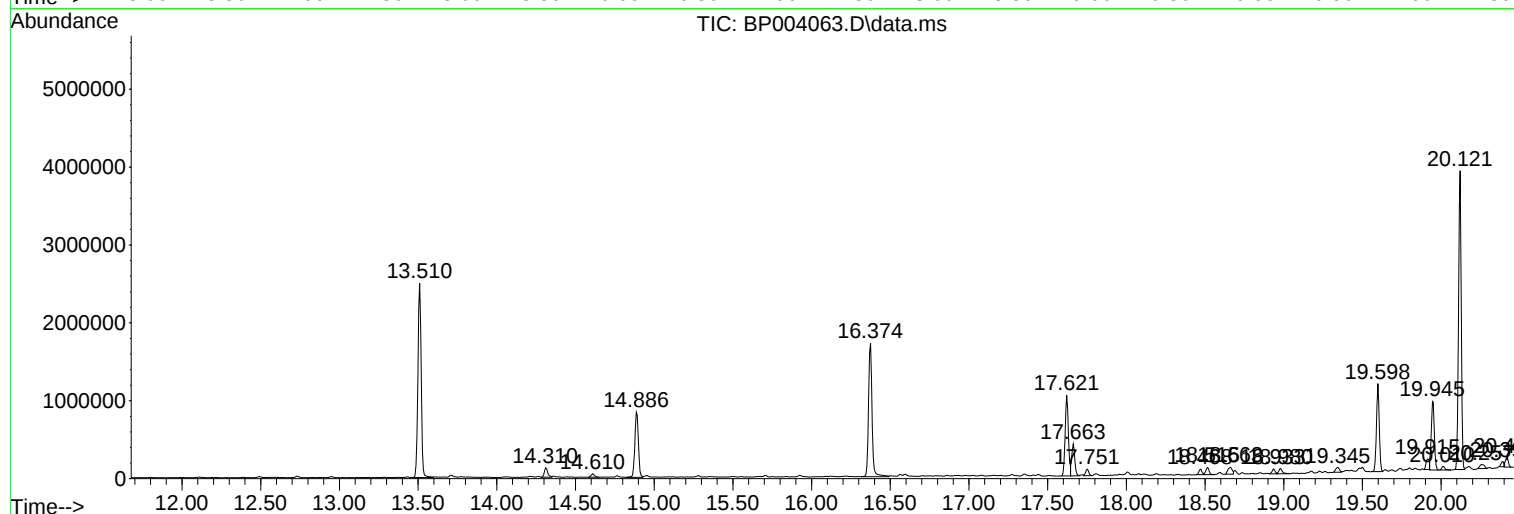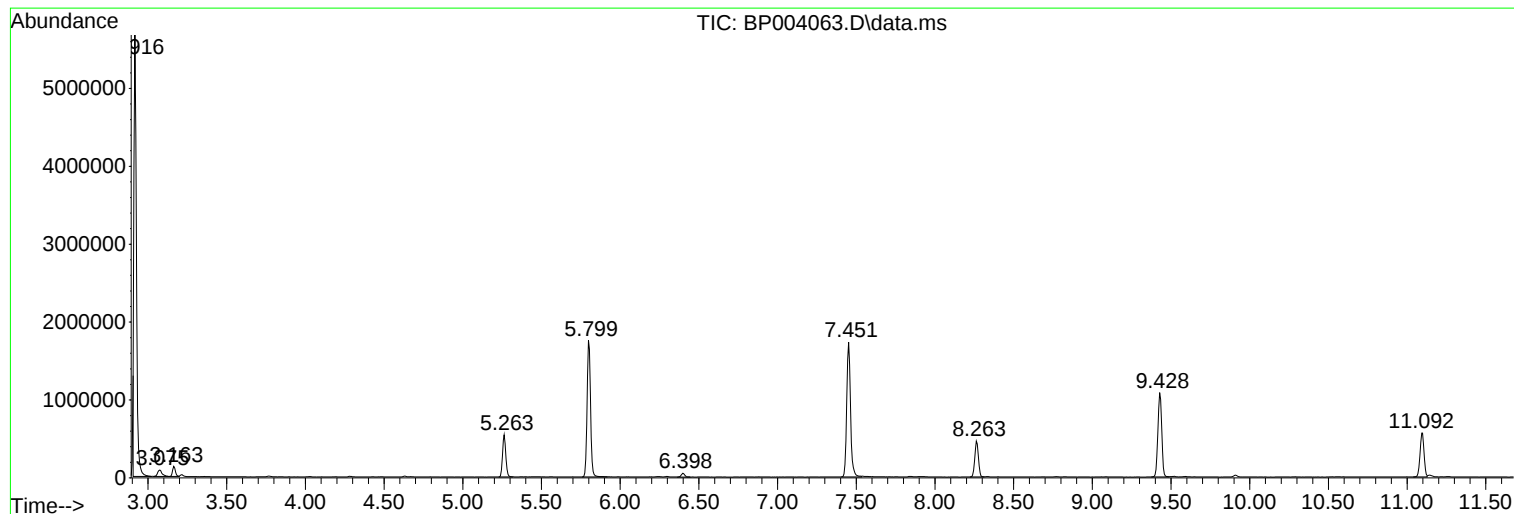

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004063.D
Acq On : 23 Nov 2020 19:38
Operator : CG/JU
Sample : L4857-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-WEST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004063.D
Acq On : 23 Nov 2020 19:38
Operator : CG/JU
Sample : L4857-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
340EM-STOCKPILE-WEST

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
