

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004064.D
 Acq On : 23 Nov 2020 20:12
 Operator : CG/JU
 Sample : L4857-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 304EM-STOCKPILE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004064.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.916	3	5	22	rVB	2504950	3043584	89.05%	8.079%
2	3.075	26	32	42	rVV2	57802	122112	3.57%	0.324%
3	3.163	42	47	53	rVV	143017	203574	5.96%	0.540%
4	4.875	331	338	346	rVB	56289	90039	2.63%	0.239%
5	5.263	398	404	413	rBV	466077	665297	19.46%	1.766%
6	5.805	489	496	514	rBV	1359255	2176087	63.67%	5.776%
7	6.399	591	597	604	rVB	38171	56279	1.65%	0.149%
8	7.451	769	776	789	rBV	1324054	2249646	65.82%	5.971%
9	8.263	904	914	923	rBV	433141	695526	20.35%	1.846%
10	9.428	1102	1112	1124	rBV	870615	1436487	42.03%	3.813%
11	11.092	1386	1395	1402	rBV	541997	939928	27.50%	2.495%
12	12.745	1668	1676	1685	rBV2	51059	113636	3.32%	0.302%
13	13.351	1772	1779	1789	rBV2	42171	99526	2.91%	0.264%
14	13.510	1799	1806	1818	rBV	1944429	2831233	82.84%	7.515%
15	13.710	1836	1840	1848	rVB3	17922	35528	1.04%	0.094%
16	14.310	1937	1942	1962	rVB	127628	248928	7.28%	0.661%
17	14.610	1987	1993	2000	rBV	108253	160398	4.69%	0.426%
18	14.886	2034	2040	2048	rBV	803064	1209422	35.38%	3.210%
19	16.310	2277	2282	2287	rBV	112509	171314	5.01%	0.455%
20	16.375	2287	2293	2307	rVB	1241037	1887744	55.23%	5.011%
21	16.792	2360	2364	2371	rBV	118374	150498	4.40%	0.399%
22	17.622	2499	2505	2510	rBV	961035	1517318	44.39%	4.027%
23	17.663	2510	2512	2520	rVV2	245236	389741	11.40%	1.034%
24	17.751	2523	2527	2532	rVB	92577	123498	3.61%	0.328%
25	17.816	2534	2538	2545	rVB6	30390	49511	1.45%	0.131%
26	17.957	2558	2562	2565	rBV2	56305	64416	1.88%	0.171%
27	18.010	2567	2571	2576	rVB	31144	41969	1.23%	0.111%
28	18.469	2645	2649	2653	rBV2	83432	133694	3.91%	0.355%
29	18.516	2654	2657	2662	rVB2	79546	104021	3.04%	0.276%
30	18.592	2667	2670	2674	rVB	30576	38888	1.14%	0.103%
31	18.645	2675	2679	2685	rBV3	94144	200353	5.86%	0.532%
32	18.739	2691	2695	2702	rBV6	25837	59922	1.75%	0.159%
33	18.939	2726	2729	2732	rVB3	32777	36603	1.07%	0.097%
34	18.980	2732	2736	2741	rVB3	49900	72820	2.13%	0.193%
35	19.339	2793	2797	2802	rBV3	65095	109487	3.20%	0.291%
36	19.410	2807	2809	2817	rVB4	66621	89638	2.62%	0.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
 Data File : BP004064.D
 Acq On : 23 Nov 2020 20:12
 Operator : CG/JU
 Sample : L4857-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 304EM-STOCKPILE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.598	2836	2841	2846	rBV	746881	1027528	30.06%	2.727%
38	19.739	2862	2865	2869	rBV	66968	89783	2.63%	0.238%
39	19.798	2873	2875	2878	rVB2	44259	43709	1.28%	0.116%
40	19.916	2891	2895	2896	rBV	78883	101503	2.97%	0.269%
41	19.945	2896	2900	2908	rVB	655604	948491	27.75%	2.518%
42	20.121	2924	2930	2935	rBV	2755518	3417917	100.00%	9.072%
43	20.386	2970	2975	2978	rBV3	182267	304860	8.92%	0.809%
44	20.715	3028	3031	3034	rBV	105459	126775	3.71%	0.337%
45	20.751	3034	3037	3043	rVB	124065	154299	4.51%	0.410%
46	20.863	3053	3056	3065	rVB2	116341	173229	5.07%	0.460%
47	21.310	3128	3132	3141	rBV3	640191	992294	29.03%	2.634%
48	21.380	3141	3144	3148	rVB3	163070	181703	5.32%	0.482%
49	21.657	3184	3191	3195	rBV2	1160764	2022426	59.17%	5.368%
50	21.692	3195	3197	3202	rVB	349855	407597	11.93%	1.082%
51	22.210	3282	3285	3288	rBV	330466	447489	13.09%	1.188%
52	22.245	3288	3291	3298	rVB2	308214	580873	16.99%	1.542%
53	23.268	3461	3465	3470	rVB	425310	630201	18.44%	1.673%
54	23.333	3473	3476	3479	rBV2	174907	288318	8.44%	0.765%
55	24.021	3589	3593	3598	rVB	256574	406082	11.88%	1.078%
56	24.127	3606	3611	3618	rBV	629986	1222772	35.78%	3.246%
57	24.609	3689	3693	3700	rVB	278854	535992	15.68%	1.423%
58	24.821	3725	3729	3736	rVB	271464	530300	15.52%	1.408%
59	27.774	4224	4231	4241	rVB3	466872	1421760	41.60%	3.774%




Sum of corrected areas: 37674566

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004064.D
Acq On : 23 Nov 2020 20:12
Operator : CG/JU
Sample : L4857-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

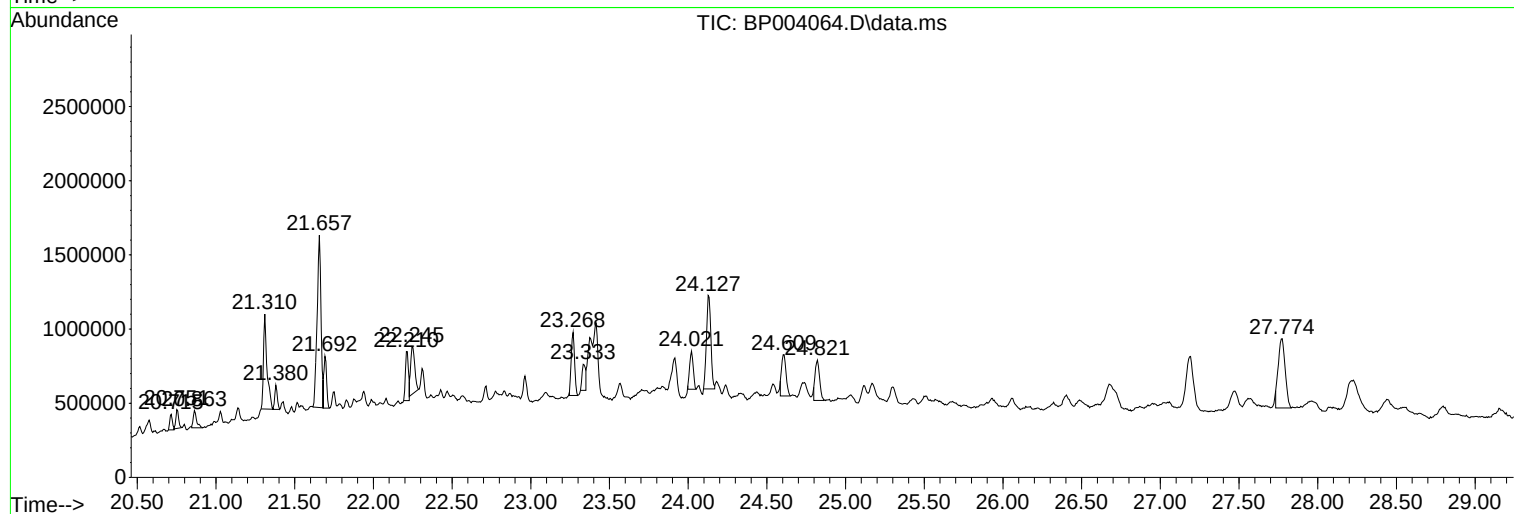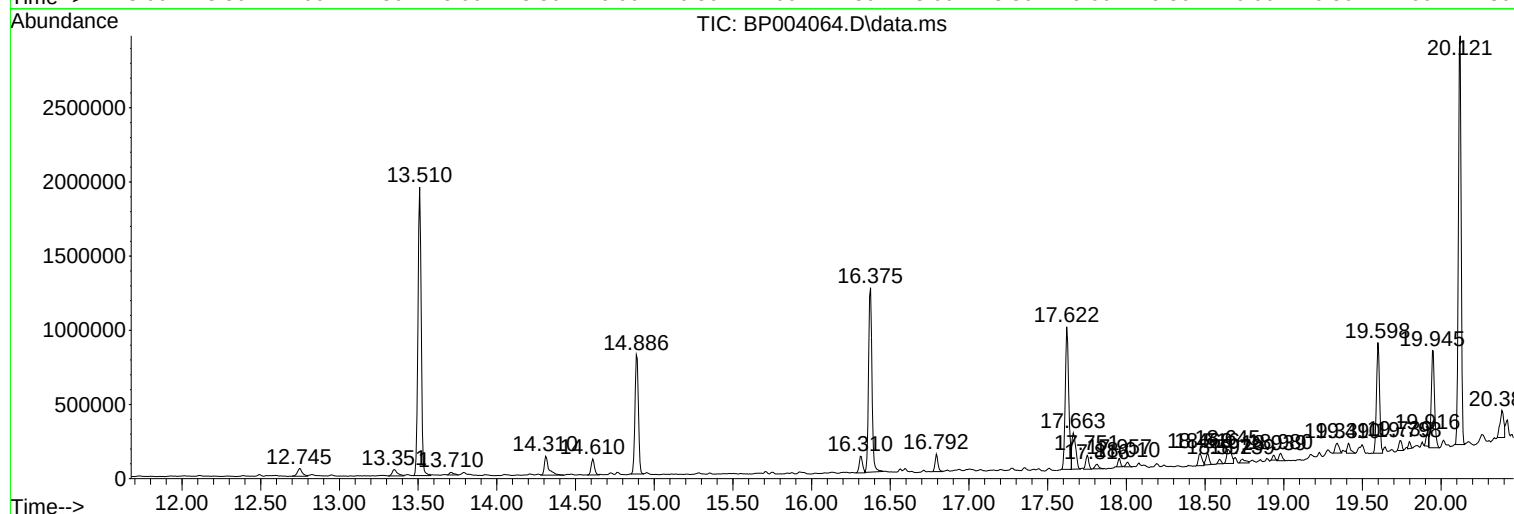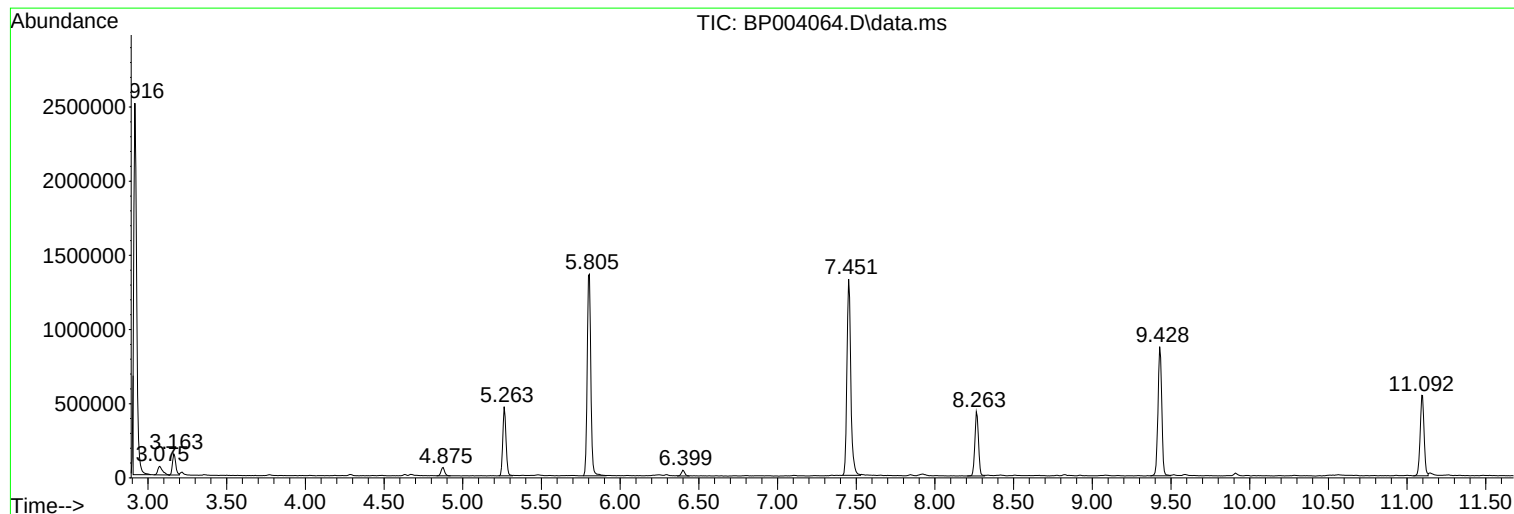

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004064.D
Acq On : 23 Nov 2020 20:12
Operator : CG/JU
Sample : L4857-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112320\
Data File : BP004064.D
Acq On : 23 Nov 2020 20:12
Operator : CG/JU
Sample : L4857-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
304EM-STOCKPILE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------