
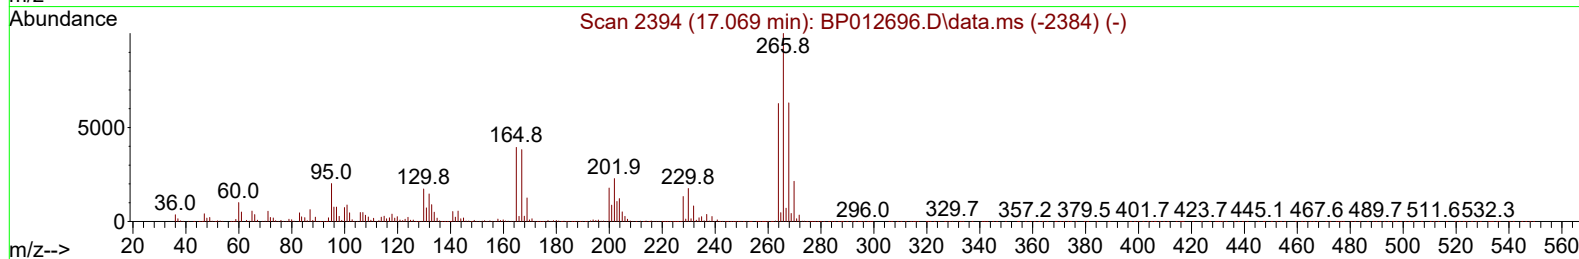
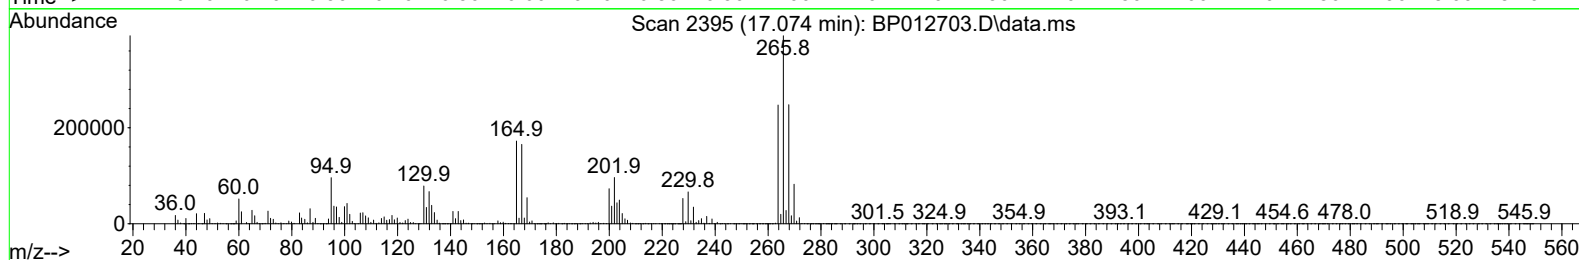


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112322\
 Data File : BP012703.D
 Acq On : 23 Nov 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 05:29:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 00:38:14 2022
 Response via : Initial Calibration

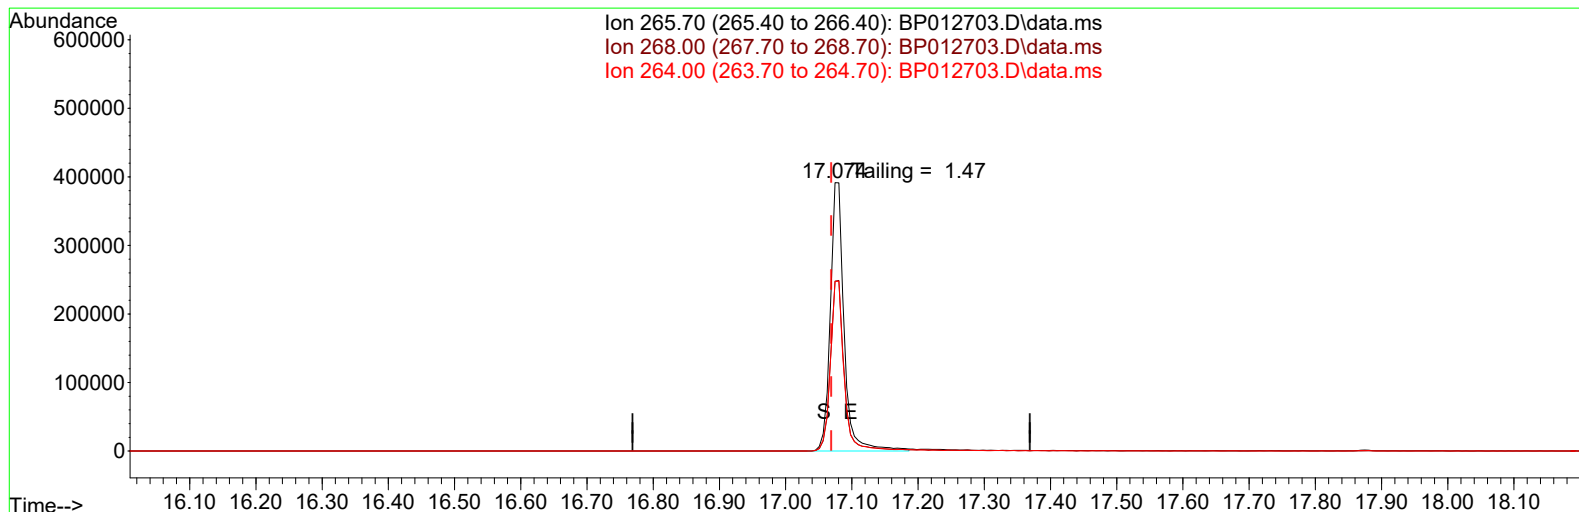

TIC: BP012703.D\data.ms

(70) Pentachlorophenol (C)




17.074min (+ 0.005) 363805.26 ng

response 571624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.31
264.00	62.70	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112322\
Data File : BP012703.D
Acq On : 23 Nov 2022 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 05:29:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 00:38:14 2022
Response via : Initial Calibration

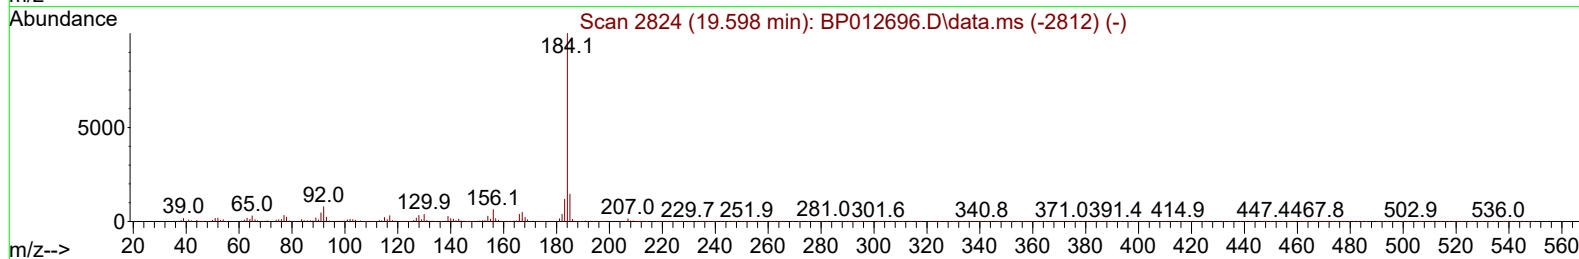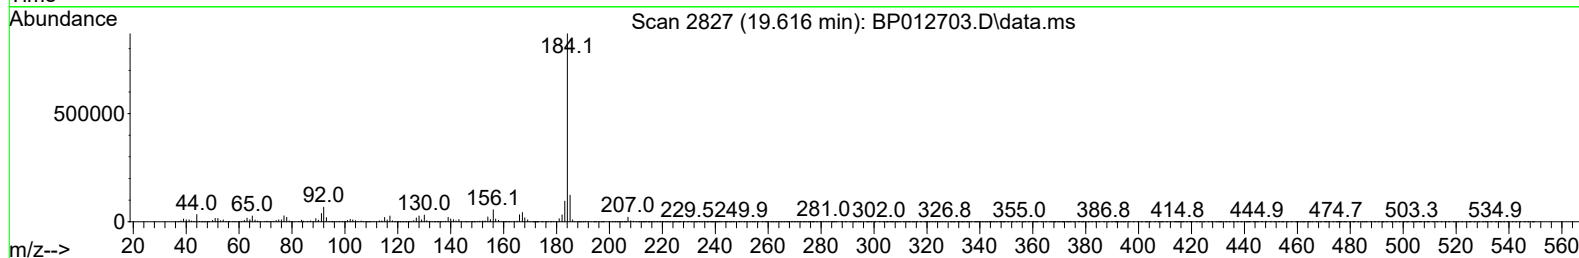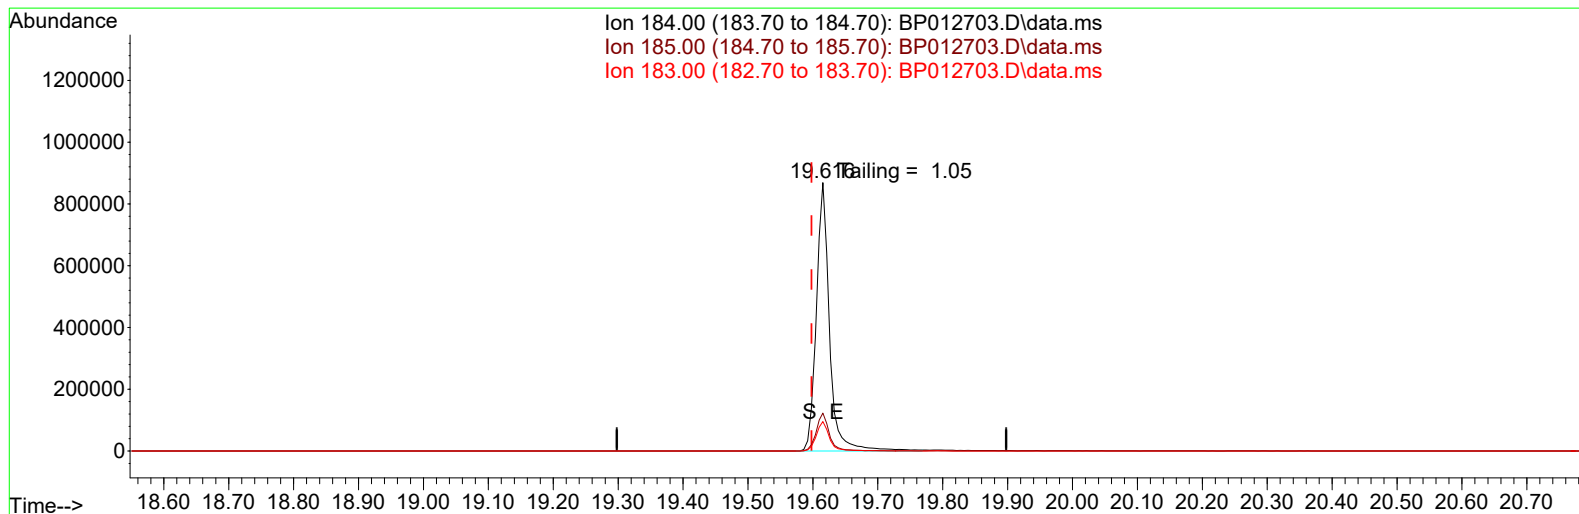

TIC: BP012703.D\data.ms

(77) Benzidine

19.616min (+ 0.018) 25957.68 ng

response 1230377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.12
183.00	11.80	11.01
0.00	0.00	0.00