
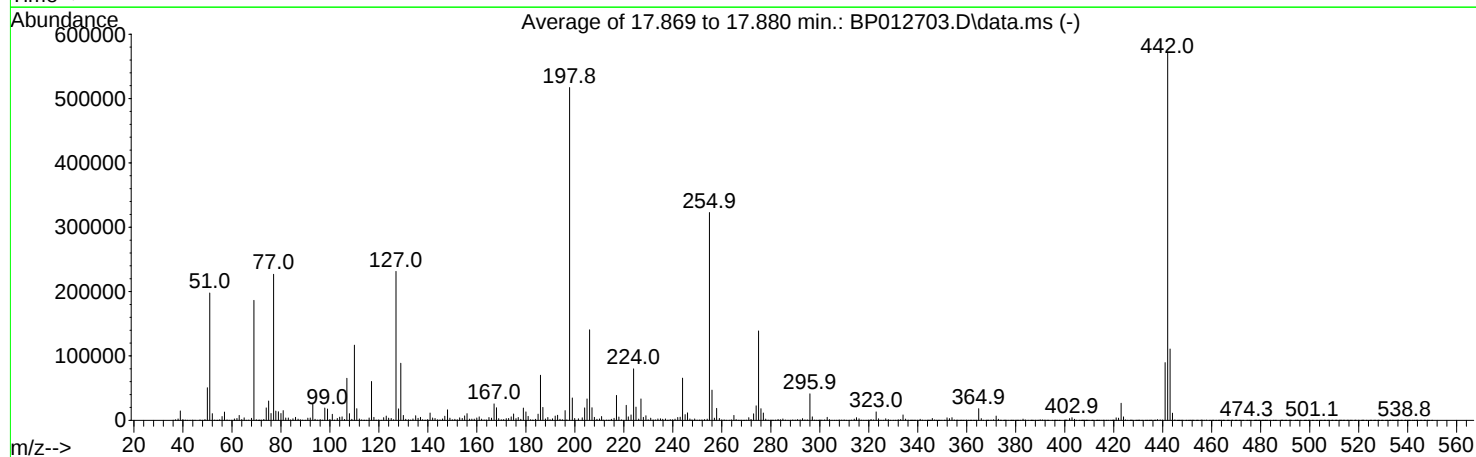


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112322\
 Data File : BP012703.D
 Acq On : 23 Nov 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 23 00:38:14 2022

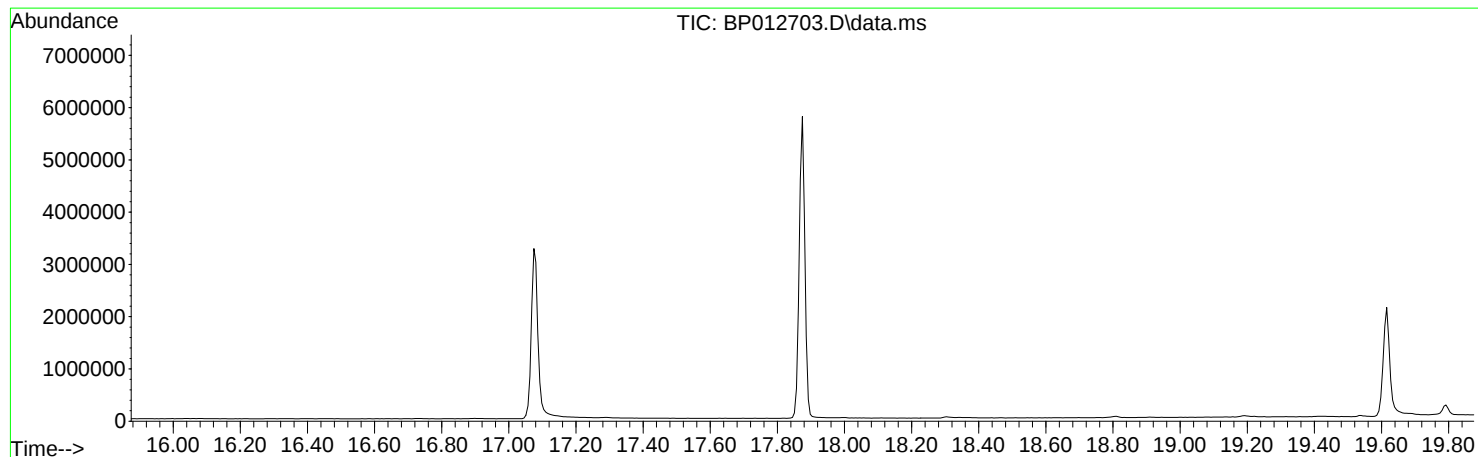




AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	197921	PASS
68	69	0.00	2	1.7	3150	PASS
69	198	0.00	100	36.1	186489	PASS
70	69	0.00	2	0.5	945	PASS
127	198	10	80	44.8	231424	PASS
197	198	0.00	2	0.1	542	PASS
198	198	100	100	100.0	517096	PASS
199	198	5	9	6.7	34840	PASS
275	198	10	60	26.8	138808	PASS
365	198	1	100	3.5	18057	PASS
441	198	0.01	100	17.3	89584	PASS
442	442	100	100	100.0	571726	PASS
443	442	15	24	19.4	110803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112322\
 Data File : BP012703.D
 Acq On : 23 Nov 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 05:29:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 00:38:14 2022
 Response via : Initial Calibration

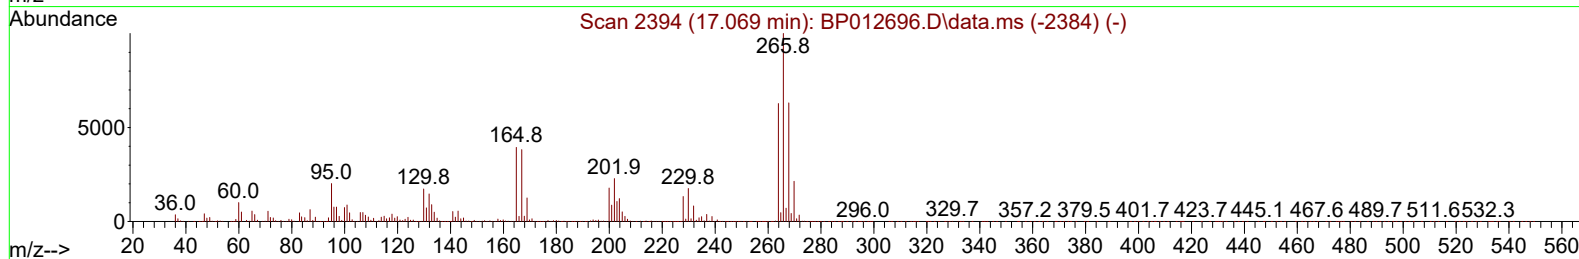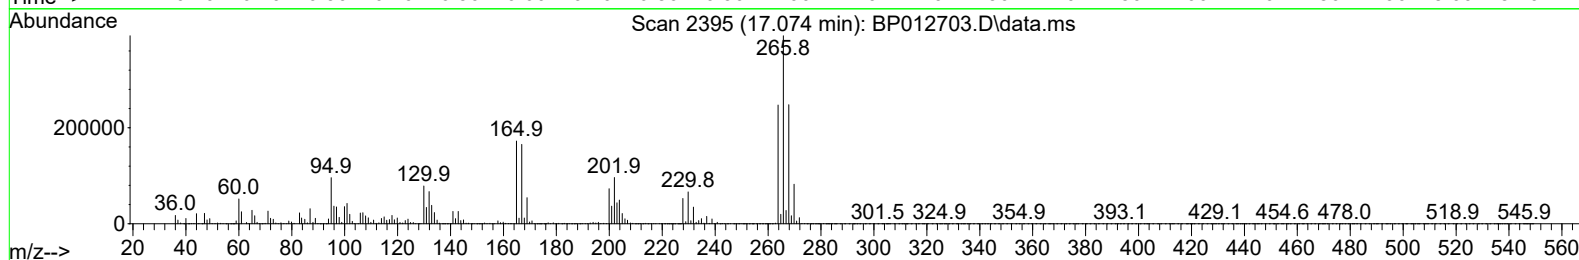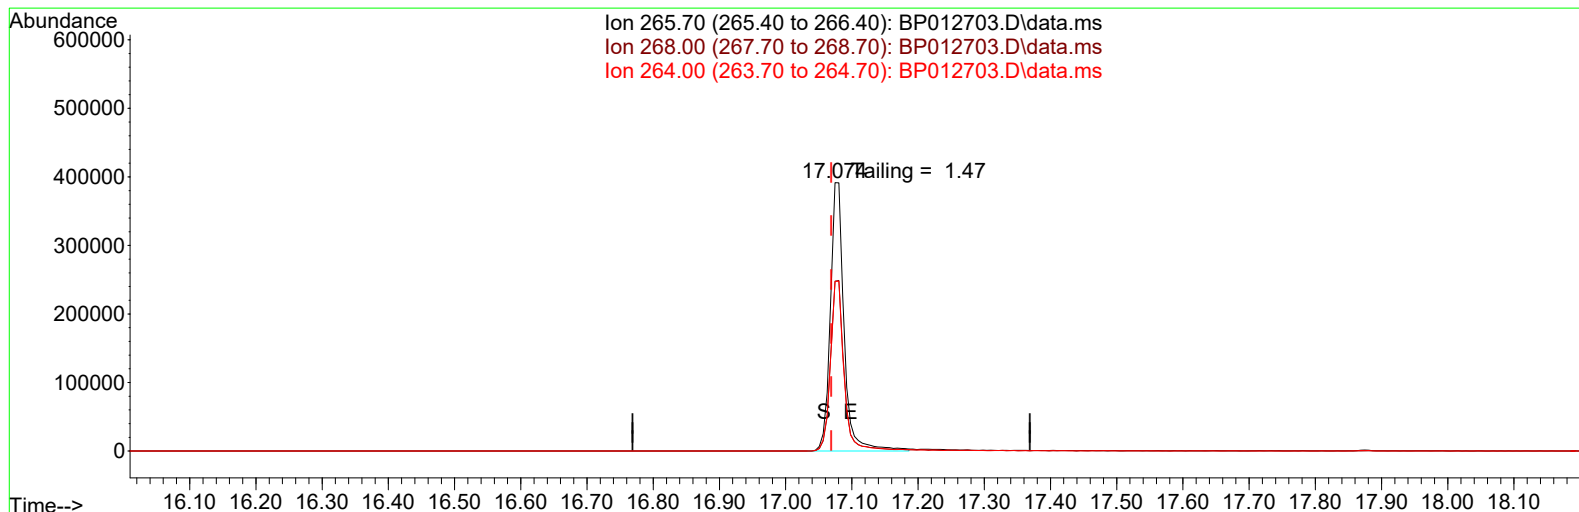

TIC: BP012703.D\data.ms

(70) Pentachlorophenol (C)

17.074min (+ 0.005) 363805.26 ng




response 571624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.31
264.00	62.70	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112322\
 Data File : BP012703.D
 Acq On : 23 Nov 2022 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 05:29:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 23 00:38:14 2022
 Response via : Initial Calibration

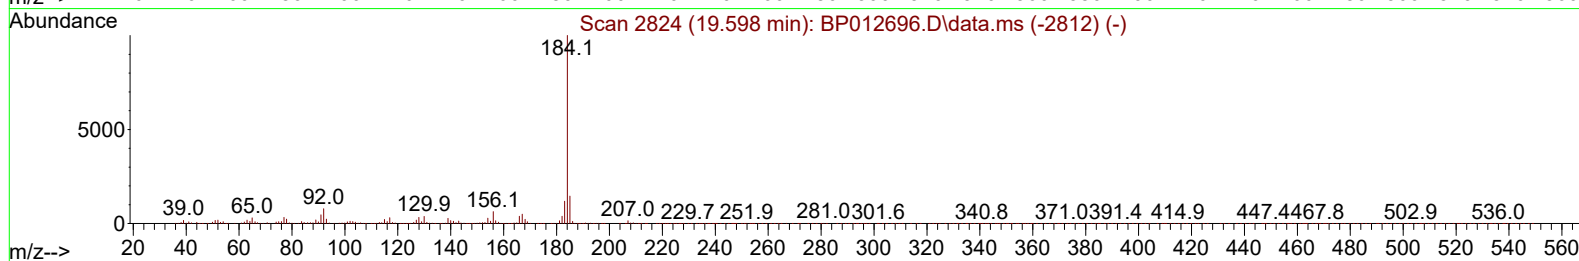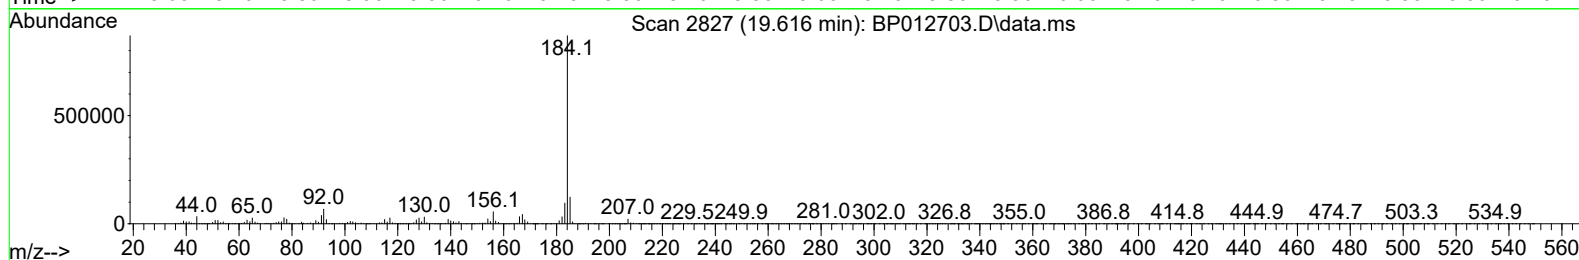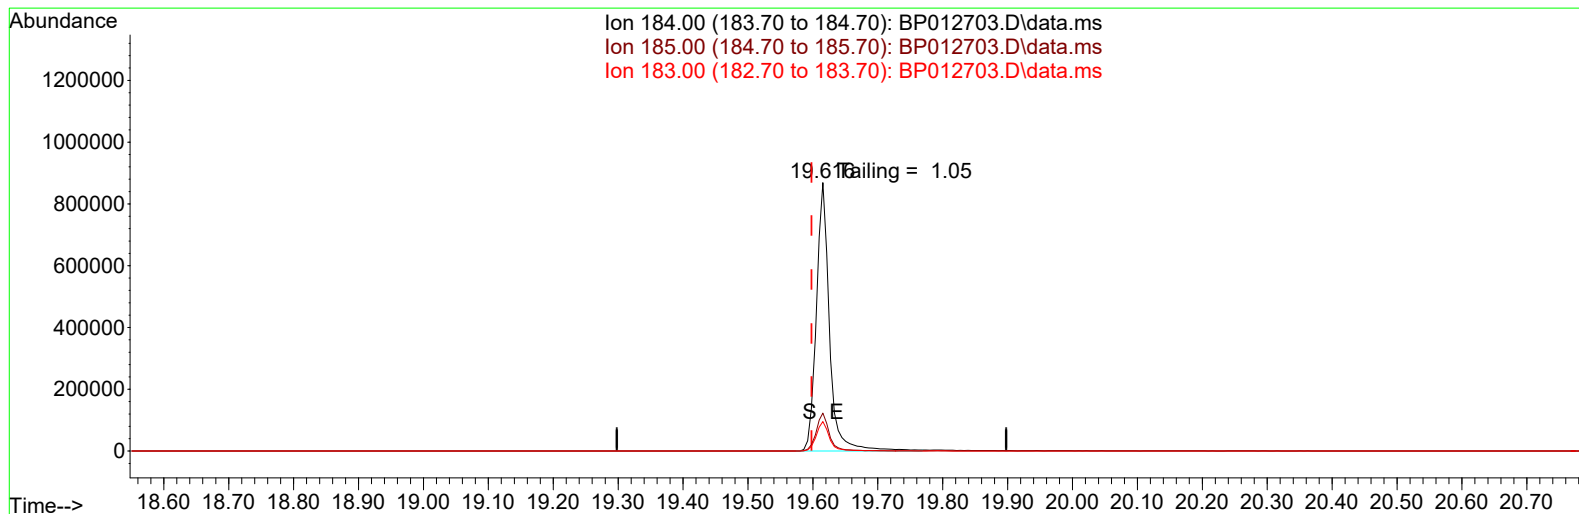

TIC: BP012703.D\data.ms

(77) Benzidine

19.616min (+ 0.018) 25957.68 ng

response 1230377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.12
183.00	11.80	11.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2022	BNA_P	<u>BP012703.D</u>
Compound Name	Response	Retention Time
DDT	1227513	20.821
DDD	12409	20.439
DDE	864	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13273	1240786	1.07

Instrument :
BNA_P
ClientSampleId :
DFTPP